

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
 Data File : VV038265.D
 Acq On : 22 Nov 2024 12:32
 Operator : SY/MD
 Sample : VIBLK403
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK403

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038265.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	87	rBV	84235	91845	12.73%	1.528%
2	1.529	145	152	166	rVB	87088	103999	14.42%	1.730%
3	2.053	306	315	331	rVB	143919	211825	29.36%	3.524%
4	3.789	842	855	889	rBV2	103046	345770	47.93%	5.753%
5	4.243	980	996	1022	rBV2	123104	330069	45.76%	5.492%
6	4.950	1202	1216	1248	rBV2	234564	631983	87.61%	10.515%
7	5.529	1386	1396	1434	rBV	236164	531116	73.63%	8.837%
8	5.844	1480	1494	1508	rBV10	4519	11706	1.62%	0.195%
9	5.982	1524	1537	1571	rBV	151887	338674	46.95%	5.635%
10	6.915	1818	1827	1856	rBV	56325	126977	17.60%	2.113%
11	7.239	1917	1928	1955	rBV	212577	413156	57.28%	6.874%
12	7.561	2019	2028	2051	rBV3	31417	72793	10.09%	1.211%
13	7.866	2112	2123	2132	rBV4	5479	10292	1.43%	0.171%
14	8.021	2162	2171	2210	rBV	313049	696119	96.50%	11.582%
15	8.362	2266	2277	2290	rBV3	11828	23604	3.27%	0.393%
16	8.780	2397	2407	2443	rBV	406589	721354	100.00%	12.002%
17	10.146	2820	2832	2853	rBV	154053	259695	36.00%	4.321%
18	10.320	2872	2886	2900	rVB3	10777	17503	2.43%	0.291%
19	11.178	3143	3153	3179	rBV	348106	589410	81.71%	9.806%
20	11.554	3255	3270	3297	rBV	282451	482525	66.89%	8.028%




Sum of corrected areas: 6010415

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038265.D
Acq On : 22 Nov 2024 12:32
Operator : SY/MD
Sample : VIBLK403
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK403

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

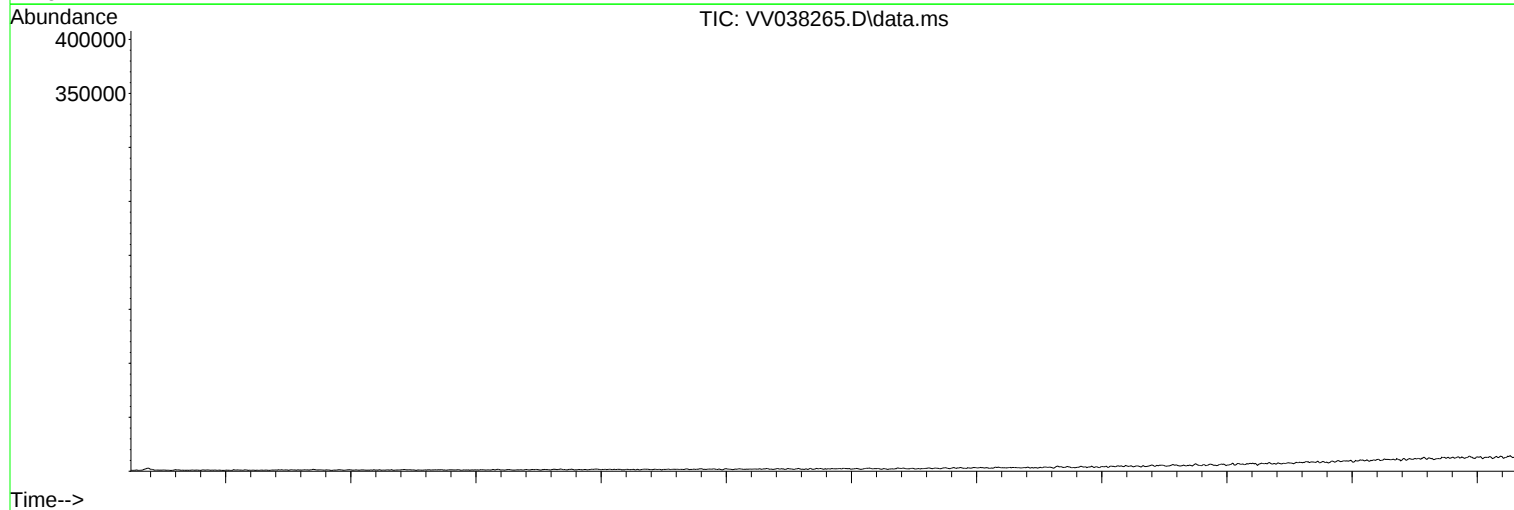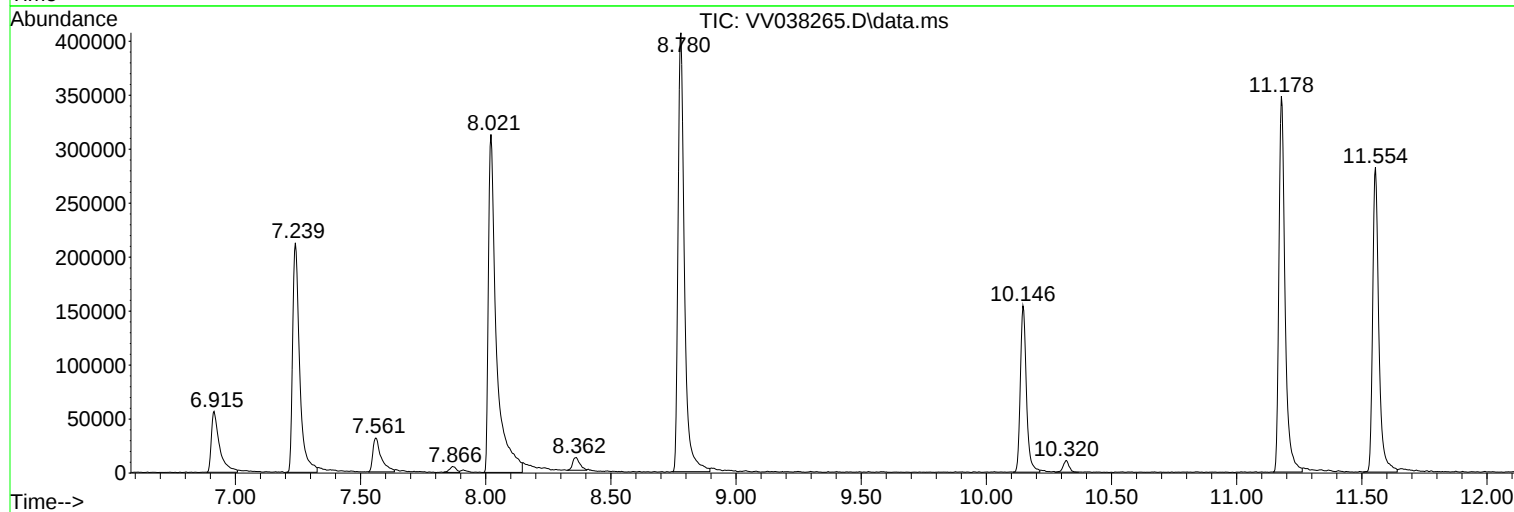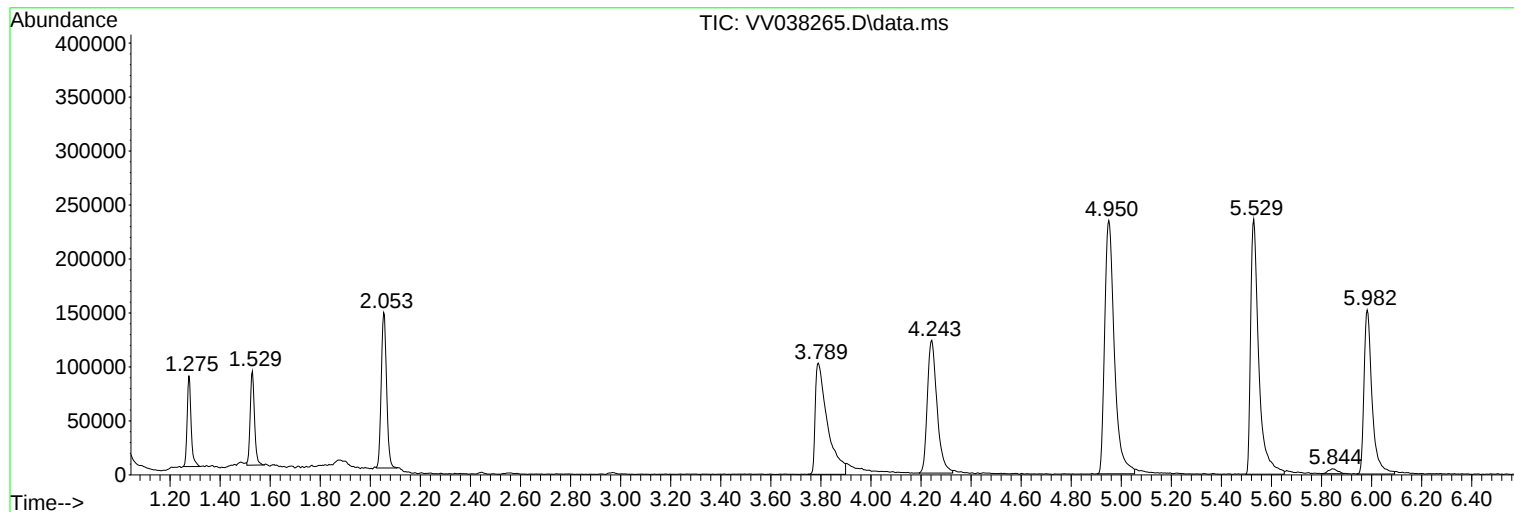

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038265.D
Acq On : 22 Nov 2024 12:32
Operator : SY/MD
Sample : VIBLK403
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK403

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038265.D
Acq On : 22 Nov 2024 12:32
Operator : SY/MD
Sample : VIBLK403
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK403

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc