

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
 Data File : VV038266.D
 Acq On : 22 Nov 2024 13:30
 Operator : SY/MD
 Sample : P4882-20
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038266.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	86	rBV	116286	125966	16.55%	1.963%
2	1.529	145	152	163	rVB	110585	127547	16.76%	1.988%
3	2.053	304	315	331	rBV	203456	296691	38.98%	4.623%
4	3.789	842	855	892	rBV2	86372	296246	38.92%	4.616%
5	4.236	979	994	1020	rBV2	141175	371226	48.77%	5.785%
6	4.947	1201	1215	1251	rBV2	284525	761149	100.00%	11.861%
7	5.526	1385	1395	1422	rBV	242314	535722	70.38%	8.348%
8	5.838	1483	1492	1506	rBV10	3844	9079	1.19%	0.141%
9	5.979	1523	1536	1558	rBV2	172696	376646	49.48%	5.869%
10	6.911	1811	1826	1851	rBV	64451	146987	19.31%	2.291%
11	7.236	1915	1927	1962	rBV	290932	554492	72.85%	8.641%
12	7.554	2016	2026	2055	rBV2	37278	86901	11.42%	1.354%
13	8.021	2162	2171	2210	rBV	263542	609383	80.06%	9.496%
14	8.358	2267	2276	2289	rBV4	8072	16103	2.12%	0.251%
15	8.776	2396	2406	2433	rBV	409483	720869	94.71%	11.233%
16	10.146	2820	2832	2856	rBV	140287	238364	31.32%	3.714%
17	10.320	2875	2886	2898	rVB4	5719	10939	1.44%	0.170%
18	11.178	3143	3153	3190	rBV	352100	611963	80.40%	9.536%
19	11.554	3256	3270	3294	rBV	299249	520948	68.44%	8.118%

Sum of corrected areas: 6417221




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038266.D
Acq On : 22 Nov 2024 13:30
Operator : SY/MD
Sample : P4882-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

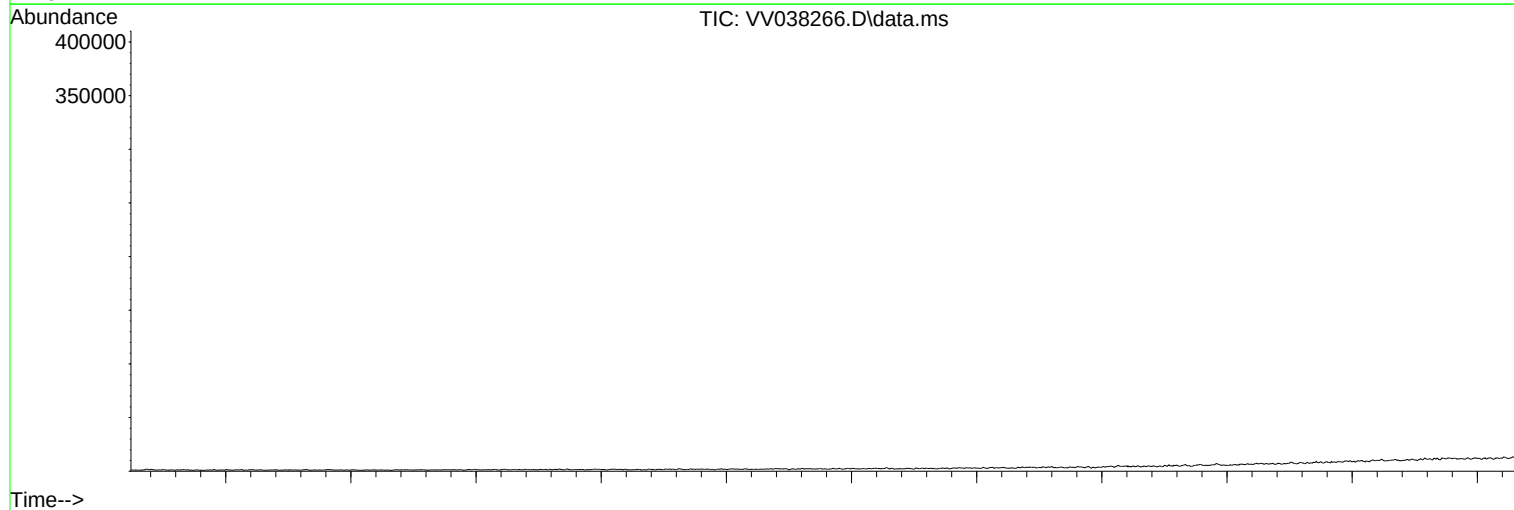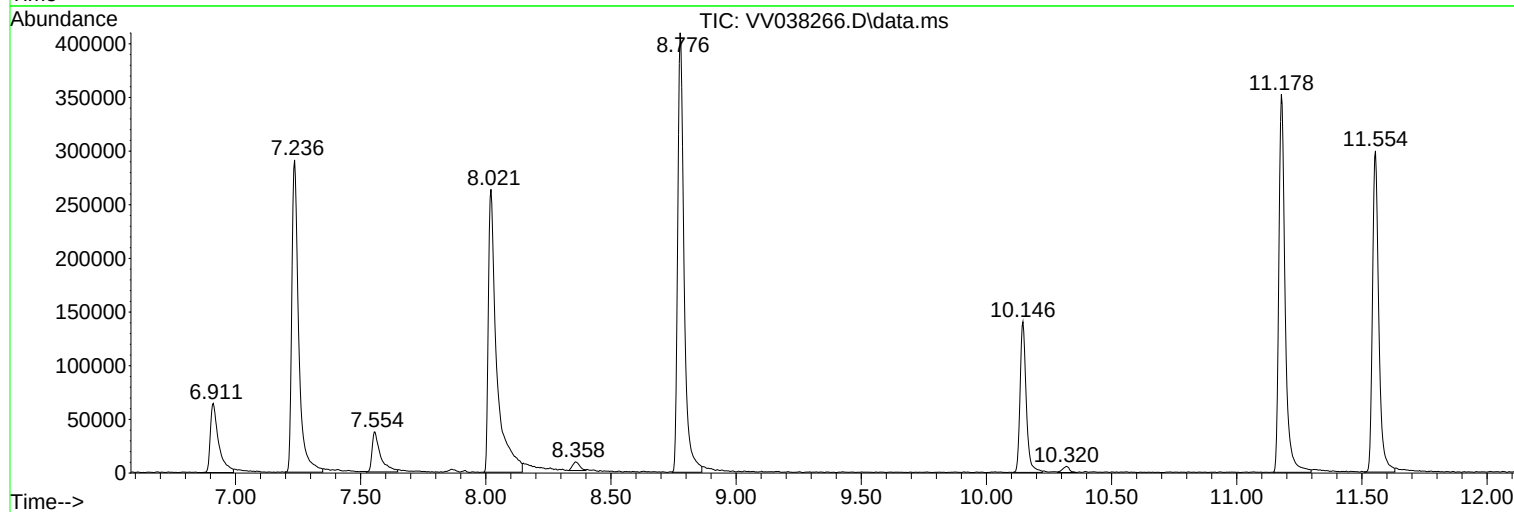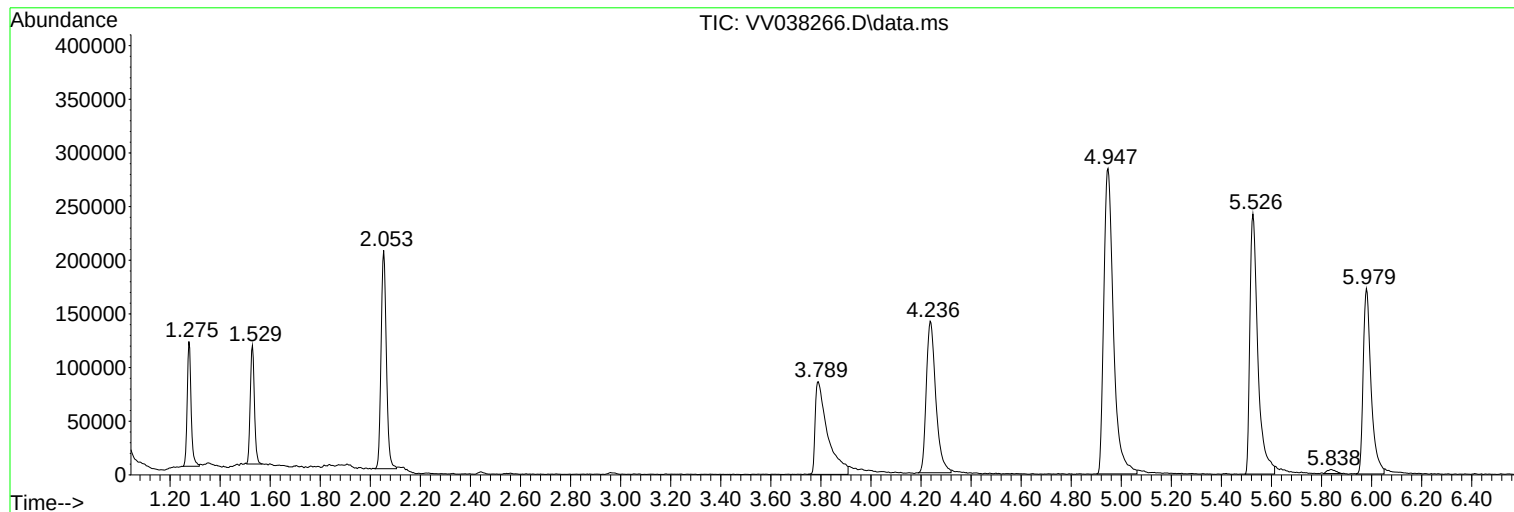

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038266.D
Acq On : 22 Nov 2024 13:30
Operator : SY/MD
Sample : P4882-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038266.D
Acq On : 22 Nov 2024 13:30
Operator : SY/MD
Sample : P4882-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc