

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
 Data File : VV038282.D
 Acq On : 22 Nov 2024 21:07
 Operator : SY/MD
 Sample : VV1122WBL02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK261

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038282.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	65	73	84	rBV	114916	123419	15.61%	1.813%
2	1.529	145	152	166	rVB	110434	129017	16.32%	1.895%
3	2.053	305	315	334	rVB	194770	286523	36.24%	4.208%
4	3.793	845	856	897	rBV2	101116	348246	44.04%	5.115%
5	4.243	979	996	1022	rBV2	137397	373630	47.25%	5.488%
6	4.950	1200	1216	1247	rBV2	299060	790694	100.00%	11.613%
7	5.529	1386	1396	1425	rBV	252892	555570	70.26%	8.160%
8	5.841	1482	1493	1502	rBV8	4813	10436	1.32%	0.153%
9	5.982	1526	1537	1566	rBV2	178114	389444	49.25%	5.720%
10	6.915	1817	1827	1851	rBV2	67254	148891	18.83%	2.187%
11	7.240	1918	1928	1956	rBV	296211	574311	72.63%	8.435%
12	7.558	2018	2027	2046	rBV2	35984	83694	10.58%	1.229%
13	7.905	2126	2135	2154	rVB3	20014	38251	4.84%	0.562%
14	8.021	2163	2171	2215	rBV	328280	745827	94.33%	10.954%
15	8.362	2269	2277	2287	rBV4	6759	12216	1.54%	0.179%
16	8.780	2395	2407	2431	rBV	419316	747509	94.54%	10.979%
17	10.146	2821	2832	2851	rBV	158870	265828	33.62%	3.904%
18	11.178	3141	3153	3177	rBV	374232	630613	79.75%	9.262%
19	11.554	3258	3270	3299	rBV	321166	554571	70.14%	8.145%




Sum of corrected areas: 6808690

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038282.D
Acq On : 22 Nov 2024 21:07
Operator : SY/MD
Sample : VV1122WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK261

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

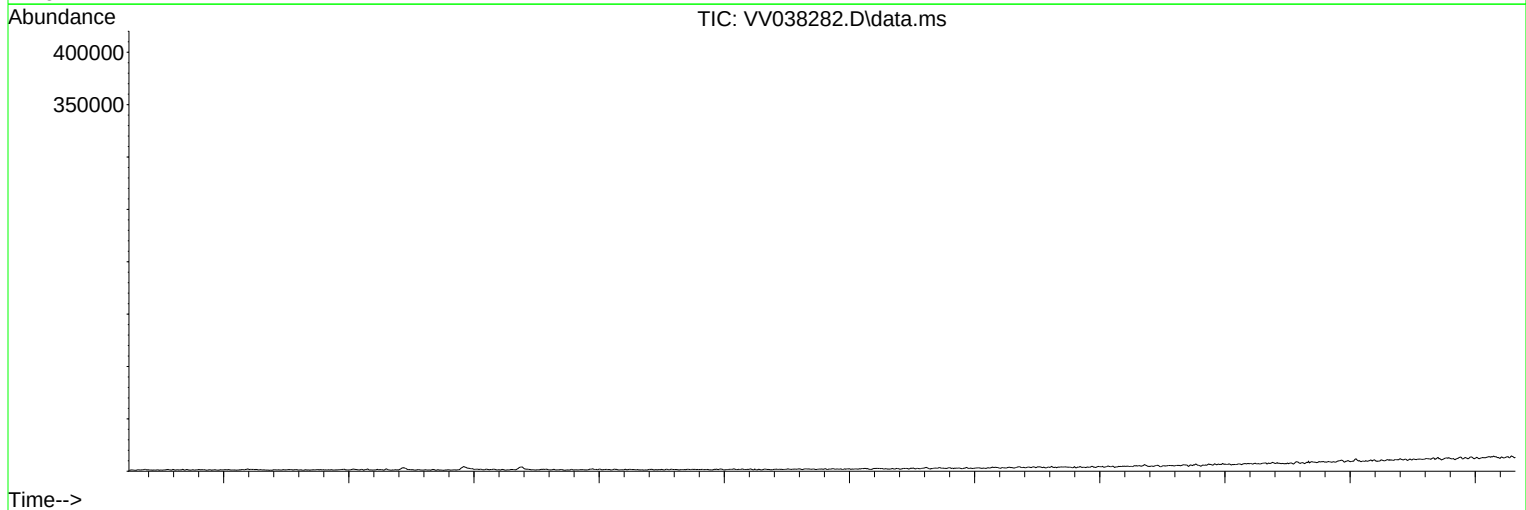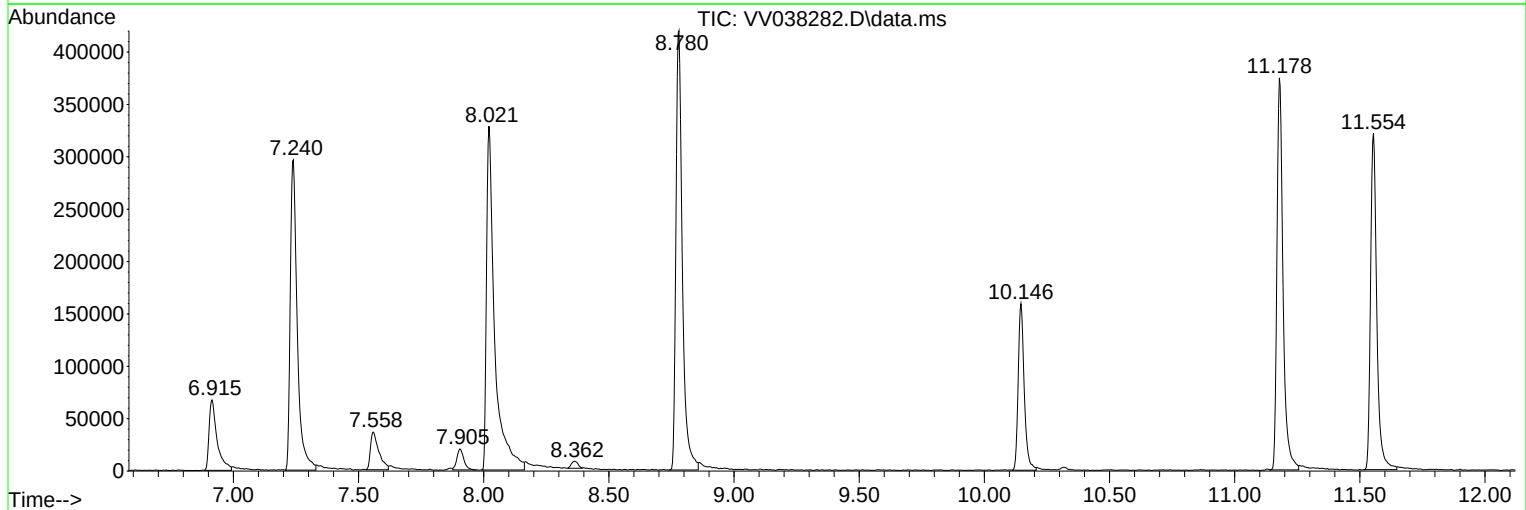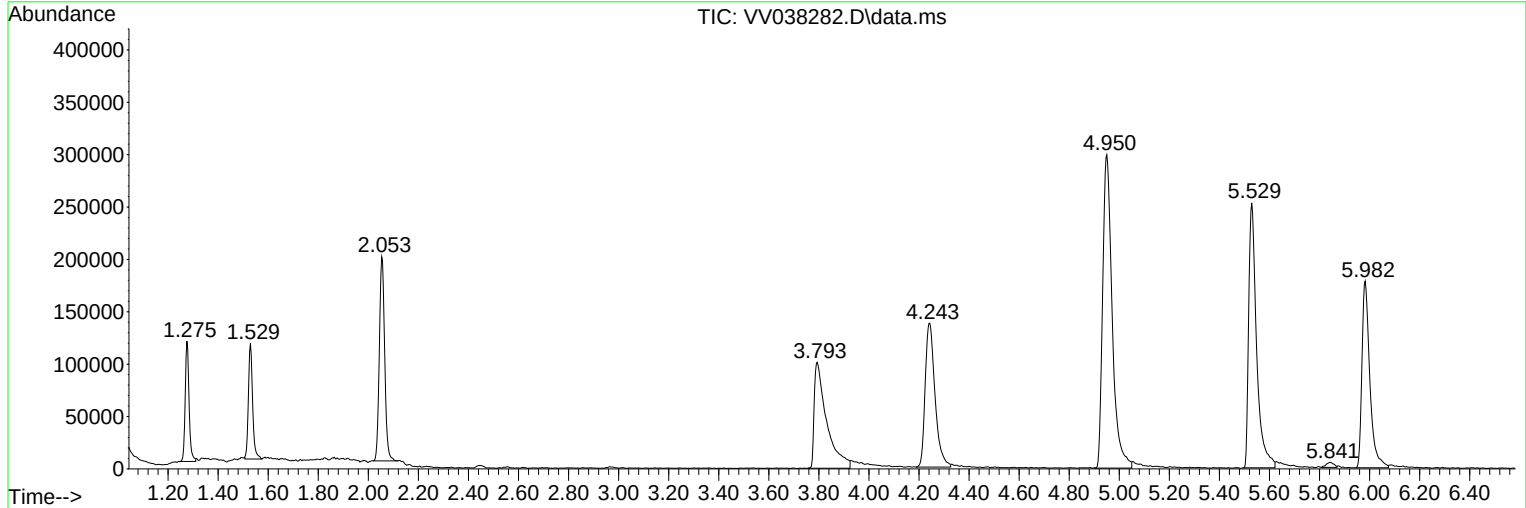

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038282.D
Acq On : 22 Nov 2024 21:07
Operator : SY/MD
Sample : VV1122WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK261

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038282.D
Acq On : 22 Nov 2024 21:07
Operator : SY/MD
Sample : VV1122WBL02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK261

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
