

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
 Data File : VV038283.D
 Acq On : 22 Nov 2024 21:31
 Operator : SY/MD
 Sample : P4883-05DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3K2DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038283.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	85	rBV	102472	110008	11.87%	1.292%
2	1.529	145	152	162	rBV	103449	123803	13.35%	1.455%
3	2.053	306	315	329	rVB	180725	270649	29.19%	3.180%
4	2.442	426	436	451	rVB	24630	42459	4.58%	0.499%
5	3.802	846	859	907	rBV2	138299	496812	53.59%	5.837%
6	4.243	976	996	1025	rBV	141869	387477	41.79%	4.552%
7	4.503	1063	1077	1098	rVB4	13767	37154	4.01%	0.437%
8	4.950	1202	1216	1248	rBV2	302538	802518	86.56%	9.429%
9	5.529	1386	1396	1425	rBV	235082	521935	56.29%	6.132%
10	5.825	1476	1488	1525	rBV	423627	898718	96.93%	10.559%
11	5.982	1525	1537	1565	rVV2	186348	401462	43.30%	4.717%
12	6.915	1815	1827	1855	rBV	67792	158420	17.09%	1.861%
13	7.239	1916	1928	1950	rBV	291306	551147	59.45%	6.475%
14	7.558	2017	2027	2046	rBV2	39057	85980	9.27%	1.010%
15	7.898	2113	2133	2155	rBV	283008	511764	55.20%	6.013%
16	8.021	2162	2171	2222	rBV	396864	927147	100.00%	10.893%
17	8.779	2397	2407	2438	rBV	404220	742369	80.07%	8.722%
18	10.146	2819	2832	2858	rBV	169749	292244	31.52%	3.434%
19	11.178	3142	3153	3176	rBV	347549	593822	64.05%	6.977%
20	11.554	3259	3270	3288	rBV2	324385	555628	59.93%	6.528%

Sum of corrected areas: 8511516




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038283.D
Acq On : 22 Nov 2024 21:31
Operator : SY/MD
Sample : P4883-05DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3K2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

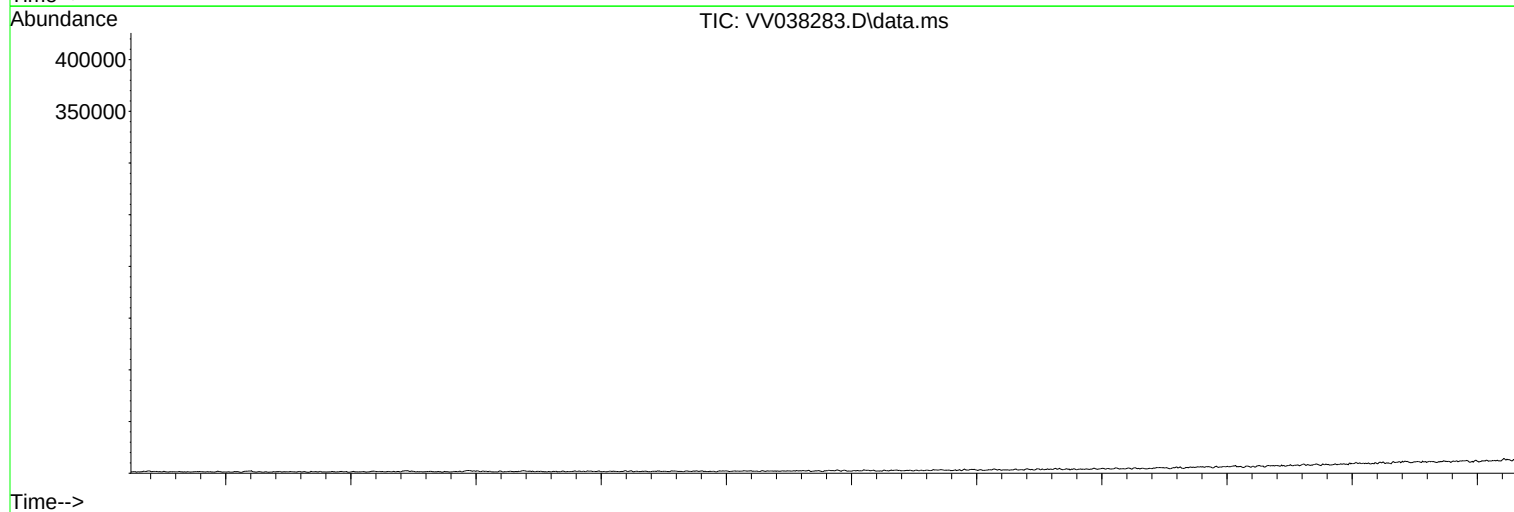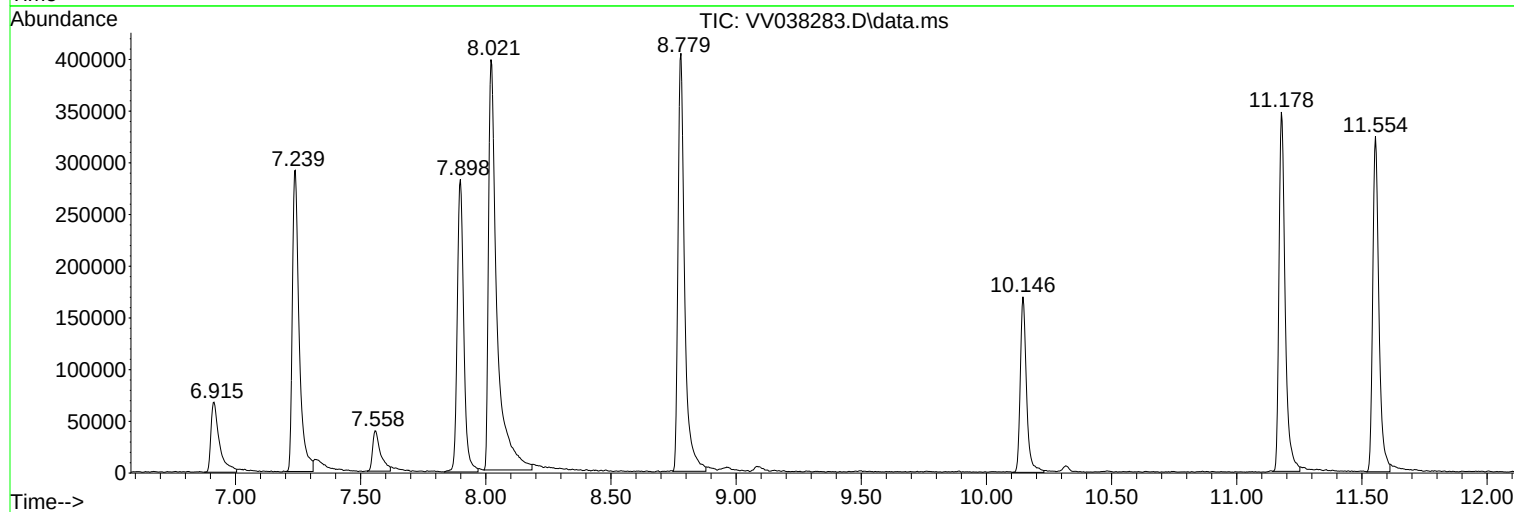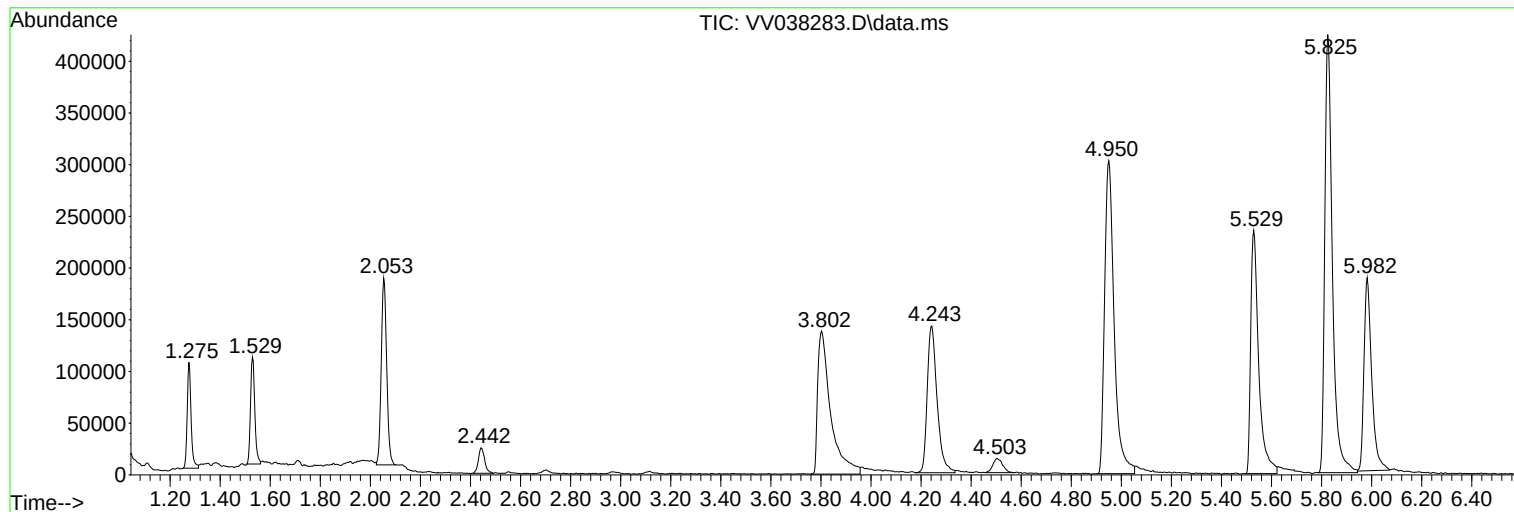

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038283.D
Acq On : 22 Nov 2024 21:31
Operator : SY/MD
Sample : P4883-05DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3K2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038283.D
Acq On : 22 Nov 2024 21:31
Operator : SY/MD
Sample : P4883-05DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3K2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------