

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
 Data File : VV038284.D
 Acq On : 22 Nov 2024 21:55
 Operator : SY/MD
 Sample : P4883-20
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038284.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	84	rBV	115481	116736	14.64%	1.800%
2	1.529	145	152	164	rBV	107724	123664	15.51%	1.907%
3	2.053	305	315	334	rBV	191118	279923	35.10%	4.316%
4	3.793	845	856	892	rBV2	104865	355129	44.53%	5.476%
5	4.240	980	995	1026	rBV2	141393	379880	47.63%	5.858%
6	4.950	1202	1216	1253	rBV3	296959	797541	100.00%	12.298%
7	5.529	1386	1396	1431	rBV	212246	481763	60.41%	7.429%
8	5.844	1481	1494	1501	rBV	5420	11427	1.43%	0.176%
9	5.982	1523	1537	1569	rBV	180546	407960	51.15%	6.291%
10	6.915	1816	1827	1850	rBV	66164	147044	18.44%	2.267%
11	7.236	1918	1927	1960	rBV	277537	544019	68.21%	8.389%
12	7.558	2018	2027	2045	rBV2	38095	83362	10.45%	1.285%
13	7.905	2127	2135	2147	rVB4	13554	25880	3.24%	0.399%
14	8.021	2163	2171	2209	rBV	328158	759055	95.17%	11.705%
15	8.362	2267	2277	2289	rBV5	10054	20133	2.52%	0.310%
16	8.780	2397	2407	2437	rBV	353350	643525	80.69%	9.923%
17	10.146	2821	2832	2850	rBV	161580	271038	33.98%	4.179%
18	10.320	2877	2886	2896	rBV4	4932	8275	1.04%	0.128%
19	11.181	3144	3154	3184	rBV	294634	514192	64.47%	7.929%
20	11.554	3260	3270	3290	rBV	302894	514571	64.52%	7.935%




Sum of corrected areas: 6485117

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038284.D
Acq On : 22 Nov 2024 21:55
Operator : SY/MD
Sample : P4883-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

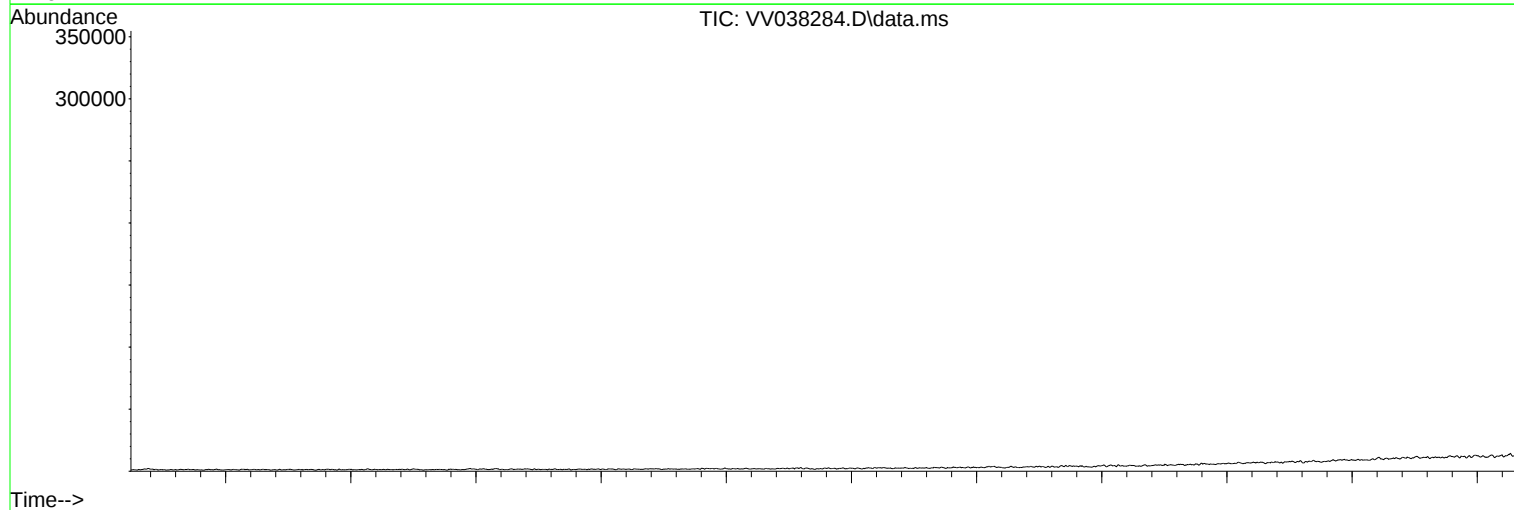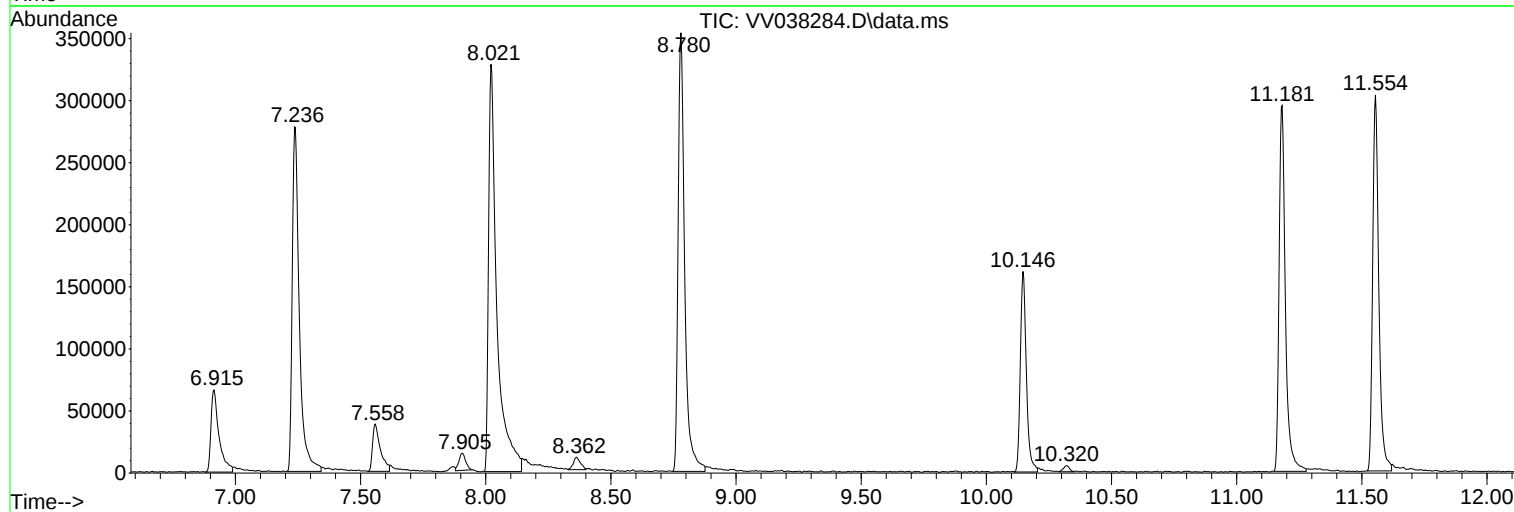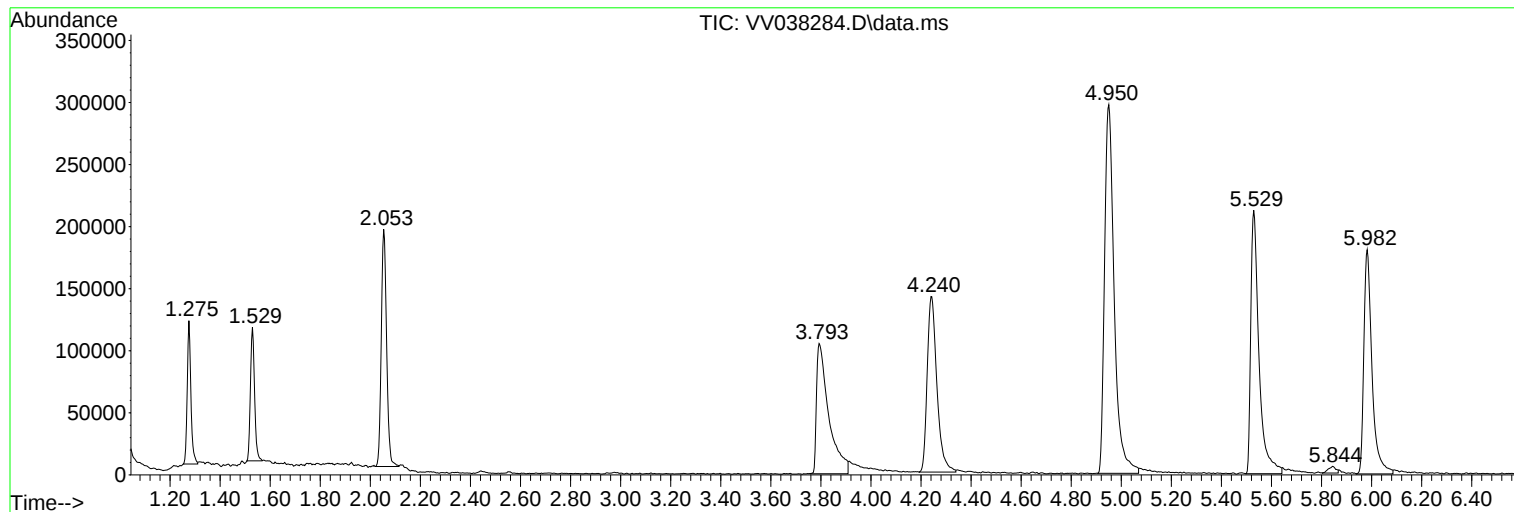

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038284.D
Acq On : 22 Nov 2024 21:55
Operator : SY/MD
Sample : P4883-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038284.D
Acq On : 22 Nov 2024 21:55
Operator : SY/MD
Sample : P4883-20
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
