

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
 Data File : VV038286.D
 Acq On : 22 Nov 2024 22:43
 Operator : SY/MD
 Sample : P4930-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG440

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038286.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	15	21	41	rVB	206793	227702	6.42%	1.549%
2	1.275	66	73	90	rBV	100949	107142	3.02%	0.729%
3	1.529	145	152	166	rVB	101607	119237	3.36%	0.811%
4	1.709	201	208	219	rVB	31385	40690	1.15%	0.277%
5	1.966	279	288	300	rVB	42245	63815	1.80%	0.434%
6	2.063	305	318	331	rBV4	604104	999530	28.18%	6.798%
7	2.256	362	378	413	rBV	103447	353968	9.98%	2.408%
8	2.442	426	436	449	rVB2	28535	49101	1.38%	0.334%
9	3.108	631	643	662	rBV2	22492	51116	1.44%	0.348%
10	3.802	844	859	900	rBV2	248763	811915	22.89%	5.522%
11	4.243	980	996	1026	rBV4	157223	496971	14.01%	3.380%
12	4.507	1063	1078	1098	rBV3	43121	114937	3.24%	0.782%
13	4.728	1131	1147	1163	rBV2	22982	54540	1.54%	0.371%
14	4.950	1200	1216	1245	rBV2	304015	815703	23.00%	5.548%
15	5.529	1384	1396	1425	rBV2	248680	558031	15.73%	3.795%
16	5.822	1474	1487	1526	rBV	1765060	3546573	100.00%	24.122%
17	5.982	1526	1537	1563	rVB2	189916	413036	11.65%	2.809%
18	6.912	1817	1826	1852	rBV	70060	156419	4.41%	1.064%
19	7.240	1916	1928	1947	rBV	290859	555905	15.67%	3.781%
20	7.555	2018	2026	2044	rBV	40705	86823	2.45%	0.591%
21	7.895	2113	2132	2156	rBV	1094353	1857564	52.38%	12.634%
22	8.021	2162	2171	2216	rBV	417704	918985	25.91%	6.250%
23	8.780	2396	2407	2435	rBV	440369	803033	22.64%	5.462%
24	10.146	2821	2832	2858	rBV	167402	290581	8.19%	1.976%
25	11.178	3143	3153	3184	rBV	368423	639127	18.02%	4.347%
26	11.554	3256	3270	3295	rBV	323102	570159	16.08%	3.878%

Sum of corrected areas: 14702603




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038286.D
Acq On : 22 Nov 2024 22:43
Operator : SY/MD
Sample : P4930-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG440

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

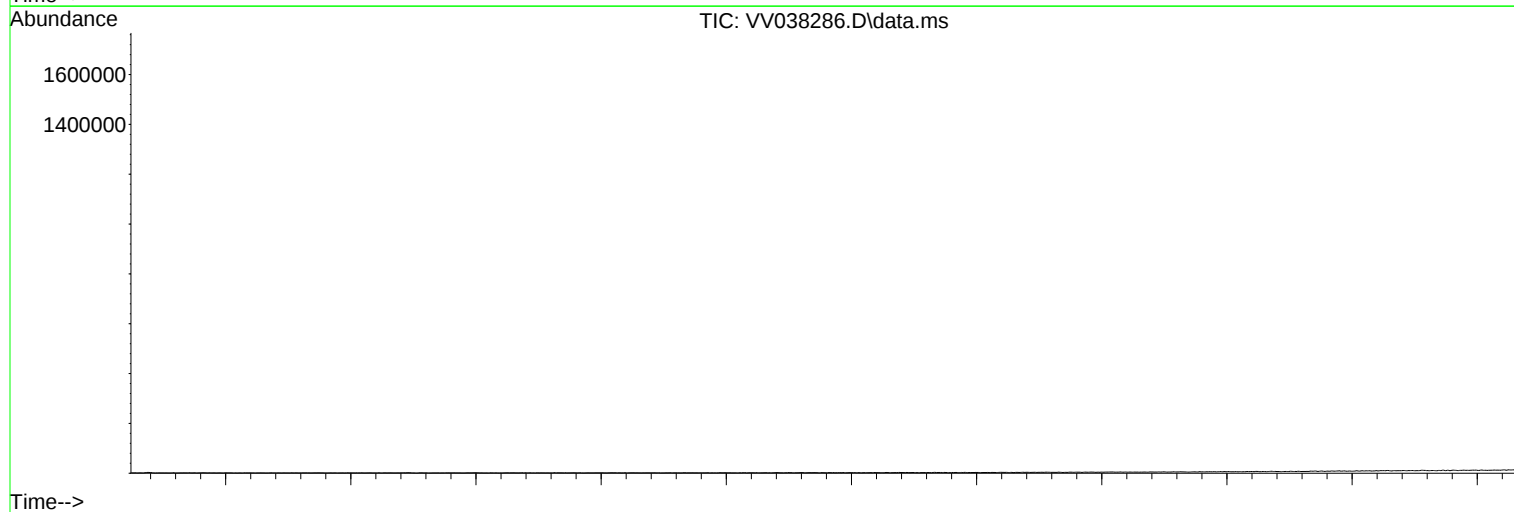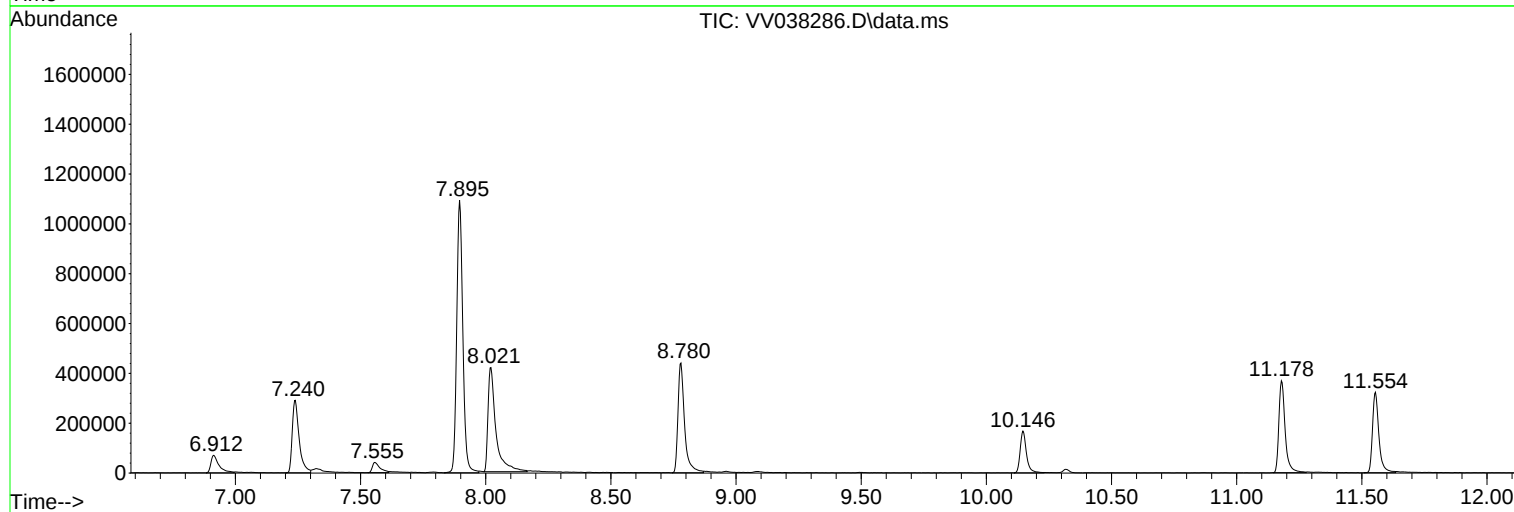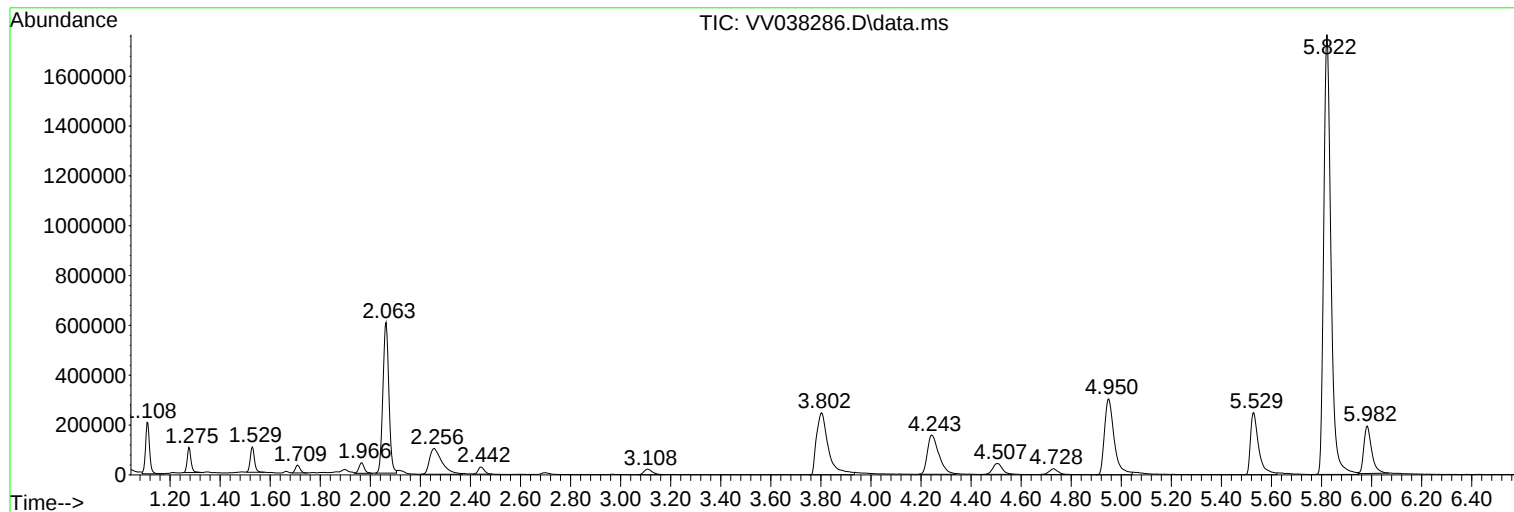

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038286.D
Acq On : 22 Nov 2024 22:43
Operator : SY/MD
Sample : P4930-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG440

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038286.D
Acq On : 22 Nov 2024 22:43
Operator : SY/MD
Sample : P4930-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG440

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
