
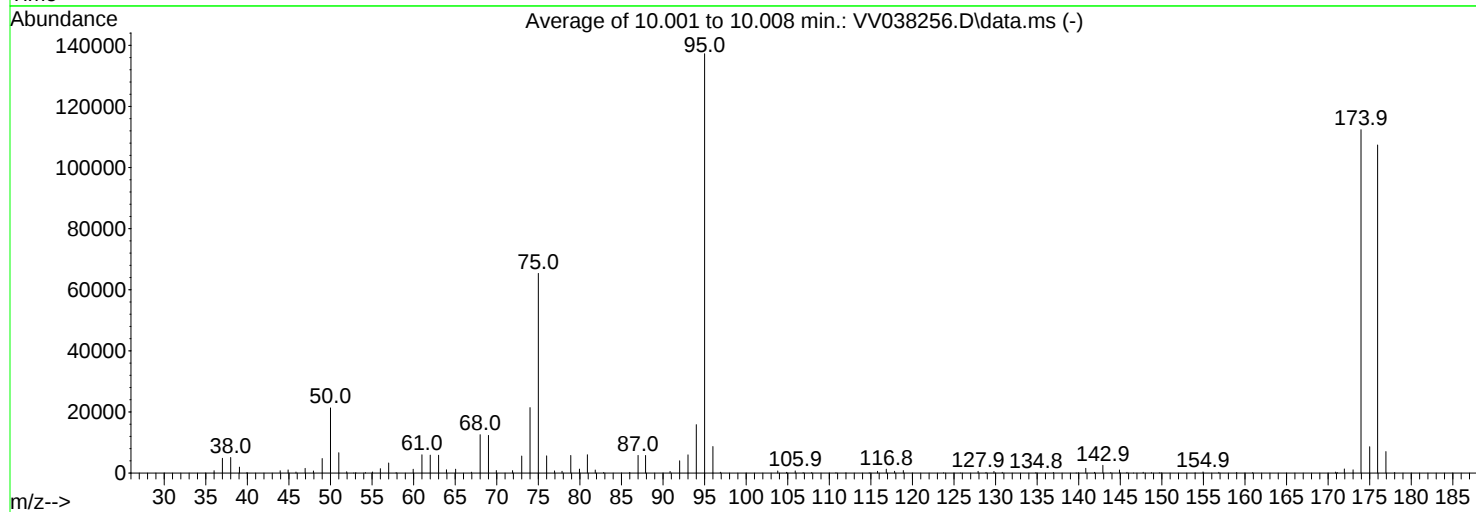


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112224\
Data File : VV038256.D
Acq On : 22 Nov 2024 08:06
Operator : SY/MD
Sample : BFB290
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB290

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Nov 25 00:21:44 2024

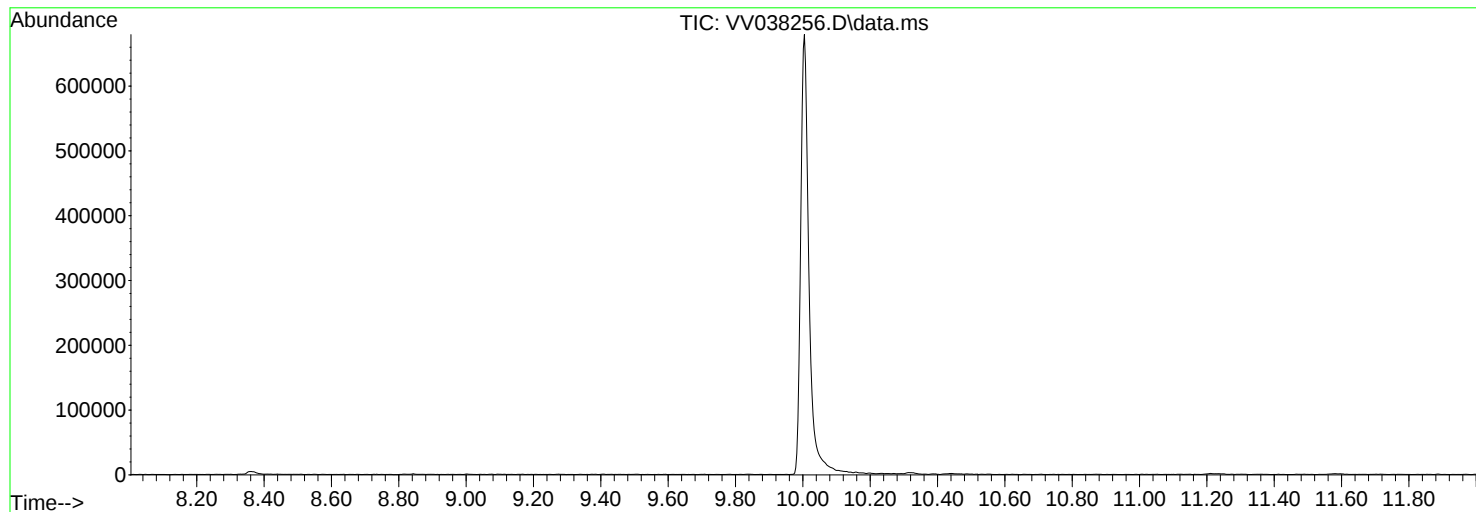

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	21339	PASS
75	95	30	80	47.6	65363	PASS
95	95	100	100	100.0	137259	PASS
96	95	5	9	6.3	8693	PASS
173	174	0.00	2	0.9	1067	PASS
174	95	50	120	81.9	112403	PASS
175	174	5	9	7.7	8627	PASS
176	174	95	105	95.5	107392	PASS
177	176	5	10	6.6	7040	PASS

m/z	Abundance
40.00	213.0
43.90	416.0
76.80	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290

m/z	Abundance
36.00	740.0
37.00	5099.0
38.00	5266.0
39.00	1942.0
40.10	386.0
44.00	1206.0
44.90	890.0
45.80	452.0
47.00	1630.0
47.90	594.0
49.00	4958.0
50.00	21720.0
51.00	6699.0
51.90	376.0
53.10	130.0
54.20	152.0
55.10	406.0
56.00	1464.0
57.00	3258.0
57.90	135.0
60.00	1219.0
61.00	5877.0
62.00	6220.0
63.00	5900.0
64.00	1096.0
65.00	1154.0
67.00	266.0
68.00	12815.0
69.00	12609.0
70.00	817.0
71.90	843.0
73.00	5632.0
74.00	21672.0
75.00	66472.0
76.00	6073.0
77.00	822.0
77.90	509.0
78.90	5772.0
80.00	1510.0
80.90	6042.0
81.90	1045.0
82.90	149.0
86.00	273.0
87.00	5954.0
87.90	5669.0
90.90	551.0
92.00	4300.0
93.00	6080.0
94.00	15657.0
95.00	138688.0
96.00	8673.0
96.90	429.0
103.80	689.0
104.90	260.0
105.90	742.0
106.80	147.0
107.90	129.0
110.80	134.0
115.80	567.0
116.90	1279.0
117.90	578.0
118.90	946.0
123.70	119.0
125.80	141.0
127.90	575.0
128.80	222.0
129.80	435.0
130.80	188.0
134.90	170.0
136.90	208.0
139.70	135.0
140.90	1500.0
141.90	308.0
142.90	2605.0
143.80	162.0
144.90	938.0
145.90	230.0
147.70	278.0
148.80	128.0
149.70	177.0
154.90	320.0
156.80	215.0
159.00	250.0
161.00	133.0
170.90	491.0
172.00	1294.0
173.00	1641.0
174.00	109856.0
175.00	8878.0
176.00	104992.0
176.90	6952.0
178.00	219.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290

m/z	Abundance
36.00	813.0
37.00	5056.0
38.00	5372.0
39.10	2004.0
39.90	363.0
44.00	1225.0
44.90	1072.0
45.90	383.0
47.00	1594.0
47.90	713.0
49.00	4899.0
50.00	21928.0
51.00	6842.0
51.90	492.0
53.10	123.0
54.20	183.0
55.10	387.0
56.00	1459.0
57.00	3405.0
57.90	174.0
60.00	1338.0
61.00	6172.0
62.00	6037.0
63.00	6110.0
64.00	1106.0
65.10	1338.0
67.00	332.0
68.00	12990.0
69.00	12619.0
70.00	848.0
71.90	859.0
73.00	5755.0
74.00	21928.0
75.00	67344.0
76.00	5758.0
77.00	883.0
77.90	666.0
78.90	5938.0
80.00	1329.0
80.90	6295.0
81.80	1022.0
82.80	214.0
86.00	200.0
87.00	6010.0
87.90	5994.0
90.80	539.0
92.00	4183.0
93.00	6159.0
94.00	16448.0
95.00	141632.0
96.00	8984.0
96.90	275.0
103.80	725.0
104.90	271.0
105.90	760.0
106.90	165.0
107.80	156.0
110.80	151.0
112.00	104.0
114.80	107.0
115.80	585.0
116.80	1334.0
117.80	618.0
118.90	848.0
123.80	116.0
127.90	583.0
128.90	244.0
129.80	557.0
130.80	263.0
134.90	165.0
136.90	217.0
139.90	111.0
140.80	1651.0
141.90	257.0
142.90	2637.0
143.80	191.0
144.90	1042.0
145.80	263.0
147.70	282.0
148.70	150.0
149.70	150.0
155.00	399.0
156.80	240.0
159.00	255.0
160.90	141.0
170.90	511.0
171.90	1373.0
173.00	1561.0
174.00	116720.0
175.00	9031.0
175.90	111168.0
176.90	7320.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290

178.00

199.0

Instrument :

MSVOA_V

ClientSampleId :

BFB290

m/z	Abundance
36.00	809.0
37.00	4365.0
38.00	4707.0
39.10	1931.0
39.90	331.0
44.00	1130.0
44.90	1153.0
45.90	222.0
46.90	1400.0
48.00	758.0
49.00	4450.0
50.00	20368.0
51.00	6452.0
52.00	487.0
52.80	115.0
53.00	108.0
54.20	172.0
55.00	300.0
56.00	1432.0
57.00	3234.0
57.90	166.0
59.90	1257.0
61.00	5917.0
62.00	5396.0
63.00	5555.0
63.90	1075.0
65.00	1327.0
66.90	328.0
68.00	11900.0
69.00	11762.0
69.90	841.0
71.90	701.0
73.00	5381.0
74.00	20672.0
75.00	62272.0
76.00	5129.0
77.00	803.0
77.80	635.0
78.90	5569.0
79.90	1112.0
80.90	5682.0
81.80	971.0
82.80	235.0
86.00	138.0
87.00	5372.0
87.90	5637.0
90.80	533.0
92.00	3571.0
93.00	5680.0
94.00	15439.0
95.00	131456.0
96.00	8421.0
96.90	162.0
103.80	685.0
104.80	252.0
105.90	636.0
106.90	148.0
107.80	174.0
110.80	150.0
112.00	104.0
114.80	124.0
115.80	593.0
116.80	1291.0
117.80	589.0
118.90	726.0
123.70	105.0
127.90	547.0
128.90	264.0
129.80	669.0
130.80	294.0
134.80	158.0
137.00	222.0
140.00	105.0
140.80	1542.0
141.90	195.0
142.90	2395.0
143.90	191.0
144.90	1093.0
145.70	288.0
146.60	105.0
147.80	266.0
148.70	148.0
149.90	137.0
154.00	101.0
155.00	413.0
156.90	290.0
159.00	189.0
160.80	160.0
171.10	527.0
171.90	1376.0
173.90	110632.0
175.00	7973.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290

175.90	106016.0
177.00	6847.0
178.00	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB290