




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112324\
Data File : VV038302.D
Acq On : 23 Nov 2024 16:48
Operator : SY/MD
Sample : P4884-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3M8

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 11/25/2024
Supervised By :Semsettin Yesilyurt 11/25/2024

Quant Time: Nov 23 23:01:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 23 02:01:29 2024
Response via : Initial Calibration

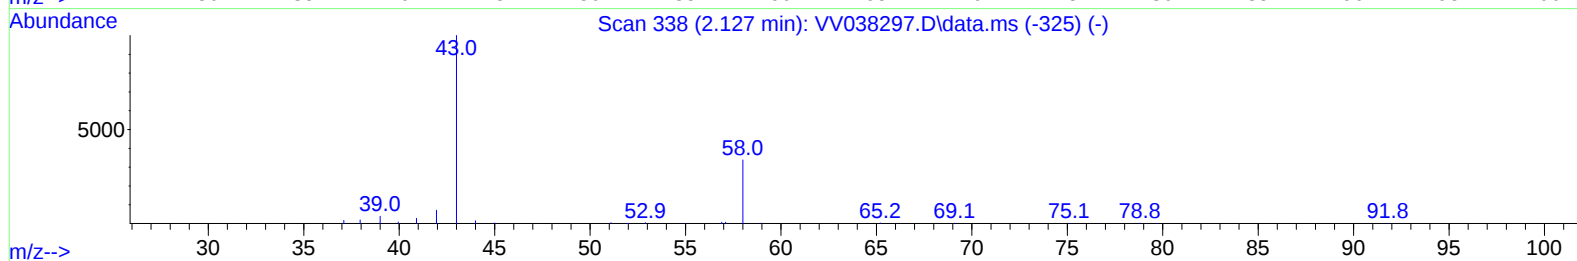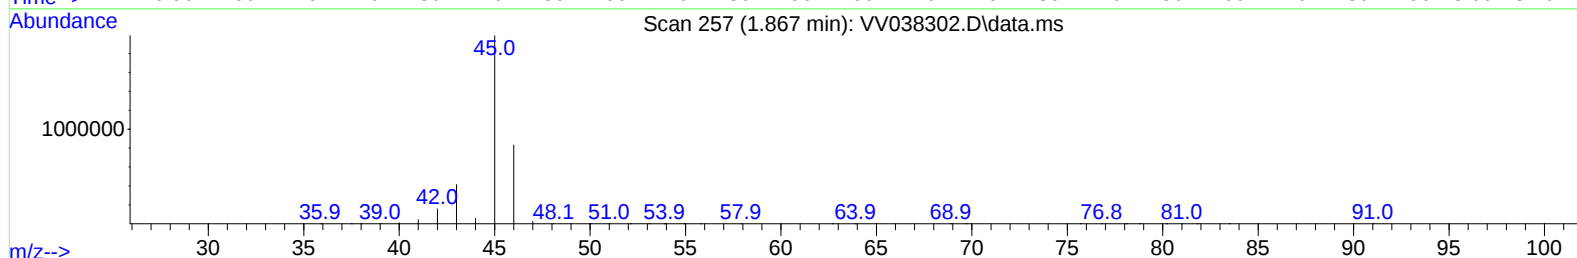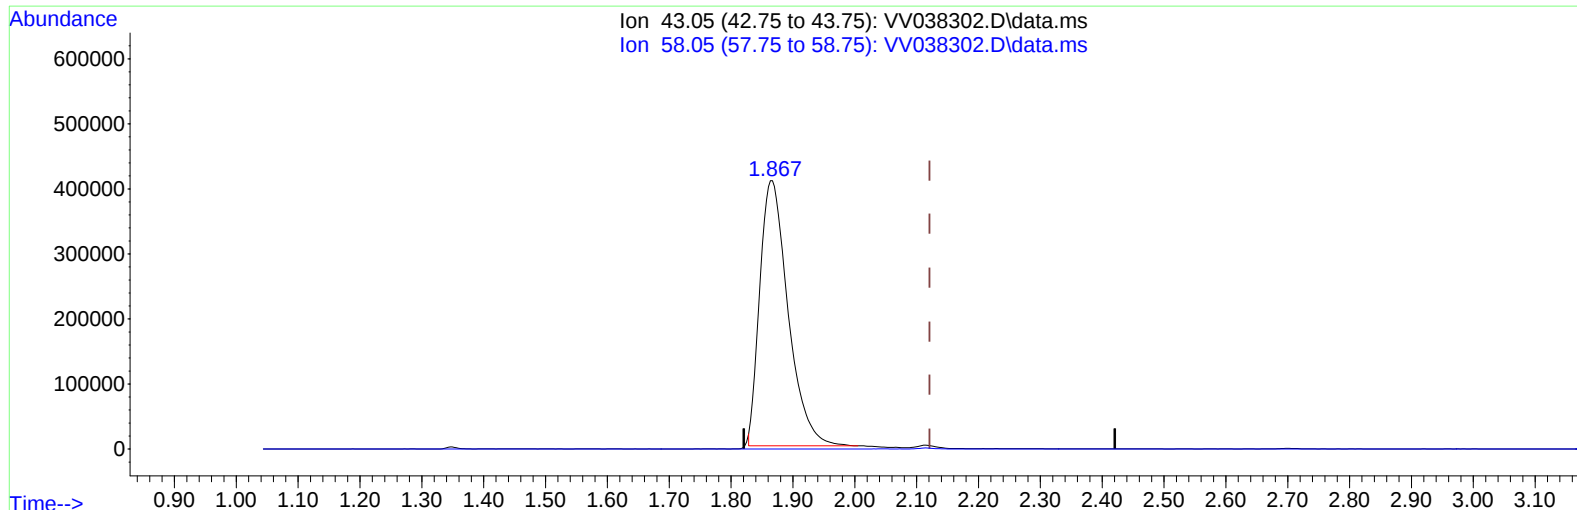

TIC: VV038302.D\data.ms

(13) Acetone (T)

1.867min (-0.254) 731.30 ug/L

response 1296595

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.60	0.01
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112324\
Data File : VV038302.D
Acq On : 23 Nov 2024 16:48
Operator : SY/MD
Sample : P4884-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3M8

Manual IntegrationsAPPROVED

Quant Time: Nov 23 23:01:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 23 02:01:29 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/25/2024
Supervised By :Semsettin Yesilyurt 11/25/2024

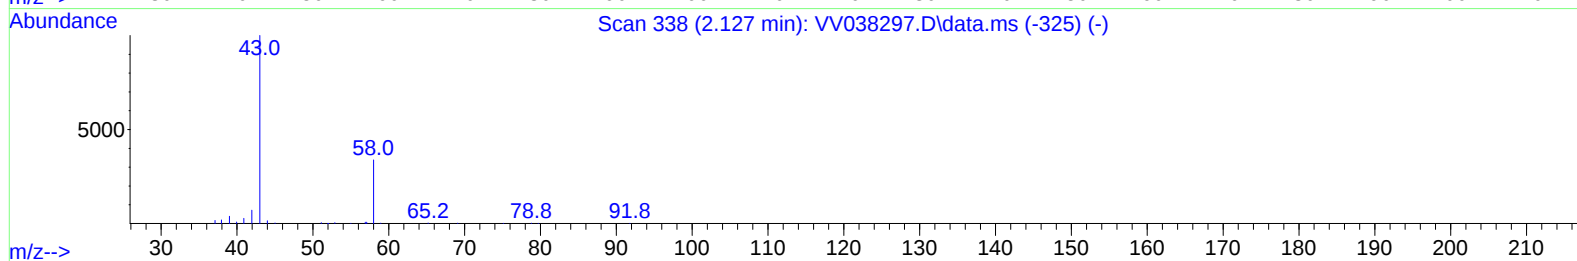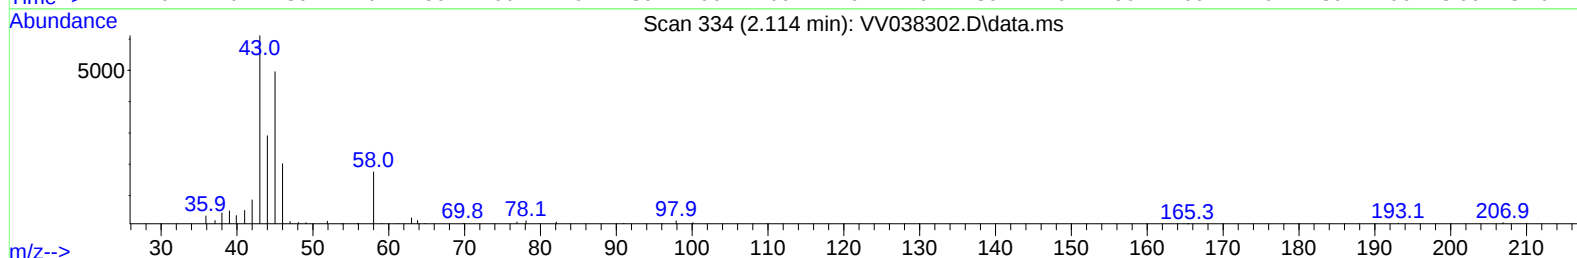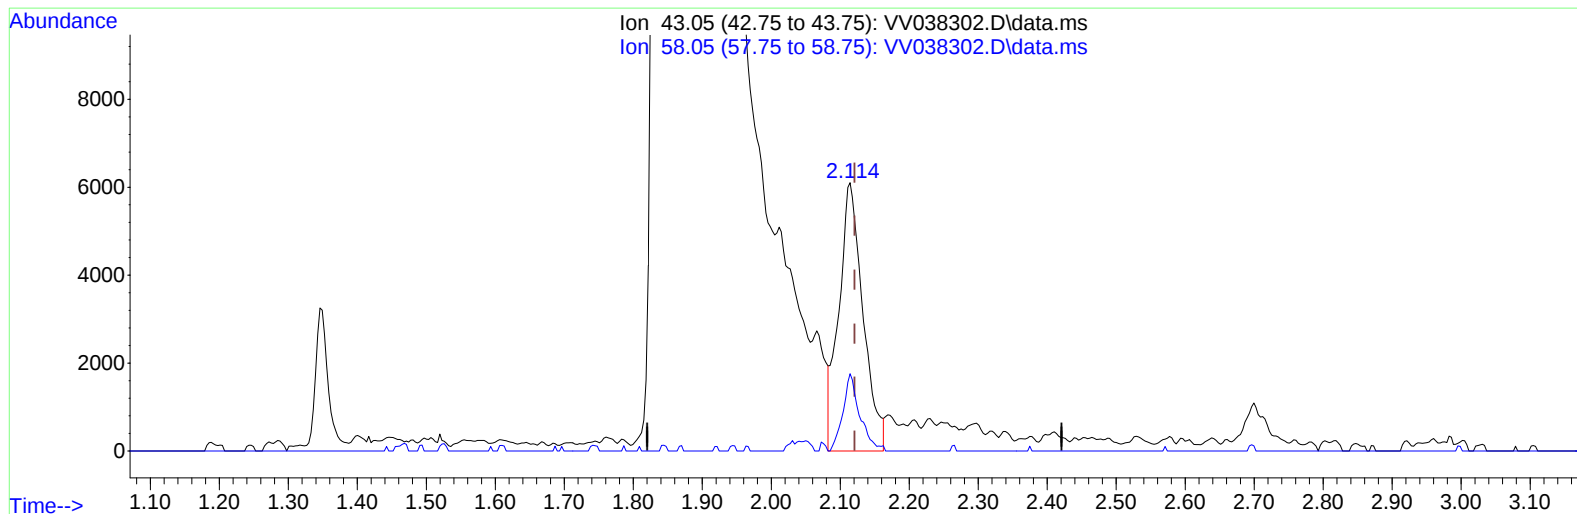

TIC: VV038302.D\data.ms

(13) Acetone (T)

2.114min (-0.006) 8.36 ug/L m

response 14814

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	33.60	1.05
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112324\
 Data File : VV038302.D
 Acq On : 23 Nov 2024 16:48
 Operator : SY/MD
 Sample : P4884-04
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3M8

Manual IntegrationsAPPROVED

Quant Time: Nov 23 23:01:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 23 02:01:29 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/25/2024
 Supervised By :Semsettin Yesilyurt 11/25/2024

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	156344	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	178206	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	74000	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	60769	5.071	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 101.400%		
7) Chloroethane-d5	1.529	69	64261	6.629	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 132.600%#		
11) 1,1-Dichloroethene-d2	2.053	65	29393	5.700	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 114.000%		
20) 2-Butanone-d5	3.786	46	166830	69.592	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 139.180%#		
24) Chloroform-d	4.243	84	164236	7.062	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 141.200%#		
26) 1,2-Dichloroethane-d4	4.937	65	79743	7.642	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 152.800%#		
32) Benzene-d6	4.953	84	284787	6.183	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 123.600%		
36) 1,2-Dichloropropane-d6	5.982	67	95698	6.752	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 135.000%		
41) Toluene-d8	7.240	98	220420	5.172	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 103.400%		
43) trans-1,3-Dichloroprop...	7.558	79	31433	5.965	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 119.400%		
46) 2-Hexanone-d5	8.018	63	135714	66.258	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 132.520%#		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	80165	6.663	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 133.200%#		
66) 1,2-Dichlorobenzene-d4	11.554	152	93088	7.383	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 147.600%#		
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.105	85	6781	0.458	ug/L	96
9) Trichlorofluoromethane	1.709	101	9881	0.481	ug/L	98
10) 1,1,2-Trichloro-1,2,2-...	2.063	101	4543	0.388	ug/L	90
13) Acetone	2.114	43	14814m	8.355	ug/L	
16) Methylene chloride	2.442	84	22262	1.748	ug/L	96
17) Methyl tert-butyl Ether	2.700	73	8801	0.349	ug/L #	89
29) 1,1,1-Trichloroethane	4.507	97	33039	1.546	ug/L	98
34) Trichloroethene	5.838	95	16718	1.225	ug/L	96
42) Toluene	7.323	91	20895	0.394	ug/L	97
47) Tetrachloroethene	7.899	164	53568	4.885	ug/L	98
51) Chlorobenzene	8.812	112	11198	0.307	ug/L	95
52) Ethylbenzene	8.953	91	6061	0.108	ug/L	85
53) m,p-Xylene	9.075	106	4166	0.196	ug/L	75
67) 1,2-Dichlorobenzene	11.574	146	4026	0.190	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112324\
Data File : VV038302.D
Acq On : 23 Nov 2024 16:48
Operator : SY/MD
Sample : P4884-04
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3M8

Manual IntegrationsAPPROVED

Quant Time: Nov 23 23:01:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 23 02:01:29 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 11/25/2024
Supervised By :Semsettin Yesilyurt 11/25/2024

