

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112324\
 Data File : VV038309.D
 Acq On : 23 Nov 2024 19:37
 Operator : SY/MD
 Sample : P4884-01DL 5X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3M5DL

Quant Time: Nov 23 23:02:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Nov 23 02:01:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	203518	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	212356	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	94046	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	55898	3.583	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.600%
7) Chloroethane-d5	1.506	69	32261	2.557	ug/L	-0.02
Spiked Amount	5.000	Range	65 - 130	Recovery	=	51.200%#
11) 1,1-Dichloroethene-d2	2.043	65	25527	3.803	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.000%
20) 2-Butanone-d5	3.789	46	175337	56.187	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	112.380%
24) Chloroform-d	4.236	84	153522	5.071	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.400%
26) 1,2-Dichloroethane-d4	4.934	65	76117	5.603	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	112.000%
32) Benzene-d6	4.950	84	264377	4.817	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.400%
36) 1,2-Dichloropropane-d6	5.982	67	89395	5.293	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.800%
41) Toluene-d8	7.236	98	205781	4.052	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.000%
43) trans-1,3-Dichloroprop...	7.558	79	31637	5.039	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	100.800%
46) 2-Hexanone-d5	8.024	63	144284	59.114	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	118.220%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	82227	5.735	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	114.800%
66) 1,2-Dichlorobenzene-d4	11.554	152	90000	5.617	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.400%
Target Compounds	Qvalue					
9) Trichlorofluoromethane	1.690	101	359203	13.434	ug/L	100
10) 1,1,2-Trichloro-1,2,2-...	2.050	101	5785	0.379	ug/L	95
12) 1,1-Dichloroethene	2.053	96	4897	0.337	ug/L #	1
16) Methylene chloride	2.436	84	20668	1.247	ug/L	88
17) Methyl tert-butyl Ether	2.699	73	44781	1.363	ug/L	97
19) 1,1-Dichloroethane	3.098	63	35561	1.279	ug/L	96
22) cis-1,2-Dichloroethene	3.809	96	4065	0.257	ug/L	92
29) 1,1,1-Trichloroethane	4.503	97	16672	0.655	ug/L	97
34) Trichloroethene	5.841	95	15516	0.954	ug/L	99
42) Toluene	7.326	91	11383	0.180	ug/L	84
47) Tetrachloroethene	7.898	164	26414	2.022	ug/L	98
51) Chlorobenzene	8.808	112	7977	0.183	ug/L	97
53) m,p-Xylene	9.082	106	2033	0.080	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112324\
Data File : VV038309.D
Acq On : 23 Nov 2024 19:37
Operator : SY/MD
Sample : P4884-01DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3M5DL

Quant Time: Nov 23 23:02:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Nov 23 02:01:29 2024
Response via : Initial Calibration




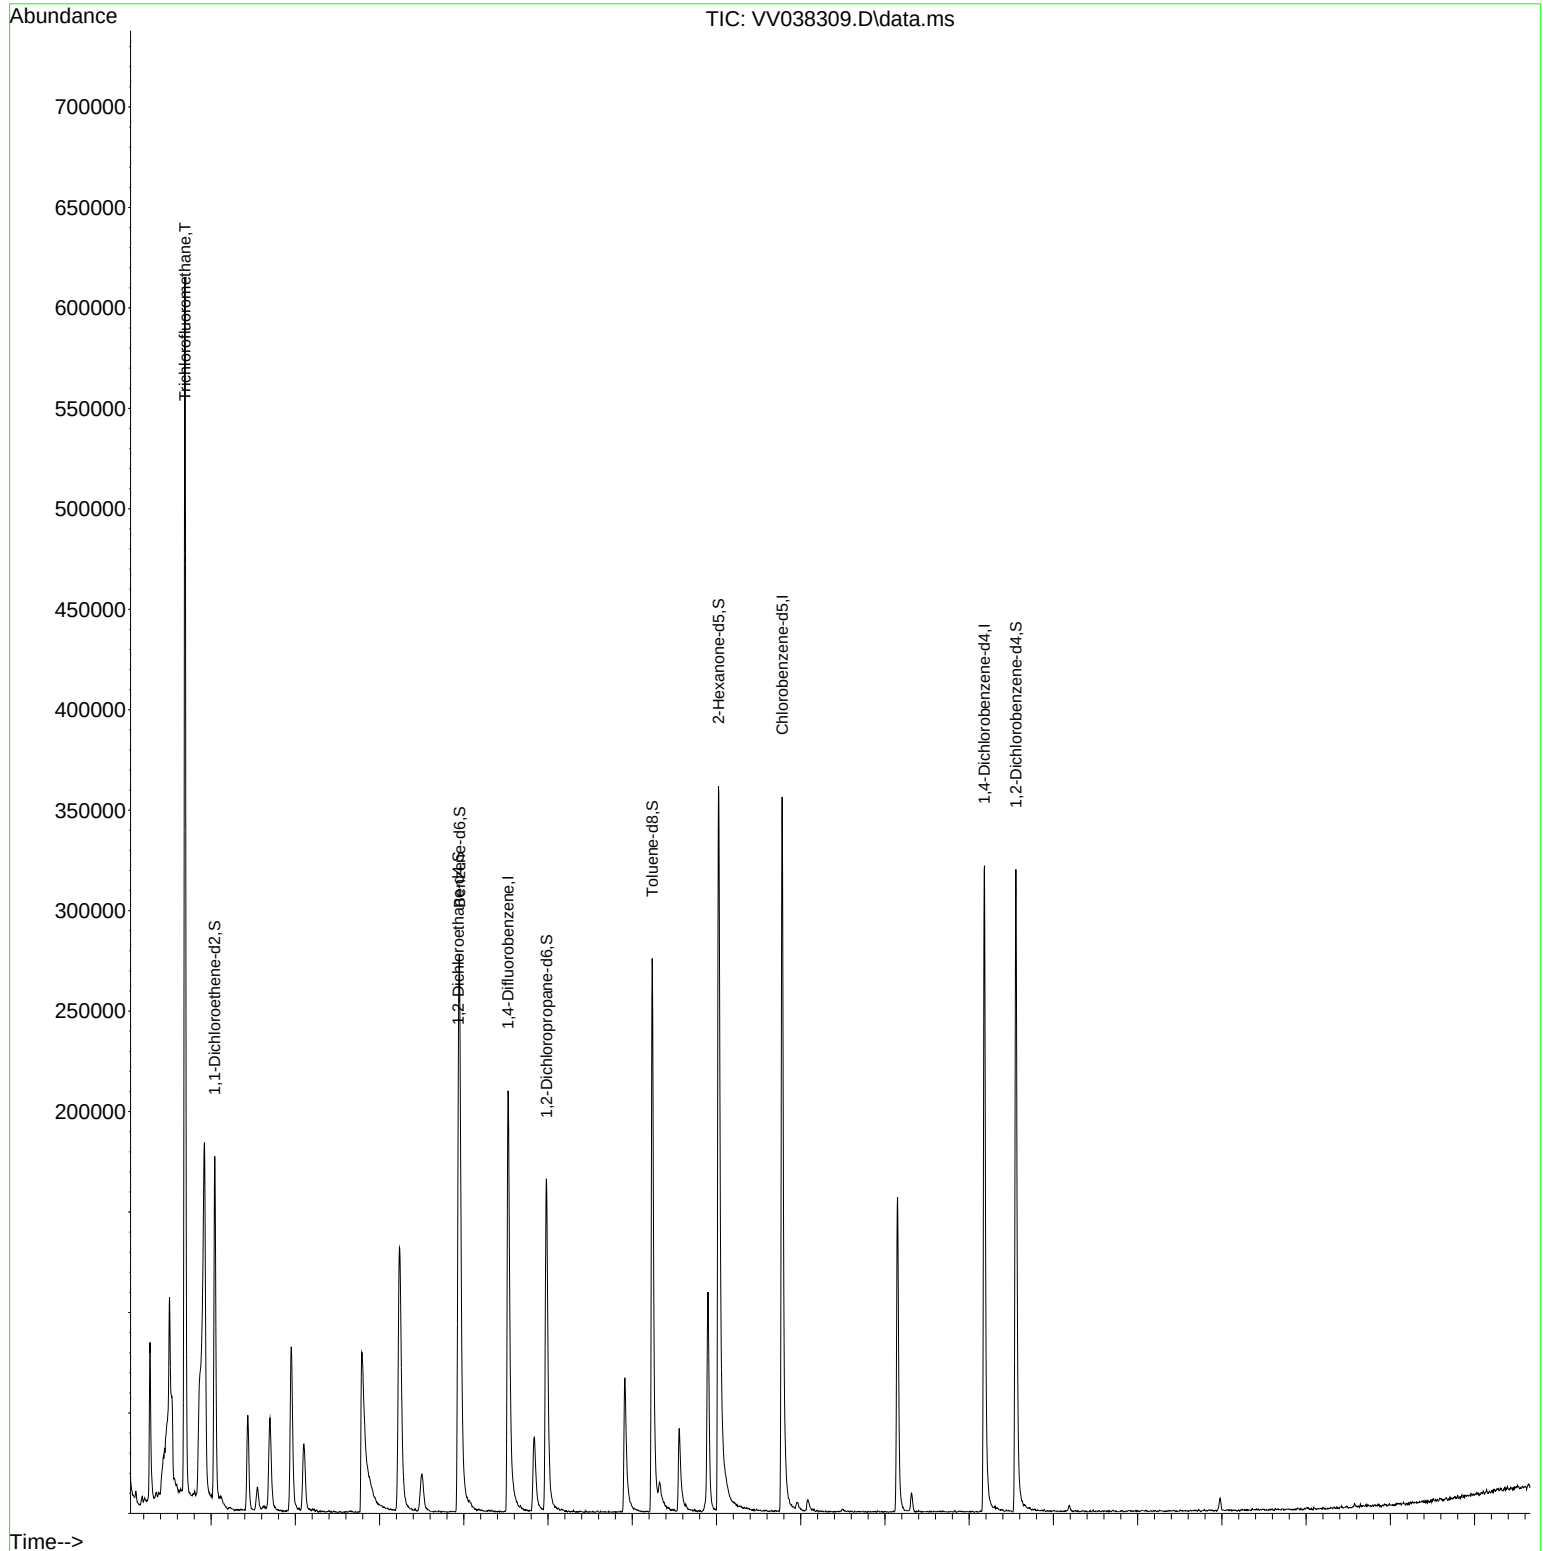




#9
Trichlorofluoromethane
Concen: 13.434 ug/L
RT: 1.690 min Scan# 208
Delta R.T. -0.019 min
Lab File: VV038309.D
Acq: 23 Nov 2024 19:37




Instrument :
MSVOA_V
ClientSampleId :
BG3M5DL


Tgt Ion:101 Resp: 359203
Ion Ratio Lower Upper
101 100
103 64.3 51.5 77.3

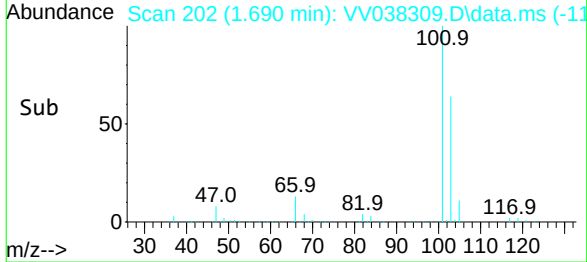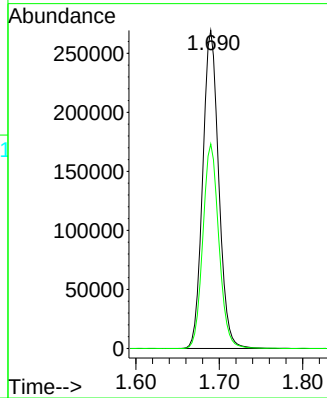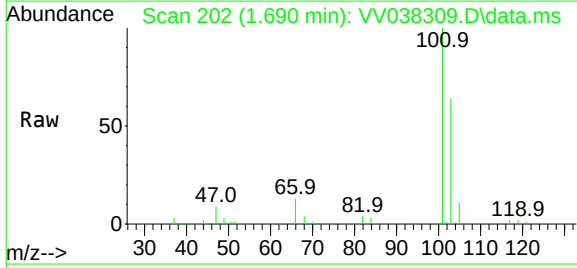

#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 0.379 ug/L
RT: 2.050 min Scan# 314
Delta R.T. -0.013 min
Lab File: VV038309.D
Acq: 23 Nov 2024 19:37

Tgt Ion:101 Resp: 5785
Ion Ratio Lower Upper
101 100
85 42.2 33.4 50.0
151 67.6 58.8 88.2


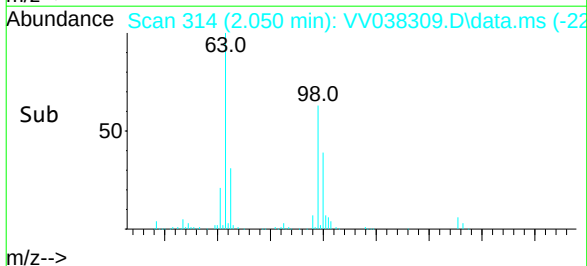
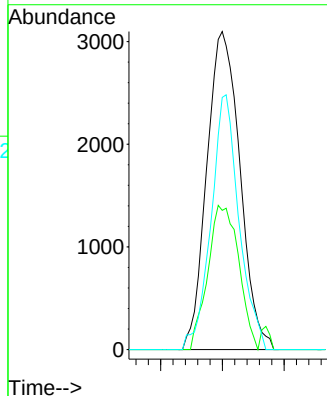
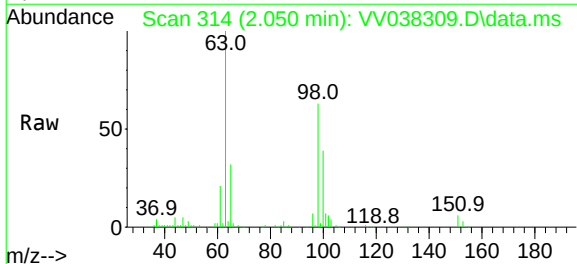




#12
1,1-Dichloroethene
Concen: 0.337 ug/L
RT: 2.053 min Scan# 31
Delta R.T. -0.010 min
Lab File: VV038309.D
Acq: 23 Nov 2024 19:37




Instrument :
MSVOA_V
ClientSampleId :
BG3M5DL


Tgt Ion: 96 Resp: 4897
Ion Ratio Lower Upper
96 100
61 254.6 115.7 214.9#
63 1035.1 101.1 187.7#

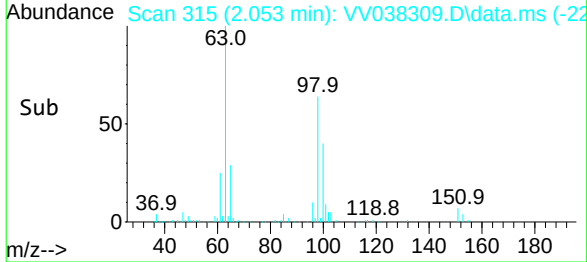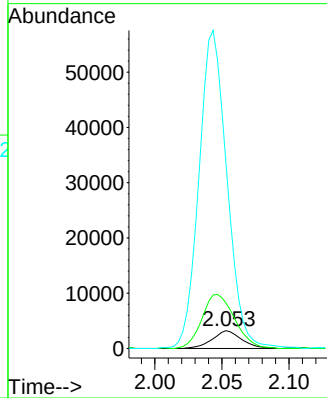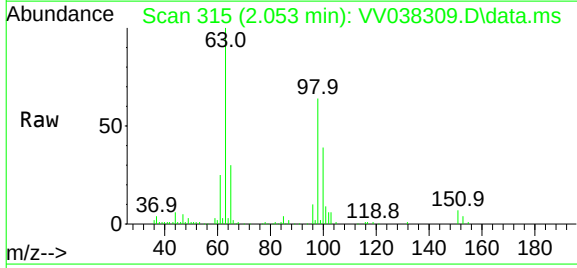

#16
Methylene chloride
Concen: 1.247 ug/L
RT: 2.436 min Scan# 434
Delta R.T. -0.003 min
Lab File: VV038309.D
Acq: 23 Nov 2024 19:37

Tgt Ion: 84 Resp: 20668
Ion Ratio Lower Upper
84 100
86 66.6 44.2 82.2
49 124.1 74.9 139.1


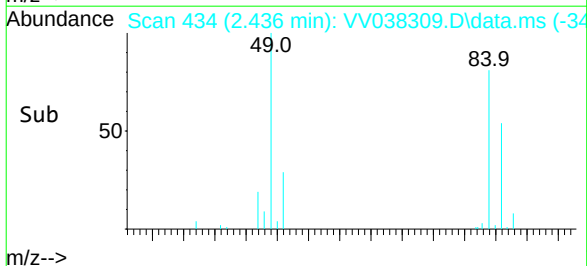
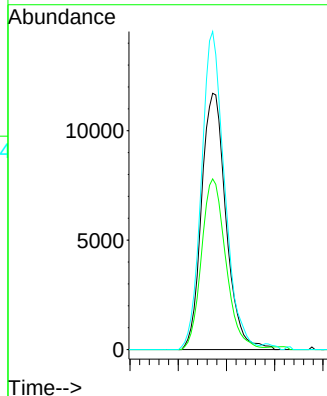
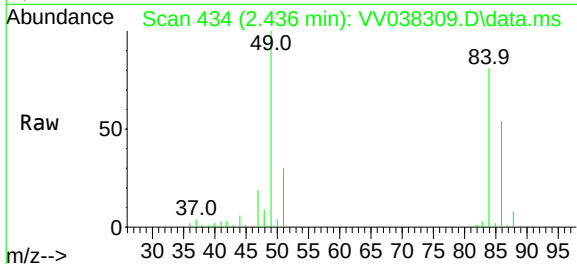




#17
Methyl tert-butyl Ether
Concen: 1.363 ug/L
RT: 2.699 min Scan# 515
Delta R.T. 0.003 min
Lab File: VV038309.D
Acq: 23 Nov 2024 19:37




Instrument :
MSVOA_V
ClientSampleId :
BG3M5DL


Tgt Ion:	73	Resp:	44781
Ion	Ratio	Lower	Upper
73	100		
43	18.4	14.2	21.2
57	24.0	17.6	26.4

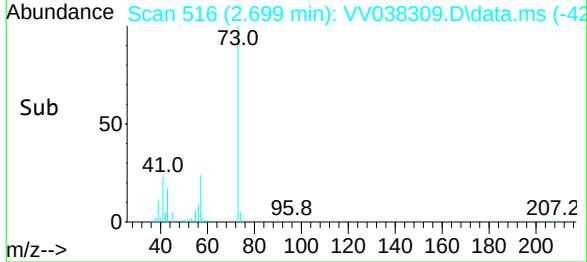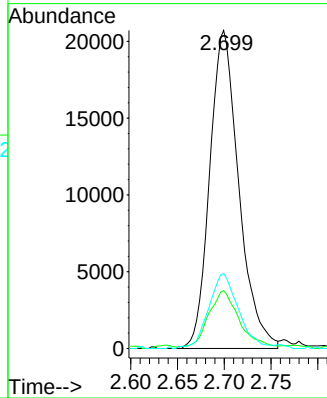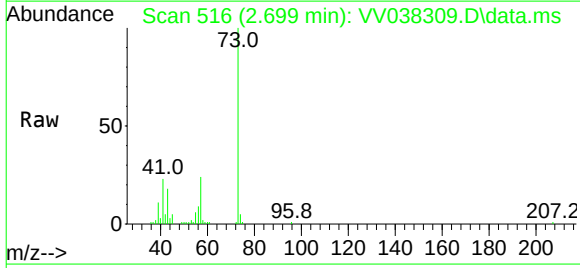

#19
1,1-Dichloroethane
Concen: 1.279 ug/L
RT: 3.098 min Scan# 640
Delta R.T. -0.006 min
Lab File: VV038309.D
Acq: 23 Nov 2024 19:37

Tgt Ion:	63	Resp:	35561
Ion	Ratio	Lower	Upper
63	100		
65	30.3	22.5	41.7
83	12.7	10.1	18.9


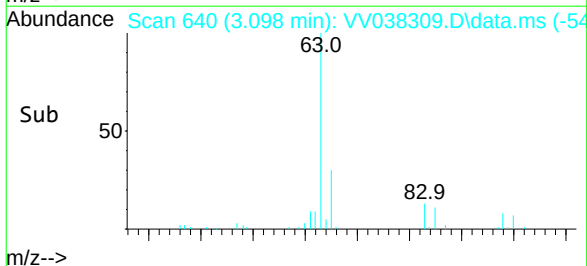
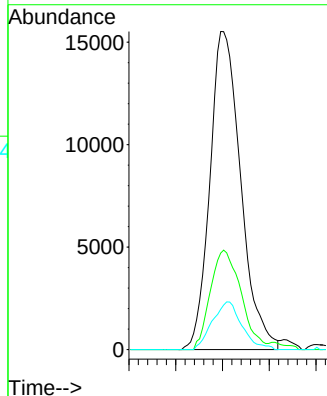
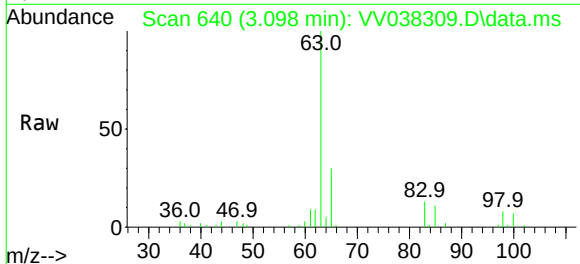




#22
cis-1,2-Dichloroethene
Concen: 0.257 ug/L
RT: 3.809 min Scan# 860
Delta R.T. 0.003 min
Lab File: VV038309.D
Acq: 23 Nov 2024 19:37




Instrument :
MSVOA_V
ClientSampleId :
BG3M5DL


Tgt Ion:	96	Resp:	4065
Ion	Ratio	Lower	Upper
96	100		
61	108.3	82.7	153.5
98	61.5	46.3	85.9

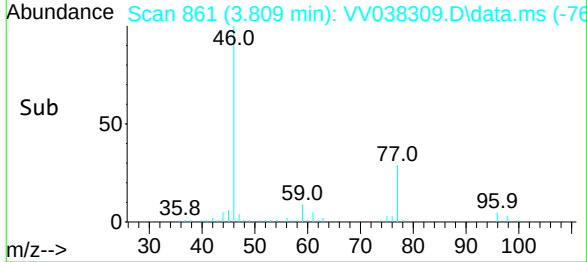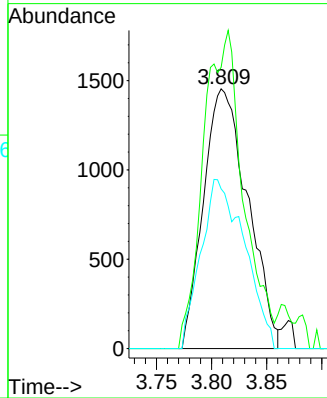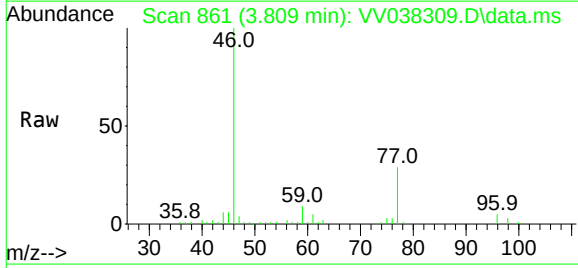

#29
1,1,1-Trichloroethane
Concen: 0.655 ug/L
RT: 4.503 min Scan# 1077
Delta R.T. -0.000 min
Lab File: VV038309.D
Acq: 23 Nov 2024 19:37

Tgt Ion:	97	Resp:	16672
Ion	Ratio	Lower	Upper
97	100		
99	65.6	51.8	77.8
61	44.1	32.2	48.2

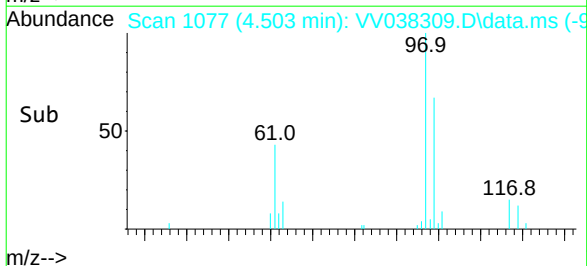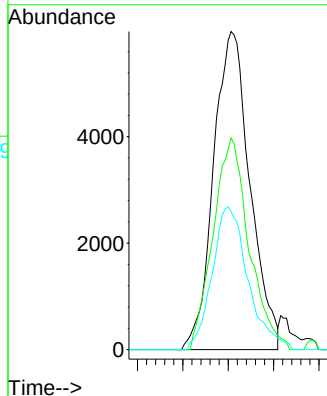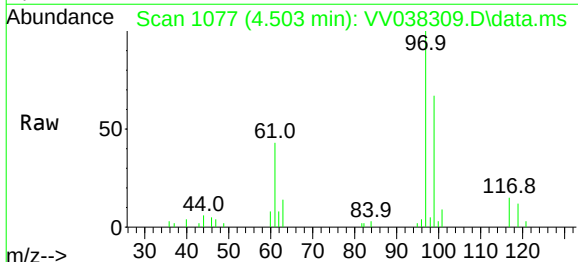

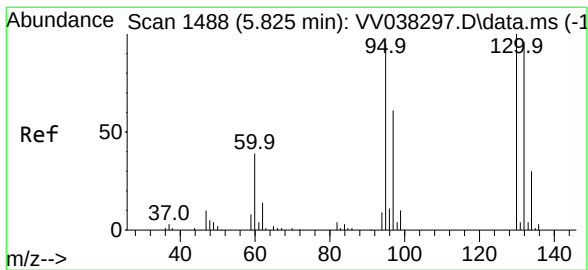

#34

Trichloroethene

Concen: 0.954 ug/L

RT: 5.841 min Scan# 14

Delta R.T. 0.013 min

Lab File: VV038309.D


Acq: 23 Nov 2024 19:37

Instrument :

MSVOA_V

ClientSampleId :

BG3M5DL

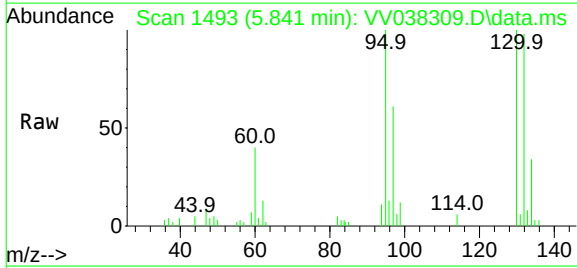

Tgt Ion: 95 Resp: 15516




Ion Ratio Lower Upper

95 100

97 60.8 44.8 83.2

132 97.9 68.3 126.8

130 100.3 70.2 130.4

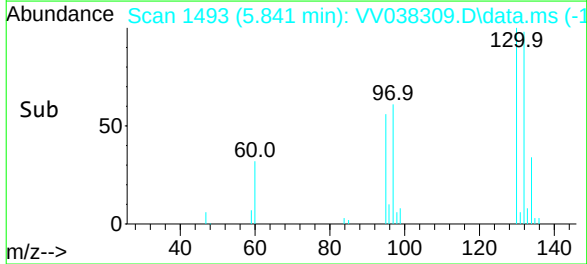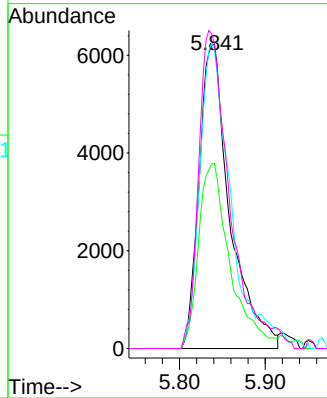

#42

Toluene

Concen: 0.180 ug/L

RT: 7.326 min Scan# 1955

Delta R.T. 0.019 min

Lab File: VV038309.D




Acq: 23 Nov 2024 19:37


Tgt Ion: 91 Resp: 11383

Ion Ratio Lower Upper

91 100

92 46.3 40.8 75.8



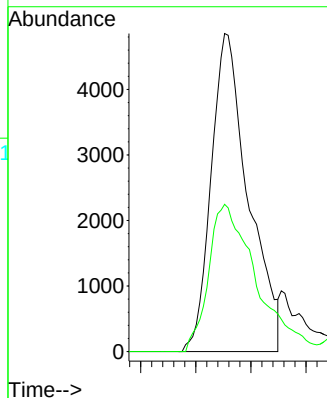
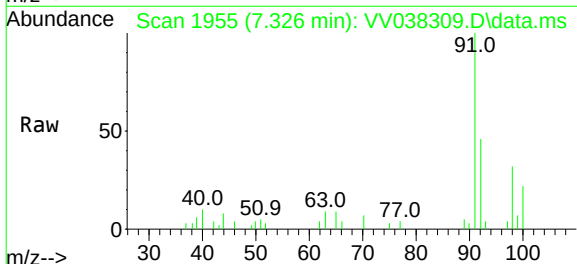


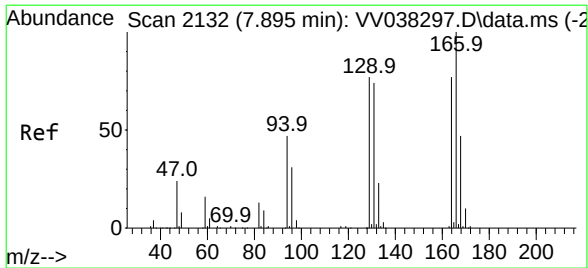

#47
Tetrachloroethene
Concen: 2.022 ug/L
RT: 7.898 min Scan# 2133
Delta R.T. 0.003 min
Lab File: VV038309.D
Acq: 23 Nov 2024 19:37




Instrument :
MSVOA_V
ClientSampleId :
BG3M5DL


Tgt Ion:	164	Resp:	26414
Ion Ratio	Lower	Upper	
164	100		
129	101.0	68.5	127.1
131	93.7	64.8	120.4
166	127.4	88.3	163.9

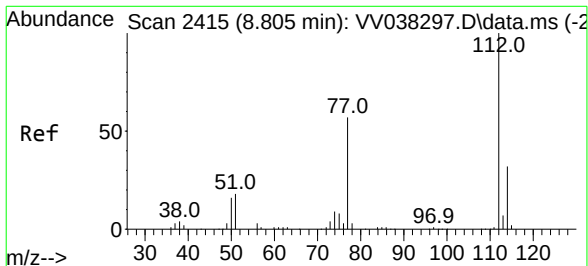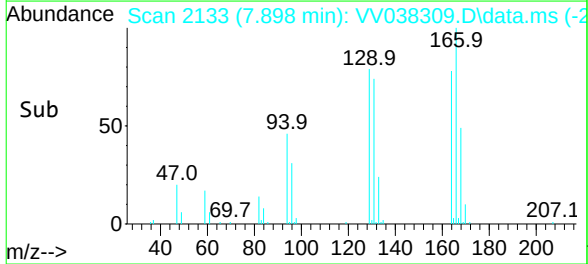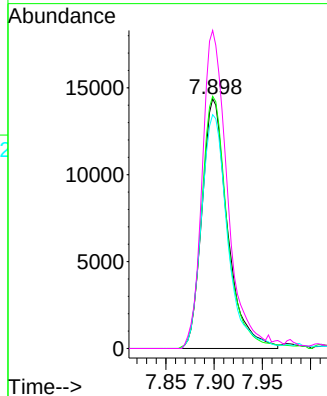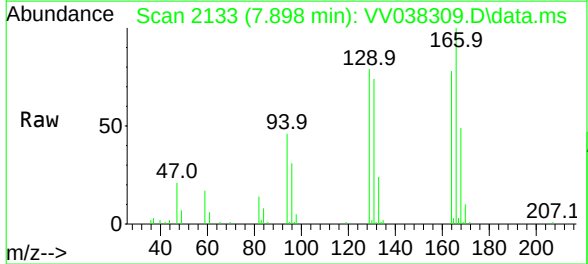

#51
Chlorobenzene
Concen: 0.183 ug/L
RT: 8.808 min Scan# 2416
Delta R.T. 0.003 min
Lab File: VV038309.D
Acq: 23 Nov 2024 19:37

Tgt Ion:	112	Resp:	7977
Ion Ratio	Lower	Upper	
112	100		
114	27.9	22.0	40.8
77	54.8	45.0	67.4

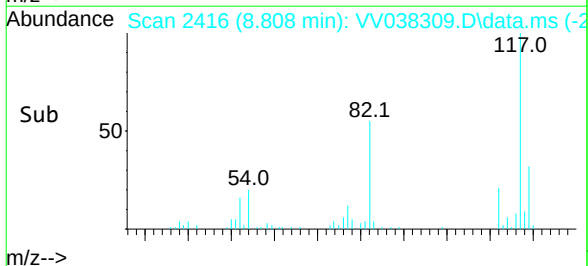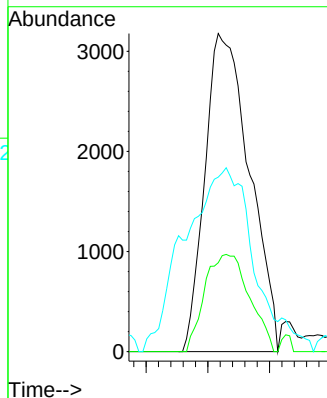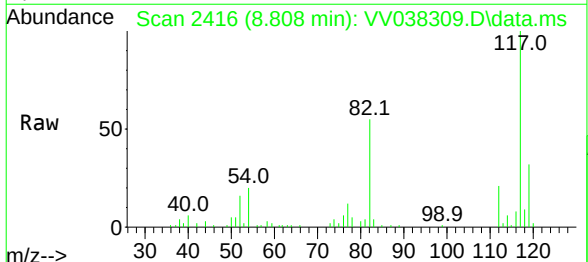

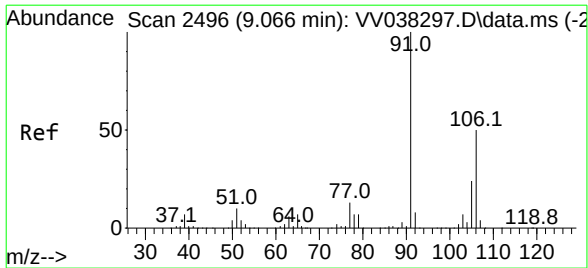

#53
 m,p-Xylene
 Concen: 0.080 ug/L
 RT: 9.082 min Scan# 251
 Delta R.T. 0.016 min
 Lab File: VV038309.D
 Acq: 23 Nov 2024 19:37

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3M5DL

Tgt Ion:	106	Resp:	2033
Ion Ratio	Lower	Upper	
106	100		
91	211.3	138.7	257.5

