

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112324\
 Data File : VV038304.D
 Acq On : 23 Nov 2024 17:36
 Operator : SY/MD
 Sample : P4884-10DL 2X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3N4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038304.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	85	rBV	89756	98490	1.66%	0.729%
2	1.529	144	152	164	rVB	93546	110533	1.86%	0.818%
3	1.867	241	257	296	rBV	1774198	5930496	100.00%	43.886%
4	2.053	307	315	328	rVV	164544	249807	4.21%	1.849%
5	3.789	846	855	887	rBV2	97650	336203	5.67%	2.488%
6	4.243	981	996	1029	rBV2	136789	366818	6.19%	2.714%
7	4.950	1202	1216	1267	rBV3	277385	759288	12.80%	5.619%
8	5.529	1387	1396	1419	rBV	195294	426955	7.20%	3.159%
9	5.828	1477	1489	1522	rBV2	274644	594294	10.02%	4.398%
10	5.982	1526	1537	1575	rVB	175097	383825	6.47%	2.840%
11	6.915	1817	1827	1857	rBV	63097	142929	2.41%	1.058%
12	7.239	1915	1928	1950	rBV	263967	507496	8.56%	3.756%
13	7.558	2016	2027	2054	rBV2	35497	84590	1.43%	0.626%
14	7.899	2115	2133	2160	rBV	511446	897268	15.13%	6.640%
15	8.021	2162	2171	2217	rVV	337449	739848	12.48%	5.475%
16	8.780	2396	2407	2437	rBV	342901	619379	10.44%	4.583%
17	10.146	2821	2832	2848	rBV	145869	246027	4.15%	1.821%
18	11.181	3144	3154	3183	rBV	284893	500911	8.45%	3.707%
19	11.554	3258	3270	3292	rBV	297661	518221	8.74%	3.835%




Sum of corrected areas: 13513378

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112324\
Data File : VV038304.D
Acq On : 23 Nov 2024 17:36
Operator : SY/MD
Sample : P4884-10DL 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3N4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

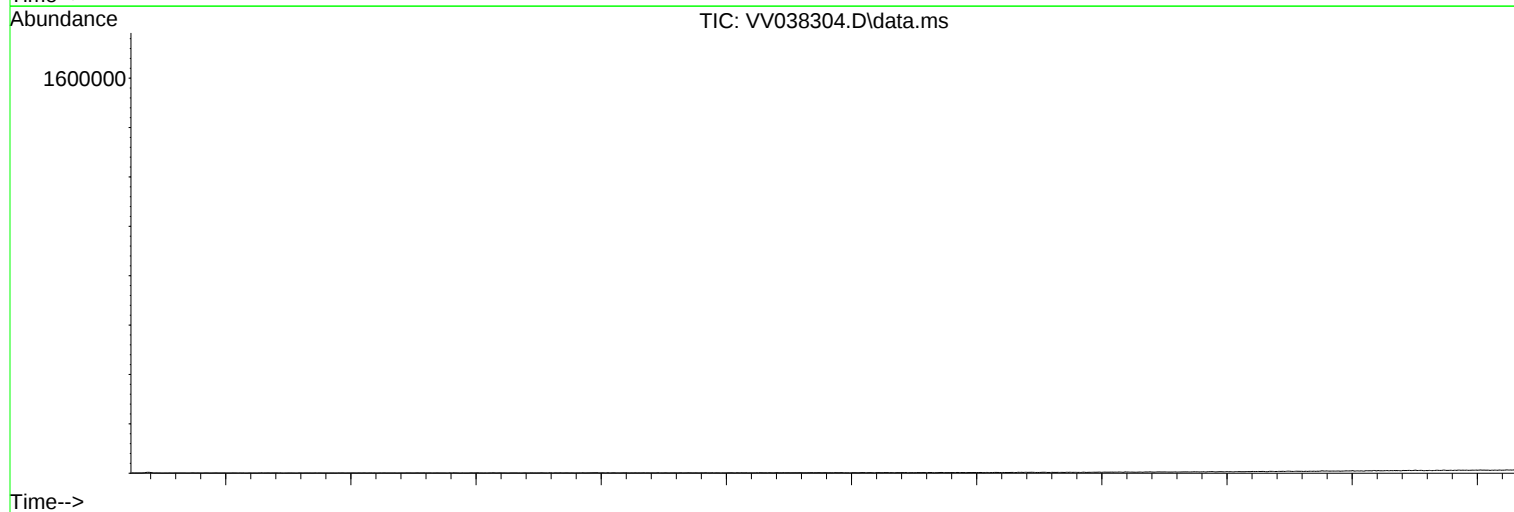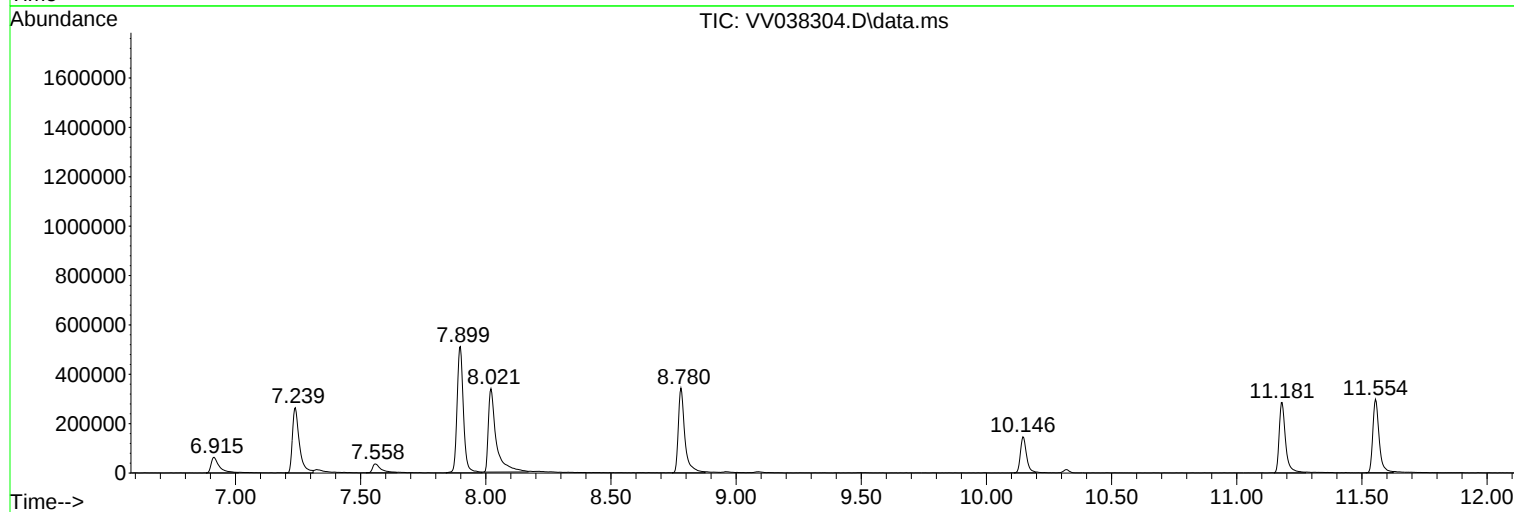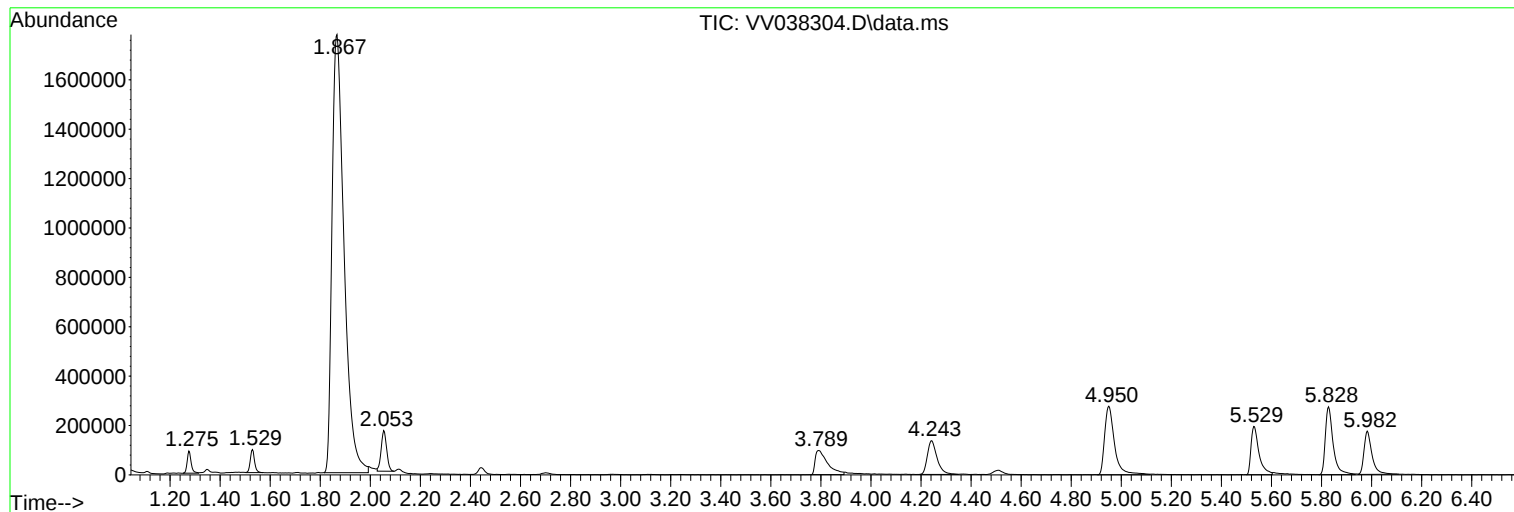

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112324\
Data File : VV038304.D
Acq On : 23 Nov 2024 17:36
Operator : SY/MD
Sample : P4884-10DL 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3N4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112324\
Data File : VV038304.D
Acq On : 23 Nov 2024 17:36
Operator : SY/MD
Sample : P4884-10DL 2X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3N4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
