

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112324\
 Data File : VV038306.D
 Acq On : 23 Nov 2024 18:25
 Operator : SY/MD
 Sample : P4884-18DL 100X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3P3DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038306.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	89	rBV	72537	81136	9.80%	1.307%
2	1.529	145	152	171	rVB	85759	103924	12.55%	1.675%
3	2.053	305	315	327	rBV	122311	178323	21.54%	2.874%
4	3.796	848	857	885	rBV	81977	263064	31.77%	4.239%
5	4.239	980	995	1020	rBV	108274	293668	35.47%	4.732%
6	4.950	1203	1216	1250	rBV2	222099	597561	72.18%	9.629%
7	5.529	1386	1396	1428	rBV	191627	430523	52.00%	6.938%
8	5.834	1478	1491	1518	rBV3	63647	156368	18.89%	2.520%
9	5.982	1525	1537	1574	rBV2	137643	309773	37.42%	4.992%
10	6.915	1816	1827	1853	rBV	49067	114059	13.78%	1.838%
11	7.239	1916	1928	1959	rBV	188665	369903	44.68%	5.961%
12	7.561	2018	2028	2054	rBV2	27360	67625	8.17%	1.090%
13	7.895	2113	2132	2160	rBV	460767	827900	100.00%	13.341%
14	8.021	2163	2171	2211	rBV	302798	682132	82.39%	10.992%
15	8.779	2393	2407	2441	rBV	340758	603793	72.93%	9.730%
16	10.146	2818	2832	2853	rBV	131383	222133	26.83%	3.580%
17	10.320	2877	2886	2898	rVB2	18877	29750	3.59%	0.479%
18	11.181	3142	3154	3186	rBV	280436	492825	59.53%	7.942%
19	11.554	3259	3270	3297	rBV	218131	381154	46.04%	6.142%

Sum of corrected areas: 6205614




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112324\
Data File : VV038306.D
Acq On : 23 Nov 2024 18:25
Operator : SY/MD
Sample : P4884-18DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3P3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

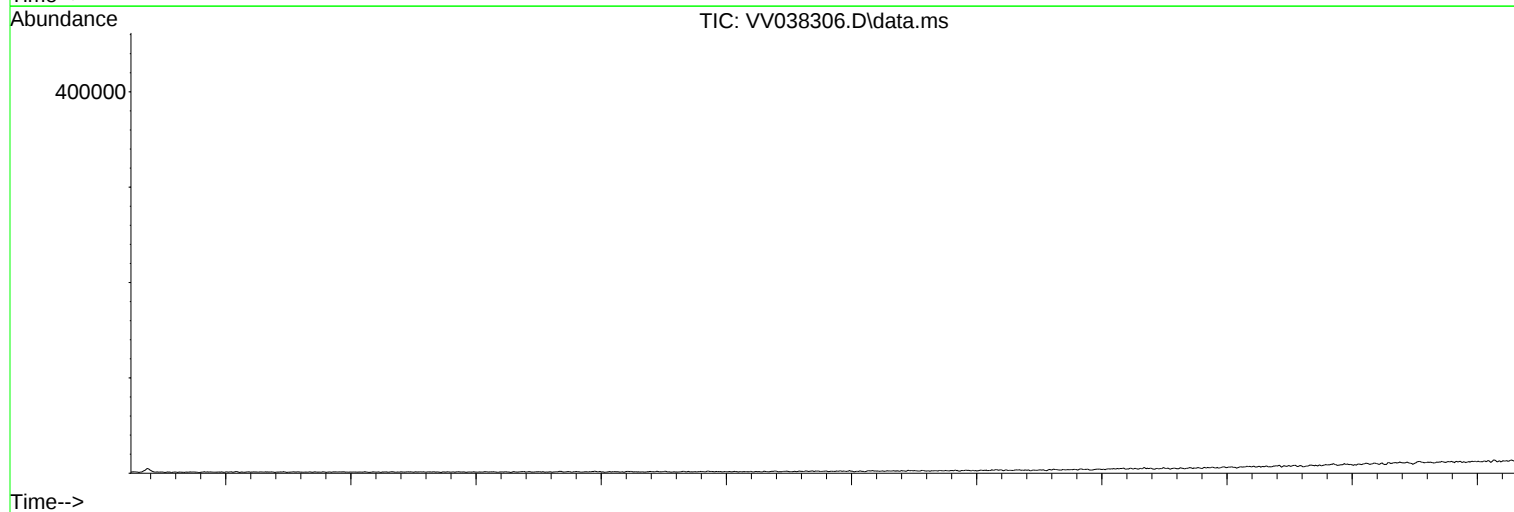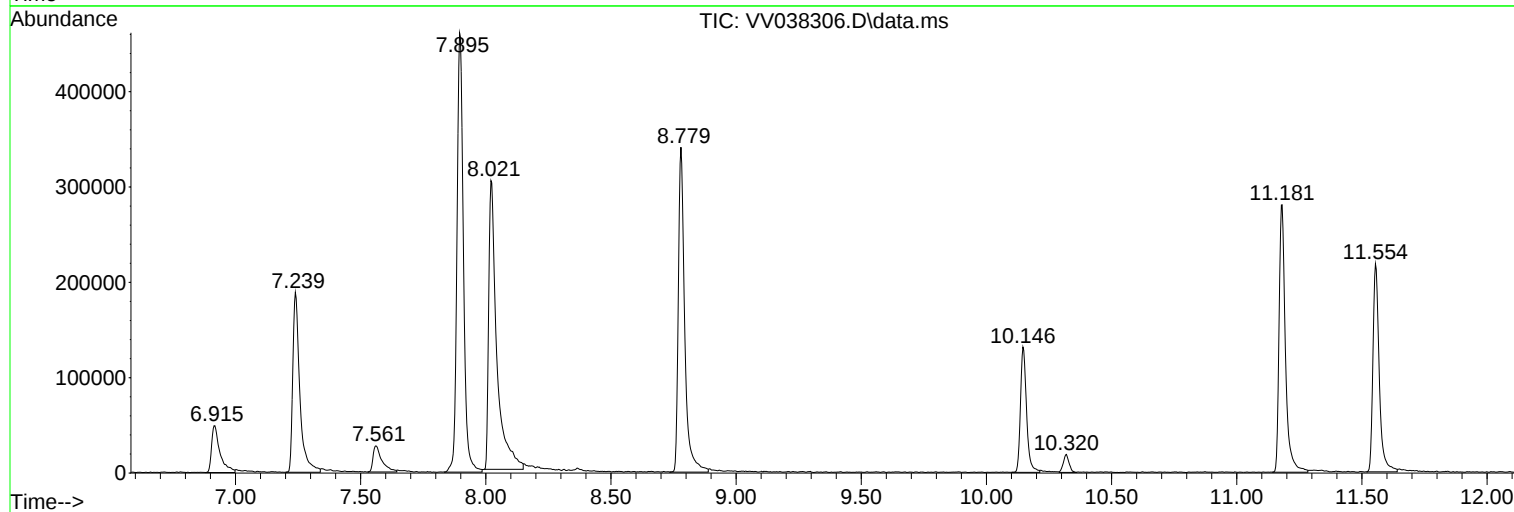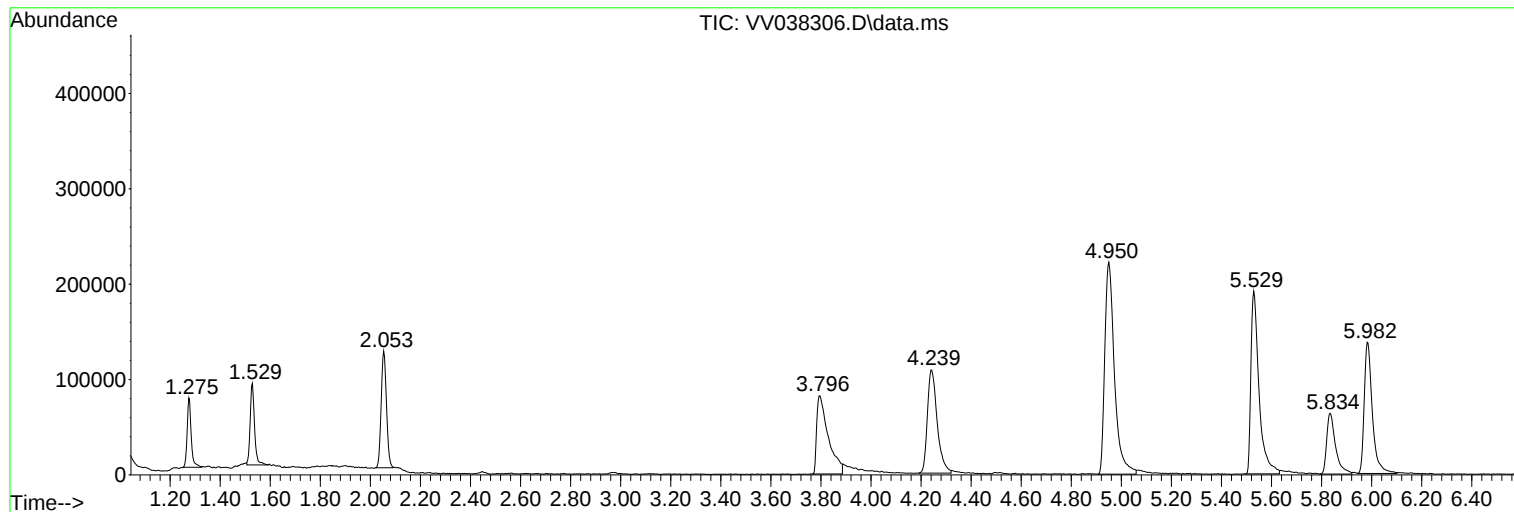

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112324\
Data File : VV038306.D
Acq On : 23 Nov 2024 18:25
Operator : SY/MD
Sample : P4884-18DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3P3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112324\
Data File : VV038306.D
Acq On : 23 Nov 2024 18:25
Operator : SY/MD
Sample : P4884-18DL 100X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3P3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc