
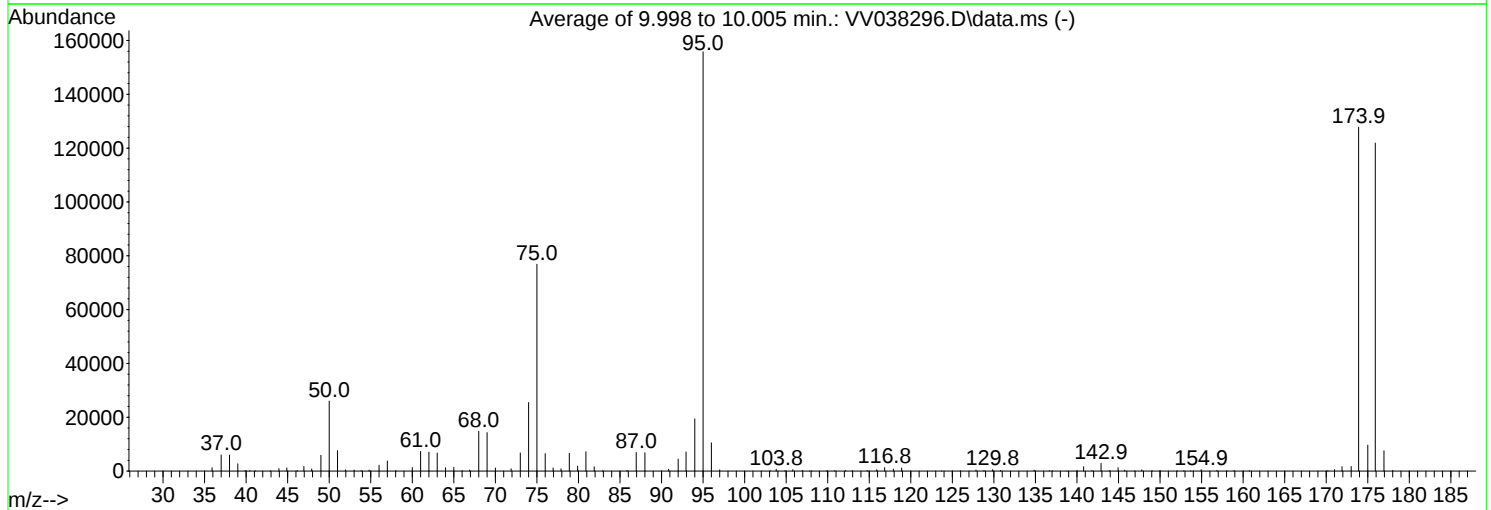


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112324\
Data File : VV038296.D
Acq On : 23 Nov 2024 13:13
Operator : SY/MD
Sample : BFB291
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB291

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Nov 26 00:39:03 2024

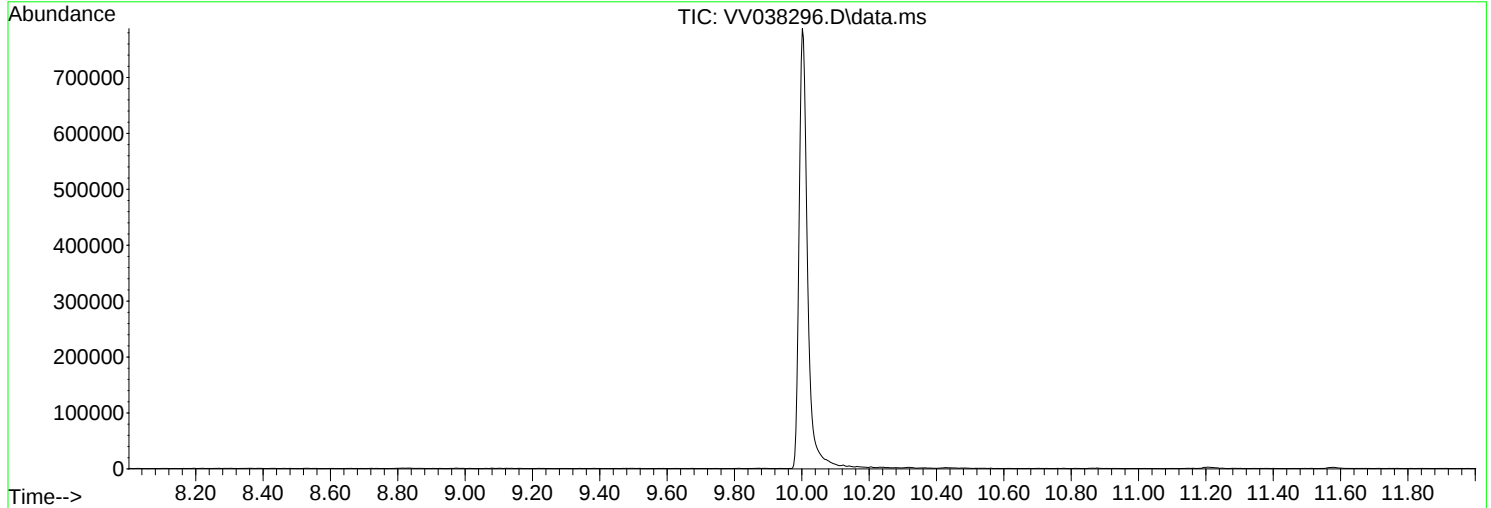

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	26000	PASS
75	95	30	80	49.3	76856	PASS
95	95	100	100	100.0	155819	PASS
96	95	5	9	6.7	10492	PASS
173	174	0.00	2	1.3	1707	PASS
174	95	50	120	82.0	127797	PASS
175	174	5	9	7.5	9635	PASS
176	174	95	105	95.4	121891	PASS
177	176	5	10	6.2	7559	PASS

m/z	Abundance
35.80	105.0
39.90	223.0
43.90	368.0
64.10	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB291

m/z	Abundance
36.00	1312.0
37.00	6447.0
38.00	5909.0
39.00	2668.0
39.90	509.0
40.50	256.0
41.20	109.0
42.90	126.0
44.00	1288.0
44.90	1255.0
46.20	263.0
47.00	1662.0
47.90	789.0
49.00	5794.0
50.00	25456.0
51.00	7771.0
51.90	497.0
53.00	348.0
53.80	204.0
54.80	472.0
56.00	2054.0
57.00	3707.0
58.00	105.0
60.00	1289.0
61.00	7163.0
62.00	6938.0
63.00	6567.0
64.00	1368.0
65.00	1161.0
66.00	135.0
66.90	348.0
68.00	14007.0
69.00	14048.0
70.00	1074.0
71.90	906.0
73.00	6578.0
74.00	24184.0
75.00	73912.0
76.00	6259.0
77.00	1154.0
77.90	781.0
78.90	6410.0
79.90	1682.0
80.90	7235.0
81.90	1494.0
82.90	150.0
85.80	279.0
87.00	6634.0
88.00	6750.0
90.90	626.0
92.00	4440.0
93.00	6548.0
94.00	18880.0
95.00	149504.0
96.00	10323.0
97.00	432.0
103.10	109.0
103.80	743.0
104.80	174.0
105.70	543.0
107.00	160.0
107.80	127.0
109.80	192.0
110.80	168.0
112.20	147.0
113.00	121.0
114.80	166.0
115.90	463.0
116.80	1304.0
117.90	669.0
118.90	998.0
123.70	113.0
125.90	140.0
127.80	407.0
128.90	215.0
129.80	466.0
130.70	235.0
134.90	334.0
136.70	106.0
137.10	126.0
140.00	100.0
140.80	1511.0
141.90	174.0
142.90	2553.0
143.90	187.0
145.00	1201.0
145.80	333.0
147.80	429.0
149.10	105.0
150.00	204.0
152.80	171.0
153.70	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB291

154.00	113.0
154.90	497.0
157.00	220.0
158.10	117.0
158.90	213.0
160.70	173.0
170.90	471.0
171.90	1424.0
173.00	1607.0
173.90	119840.0
175.00	9077.0
175.90	113616.0
176.90	7301.0
178.00	193.0

Instrument :
MSVOA_V
ClientSampleId :
BFB291

m/z	Abundance
36.00	1421.0
37.00	6088.0
38.00	6195.0
39.00	2833.0
39.90	463.0
40.40	308.0
41.10	107.0
42.90	143.0
44.00	1350.0
44.90	1225.0
46.10	260.0
46.90	1710.0
47.90	779.0
49.00	6081.0
50.00	26784.0
51.00	7688.0
52.00	486.0
53.00	407.0
53.90	172.0
54.80	381.0
56.00	2257.0
57.00	3836.0
58.10	149.0
60.00	1319.0
61.00	7500.0
62.00	7283.0
63.00	6954.0
64.00	1373.0
65.00	1489.0
66.00	163.0
66.90	363.0
68.00	15495.0
69.00	14740.0
70.00	1212.0
71.90	897.0
73.00	6911.0
74.00	26264.0
75.00	79608.0
76.00	6705.0
77.00	1205.0
77.90	854.0
78.90	6838.0
79.90	1896.0
80.90	7355.0
81.90	1652.0
82.90	117.0
85.90	296.0
87.00	7072.0
88.00	7170.0
90.80	682.0
92.00	4656.0
92.90	7424.0
94.00	19984.0
95.00	160768.0
96.00	10828.0
97.00	491.0
103.80	687.0
104.90	199.0
105.80	524.0
106.90	201.0
108.10	115.0
109.90	144.0
110.90	183.0
112.20	193.0
113.00	144.0
114.70	261.0
115.90	507.0
116.80	1295.0
117.90	762.0
118.90	1196.0
126.00	187.0
127.80	460.0
128.70	220.0
129.80	569.0
130.80	247.0
134.80	371.0
136.70	127.0
137.00	115.0
138.80	121.0
140.00	121.0
140.80	1687.0
141.80	184.0
142.90	3027.0
143.90	222.0
145.00	1299.0
145.80	381.0
147.80	487.0
149.00	113.0
150.00	211.0
152.10	135.0
152.90	171.0
153.70	123.0

Instrument :
MSVOA_V
ClientSampleId :
BFB291

154.90	570.0
156.80	294.0
158.00	121.0
158.90	237.0
160.70	185.0
170.20	190.0
171.00	566.0
171.90	1683.0
173.00	1737.0
173.90	132224.0
175.00	9970.0
175.90	125920.0
177.00	7829.0
178.00	180.0

Instrument :
MSVOA_V
ClientSampleId :
BFB291

m/z	Abundance
35.90	1346.0
37.00	5495.0
38.00	5758.0
39.00	2640.0
40.00	384.0
42.90	111.0
44.00	1290.0
44.90	1085.0
46.10	252.0
46.90	1794.0
47.90	753.0
49.00	5758.0
50.00	25760.0
51.00	7331.0
52.00	445.0
53.00	385.0
53.90	120.0
54.80	278.0
56.00	2245.0
57.00	3745.0
58.10	179.0
60.00	1360.0
61.00	7279.0
62.00	6925.0
63.00	6667.0
64.00	1334.0
65.00	1567.0
66.00	111.0
66.90	347.0
68.00	14924.0
69.00	14107.0
70.00	1190.0
71.90	847.0
73.00	6739.0
74.00	25984.0
75.00	77048.0
76.00	6592.0
76.90	1176.0
77.90	891.0
78.90	6531.0
79.90	1876.0
80.90	7005.0
81.90	1670.0
85.90	282.0
86.90	7001.0
88.00	6603.0
90.80	722.0
92.00	4326.0
92.90	7396.0
94.00	19288.0
95.00	157184.0
96.00	10324.0
97.00	442.0
103.80	657.0
104.90	237.0
105.90	563.0
106.90	238.0
108.10	120.0
110.00	128.0
110.90	161.0
112.10	219.0
112.90	193.0
114.70	295.0
115.90	583.0
116.90	1255.0
117.90	725.0
118.90	1262.0
126.00	153.0
127.90	486.0
128.80	250.0
129.90	615.0
130.90	222.0
134.90	329.0
136.70	184.0
140.00	159.0
140.80	1688.0
141.70	192.0
142.90	3093.0
143.90	229.0
144.90	1315.0
145.70	345.0
146.90	123.0
147.80	489.0
149.00	111.0
150.00	182.0
152.10	118.0
152.90	124.0
153.70	117.0
155.00	561.0
156.80	304.0
158.90	193.0
160.80	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB291

170.20	238.0
171.10	584.0
171.90	1775.0
173.00	1776.0
173.90	131328.0
175.00	9857.0
175.90	126136.0
177.00	7547.0
178.00	163.0

Instrument :
MSVOA_V
ClientSampleId :
BFB291