

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV112524\  
 Data File : VV038333.D  
 Acq On : 25 Nov 2024 10:46  
 Operator : SY/MD  
 Sample : VV1125WBL01  
 Misc : 25mL/MSVOA\_V/WATER  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 VBLK264

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR111924WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV038333.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.278       | 66            | 74          | 92           | rBV      | 100820         | 112644        | 14.87%          | 1.794%        |
| 2         | 1.532       | 145           | 153         | 169          | rBV      | 99514          | 119681        | 15.80%          | 1.906%        |
| 3         | 2.053       | 306           | 315         | 335          | rBV      | 188426         | 275813        | 36.40%          | 4.393%        |
| 4         | 3.825       | 852           | 866         | 906          | rBV2     | 51613          | 265065        | 34.99%          | 4.221%        |
| 5         | 4.239       | 980           | 995         | 1034         | rBV2     | 136056         | 369898        | 48.82%          | 5.891%        |
| 6         | 4.950       | 1202          | 1216        | 1252         | rBV3     | 285149         | 757650        | 100.00%         | 12.066%       |
| 7         | 5.529       | 1386          | 1396        | 1431         | rBV      | 230218         | 525359        | 69.34%          | 8.367%        |
| 8         | 5.982       | 1525          | 1537        | 1574         | rBV      | 174145         | 390839        | 51.59%          | 6.224%        |
| 9         | 6.915       | 1817          | 1827        | 1859         | rBV2     | 62765          | 146045        | 19.28%          | 2.326%        |
| 10        | 7.236       | 1916          | 1927        | 1958         | rBV      | 282098         | 547296        | 72.24%          | 8.716%        |
| 11        | 7.558       | 2018          | 2027        | 2053         | rBV      | 36507          | 78660         | 10.38%          | 1.253%        |
| 12        | 8.027       | 2163          | 2173        | 2221         | rBV2     | 239029         | 635643        | 83.90%          | 10.123%       |
| 13        | 8.779       | 2396          | 2407        | 2433         | rBV      | 396145         | 715993        | 94.50%          | 11.403%       |
| 14        | 10.146      | 2819          | 2832        | 2857         | rBV      | 141401         | 246519        | 32.54%          | 3.926%        |
| 15        | 11.178      | 3143          | 3153        | 3179         | rBV      | 344087         | 581464        | 76.75%          | 9.260%        |
| 16        | 11.554      | 3259          | 3270        | 3294         | rBV      | 294691         | 510513        | 67.38%          | 8.130%        |




Sum of corrected areas: 6279082

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV112524\  
Data File : VV038333.D  
Acq On : 25 Nov 2024 10:46  
Operator : SY/MD  
Sample : VV1125WBL01  
Misc : 25mL/MSVOA\_V/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR111924WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

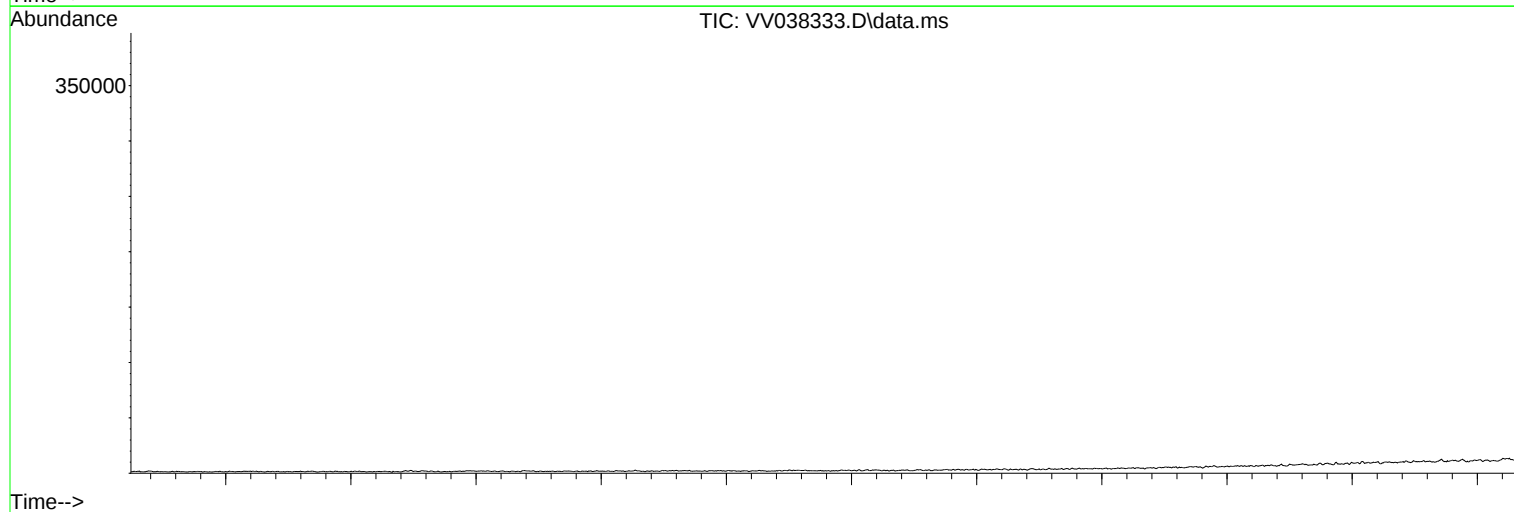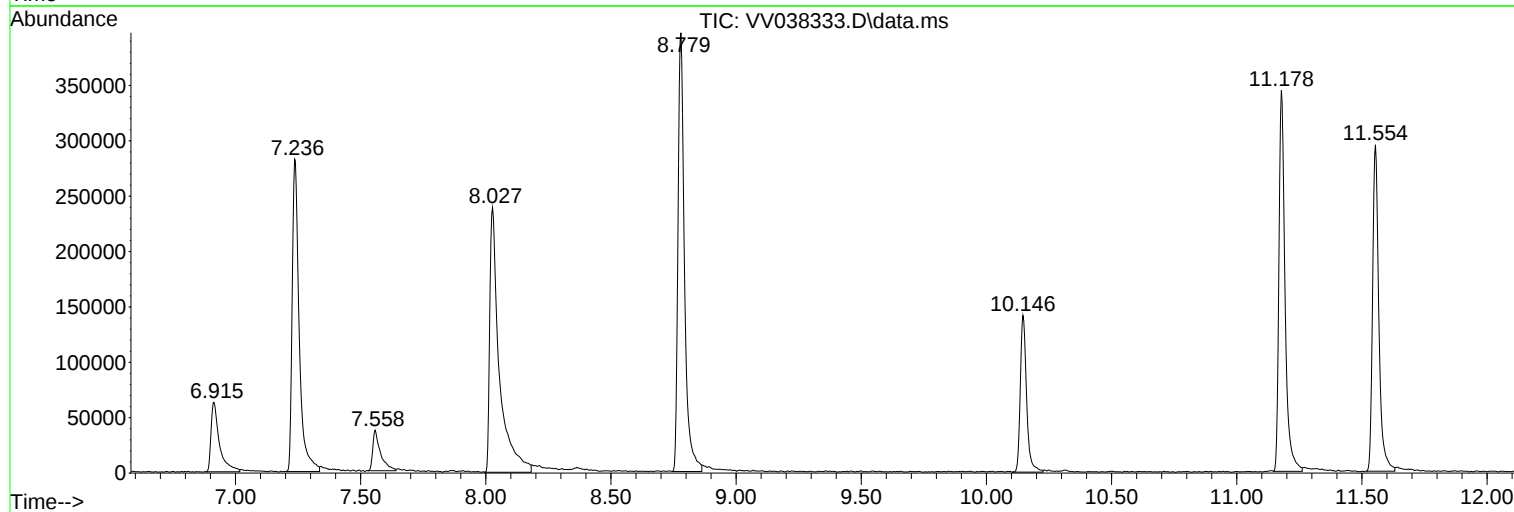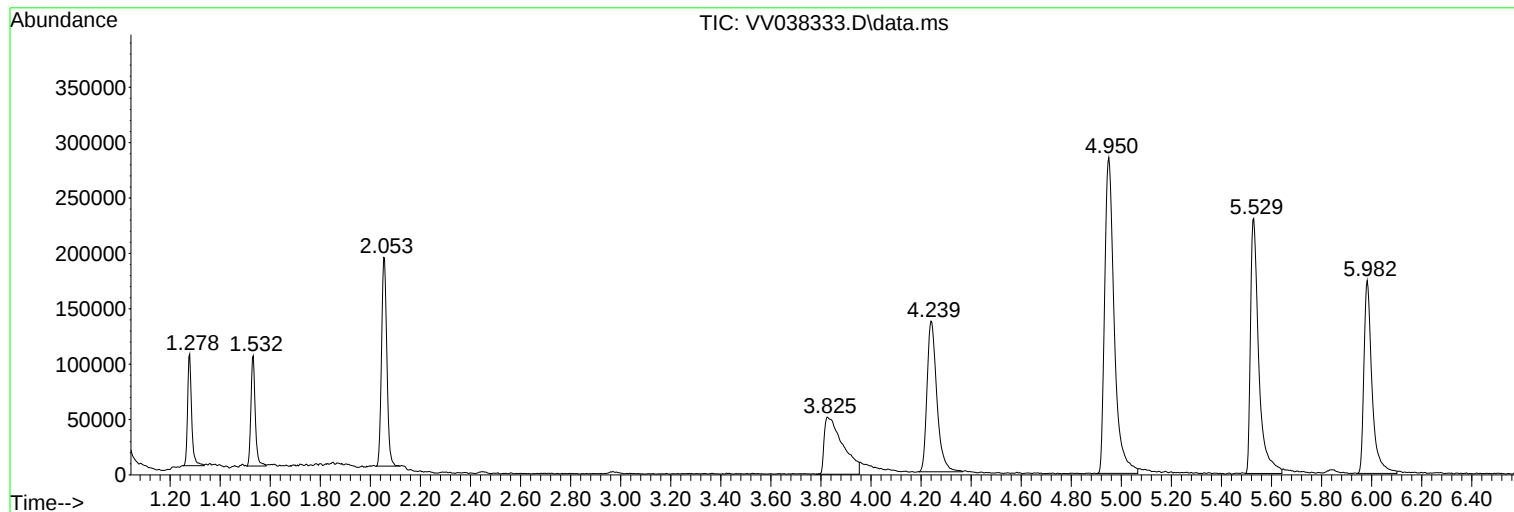

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV112524\  
Data File : VV038333.D  
Acq On : 25 Nov 2024 10:46  
Operator : SY/MD  
Sample : VV1125WBL01  
Misc : 25mL/MSVOA\_V/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR111924WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV112524\  
Data File : VV038333.D  
Acq On : 25 Nov 2024 10:46  
Operator : SY/MD  
Sample : VV1125WBL01  
Misc : 25mL/MSVOA\_V/WATER  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR111924WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       | #        | RT Resp Conc          |