

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112524\
 Data File : VV038350.D
 Acq On : 25 Nov 2024 18:05
 Operator : SY/MD
 Sample : P4930-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG443

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038350.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	16	22	33	rVB	39438	45963	4.98%	0.537%
2	1.275	66	73	85	rBV2	88120	97712	10.59%	1.142%
3	1.529	144	152	163	rBV	87442	105581	11.45%	1.234%
4	1.664	187	194	204	rVB	20264	27924	3.03%	0.326%
5	1.864	242	256	283	rBV	280983	922269	100.00%	10.779%
6	2.053	306	315	329	rVB2	156934	233693	25.34%	2.731%
7	2.243	363	374	402	rBV	44609	125445	13.60%	1.466%
8	2.442	426	436	450	rVB2	15217	25282	2.74%	0.295%
9	2.700	507	516	531	rVB6	9375	18906	2.05%	0.221%
10	3.796	845	857	897	rBV3	129849	487454	52.85%	5.697%
11	4.240	980	995	1025	rBV2	131486	355896	38.59%	4.159%
12	4.503	1068	1077	1096	rVB5	10517	25835	2.80%	0.302%
13	4.950	1202	1216	1243	rBV2	270146	720974	78.17%	8.426%
14	5.529	1386	1396	1429	rBV2	222432	501947	54.43%	5.866%
15	5.825	1474	1488	1524	rBV	345857	747985	81.10%	8.742%
16	5.982	1526	1537	1565	rVV2	173349	373714	40.52%	4.368%
17	6.915	1817	1827	1856	rBV2	60263	136831	14.84%	1.599%
18	7.240	1918	1928	1950	rBV	252139	483912	52.47%	5.656%
19	7.558	2018	2027	2050	rBV	36274	82720	8.97%	0.967%
20	7.902	2113	2134	2154	rBV3	55834	114422	12.41%	1.337%
21	8.021	2162	2171	2218	rBV	368705	844334	91.55%	9.868%
22	8.780	2396	2407	2448	rBV	395822	728706	79.01%	8.517%
23	10.146	2819	2832	2857	rBV	157375	269375	29.21%	3.148%
24	10.317	2878	2885	2894	rBV3	9534	15102	1.64%	0.177%
25	11.178	3143	3153	3177	rBV	329257	568568	61.65%	6.645%
26	11.554	3256	3270	3292	rBV	288184	495728	53.75%	5.794%




Sum of corrected areas: 8556278

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112524\
Data File : VV038350.D
Acq On : 25 Nov 2024 18:05
Operator : SY/MD
Sample : P4930-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG443

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

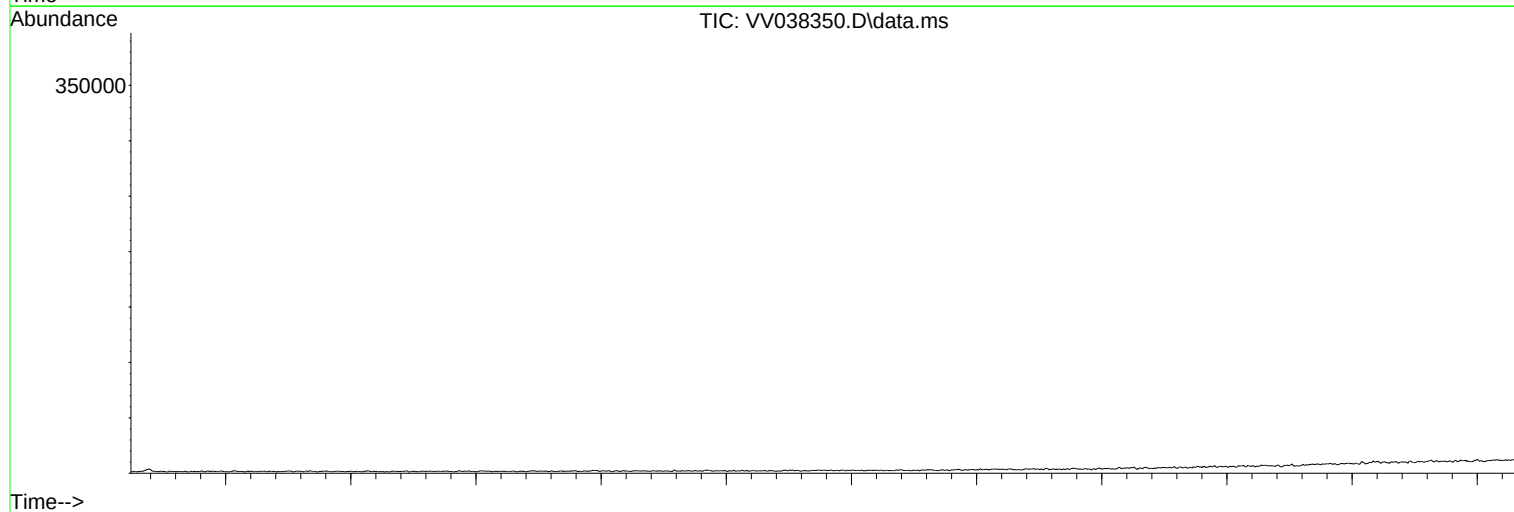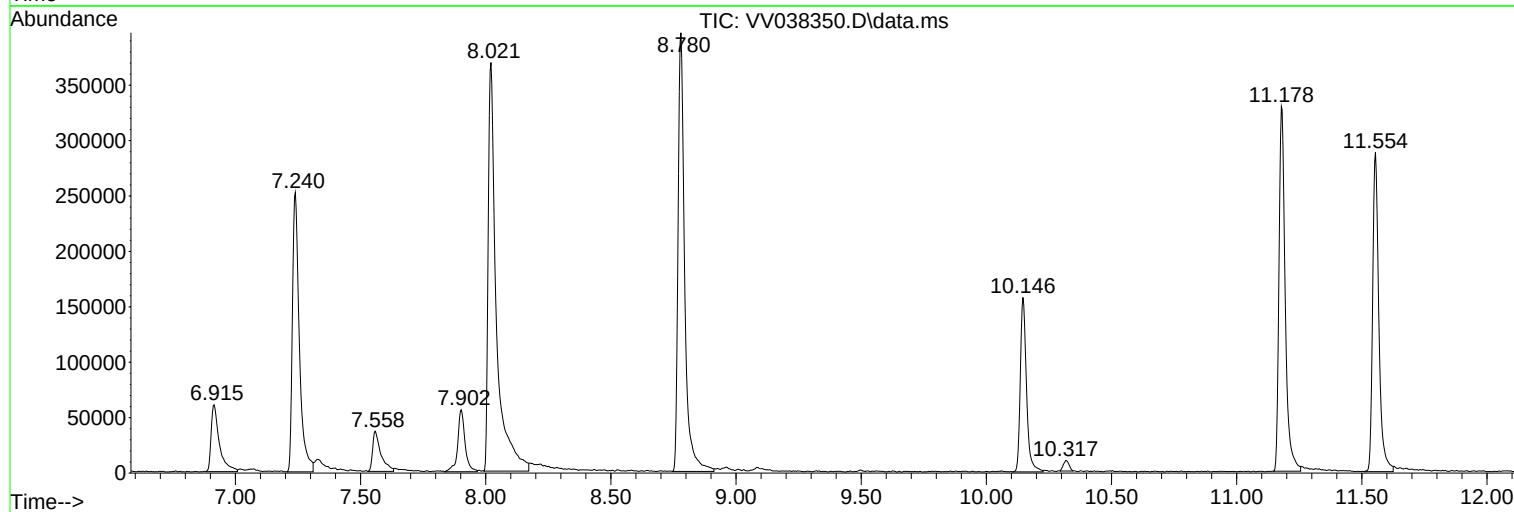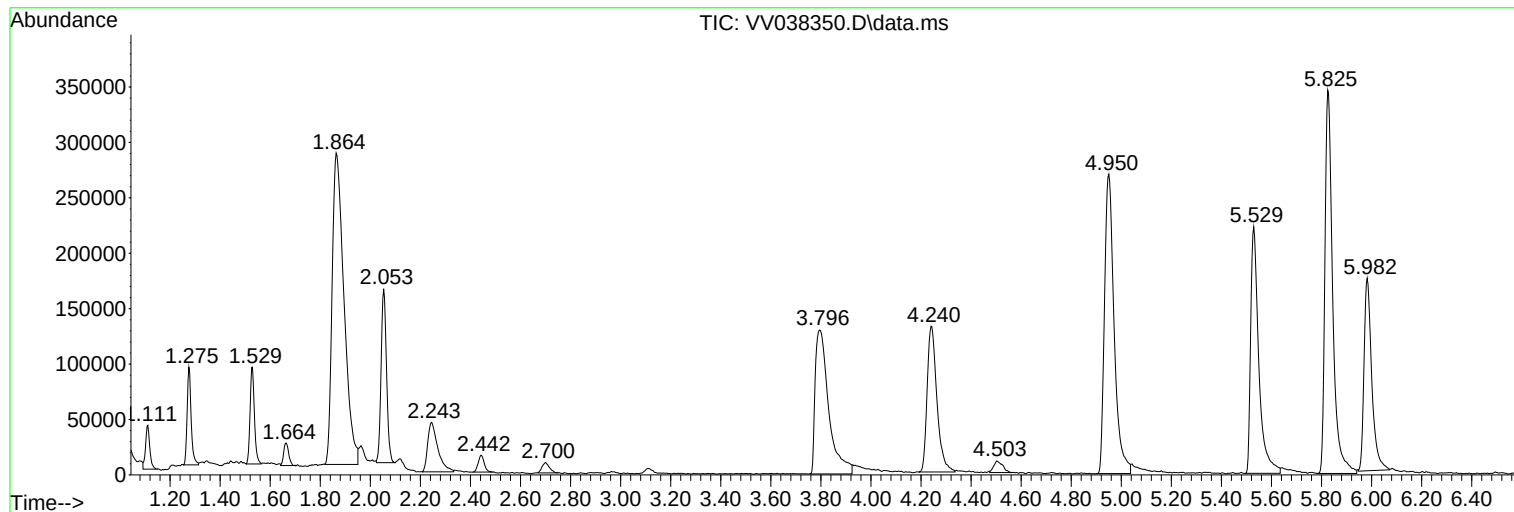

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112524\
Data File : VV038350.D
Acq On : 25 Nov 2024 18:05
Operator : SY/MD
Sample : P4930-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG443

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112524\
Data File : VV038350.D
Acq On : 25 Nov 2024 18:05
Operator : SY/MD
Sample : P4930-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG443

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc