

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112524\
 Data File : VV038352.D
 Acq On : 25 Nov 2024 18:53
 Operator : SY/MD
 Sample : P4930-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG447

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038352.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	47	54	61	rBV2	5299	9274	1.19%	0.146%
2	1.275	66	73	84	rVV	75477	83441	10.73%	1.312%
3	1.426	110	120	125	rBV7	7136	12843	1.65%	0.202%
4	1.529	144	152	162	rBV	87899	103047	13.25%	1.621%
5	1.844	240	250	265	rBV	17589	35272	4.54%	0.555%
6	1.963	279	287	301	rVV	27162	42283	5.44%	0.665%
7	2.053	304	315	325	rVV	147588	217884	28.02%	3.427%
8	2.111	325	333	356	rVB	57832	104571	13.45%	1.645%
9	2.227	357	369	393	rBV	63181	124848	16.06%	1.964%
10	2.568	464	475	490	rBV3	8090	19374	2.49%	0.305%
11	3.783	845	853	885	rBV	100462	309741	39.83%	4.872%
12	4.240	981	995	1020	rBV	131100	345250	44.40%	5.431%
13	4.950	1203	1216	1251	rBV2	257361	693793	89.22%	10.913%
14	5.529	1382	1396	1423	rBV	208581	472002	60.70%	7.424%
15	5.847	1478	1495	1502	rBV	8226	19464	2.50%	0.306%
16	5.982	1526	1537	1566	rBV2	164016	358662	46.12%	5.642%
17	6.915	1818	1827	1858	rBV2	57880	132821	17.08%	2.089%
18	7.239	1917	1928	1952	rBV	241381	458148	58.92%	7.206%
19	7.558	2018	2027	2047	rBV2	34266	75778	9.75%	1.192%
20	7.908	2128	2136	2150	rVB6	7194	14804	1.90%	0.233%
21	8.018	2161	2170	2206	rBV	343896	777607	100.00%	12.231%
22	8.780	2394	2407	2436	rBV	376539	673026	86.55%	10.586%
23	10.146	2820	2832	2850	rBV	150054	249917	32.14%	3.931%
24	10.320	2874	2886	2894	rVB4	6716	10218	1.31%	0.161%
25	11.178	3143	3153	3177	rBV	316483	540546	69.51%	8.502%
26	11.554	3259	3270	3294	rBV	272579	472937	60.82%	7.439%

Sum of corrected areas: 6357551




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112524\
Data File : VV038352.D
Acq On : 25 Nov 2024 18:53
Operator : SY/MD
Sample : P4930-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG447

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

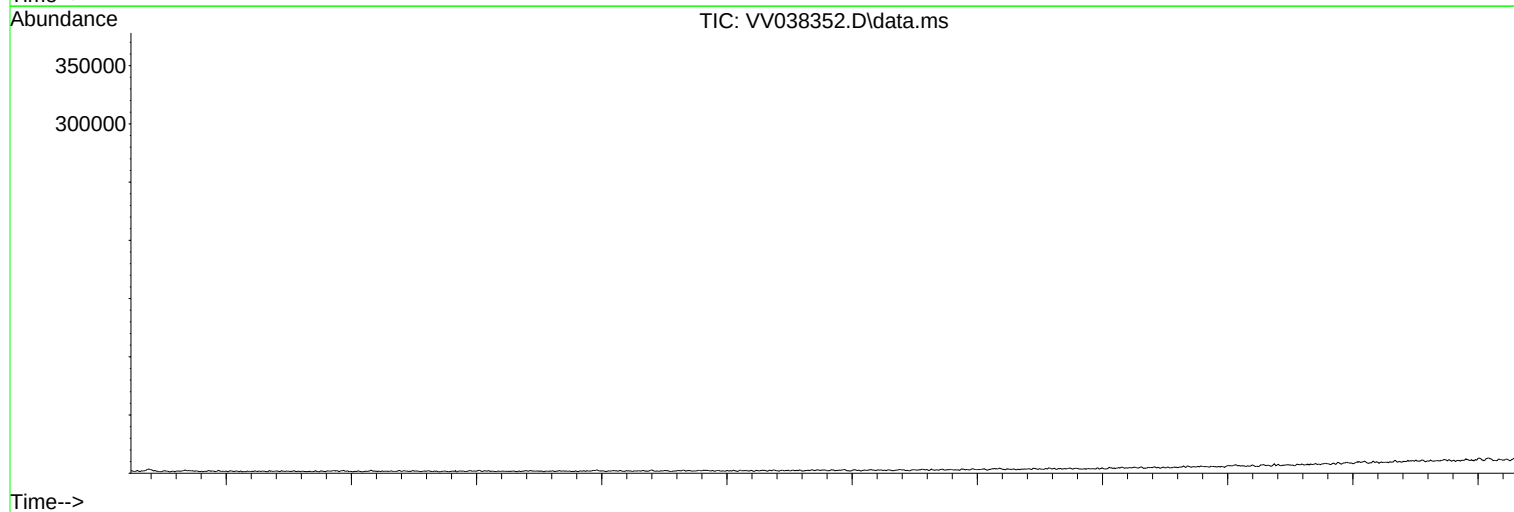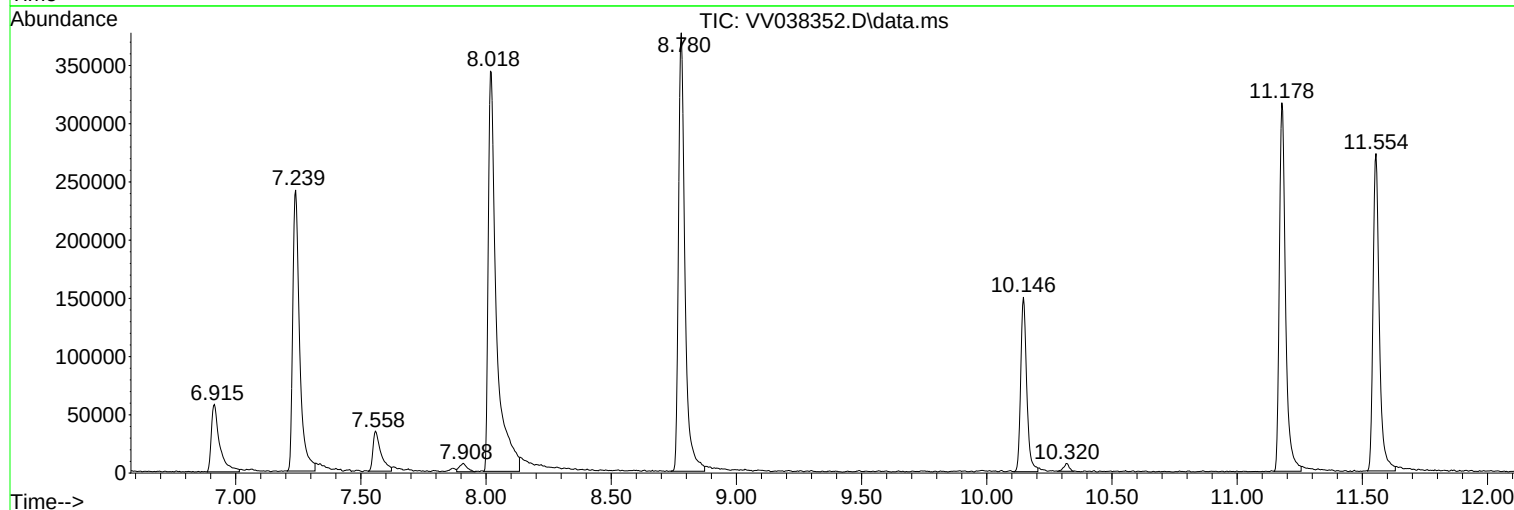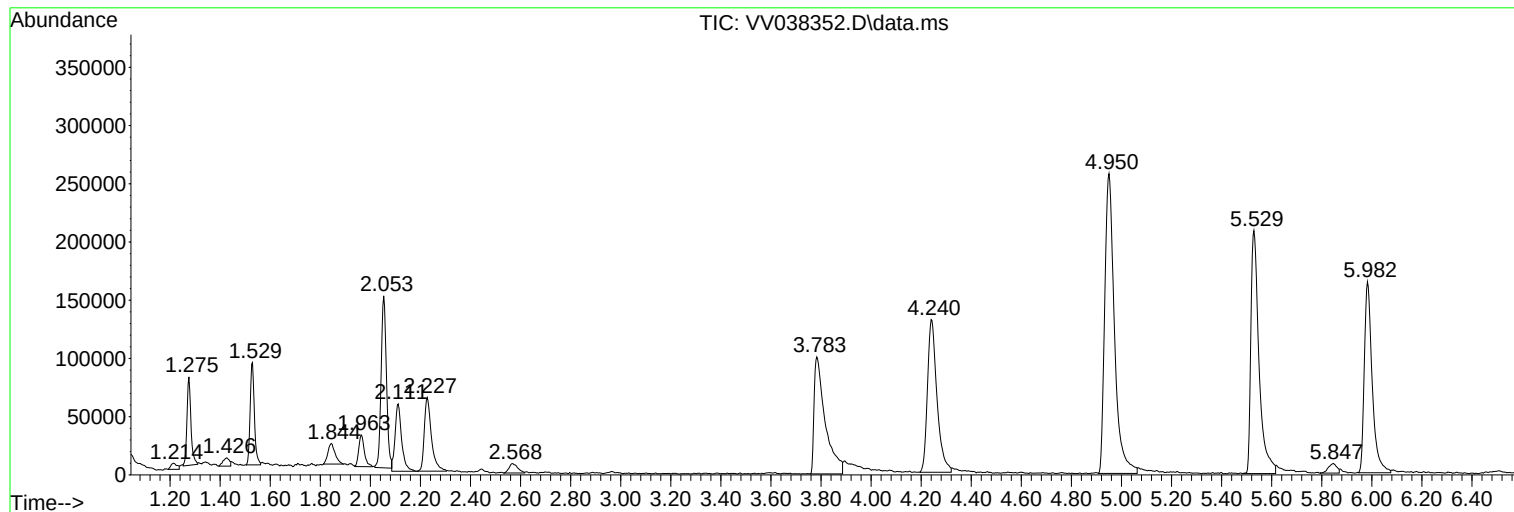

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112524\
Data File : VV038352.D
Acq On : 25 Nov 2024 18:53
Operator : SY/MD
Sample : P4930-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG447

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0










TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.227	1.32 ug/L	124848	1,4-Difluorobenzene	5.529

Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2	Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol	60	C3H8O	000067-63-0	72
4	Isopropyl Alcohol	60	C3H8O	000067-63-0	64
5	Isopropyl Alcohol	60	C3H8O	000067-63-0	56

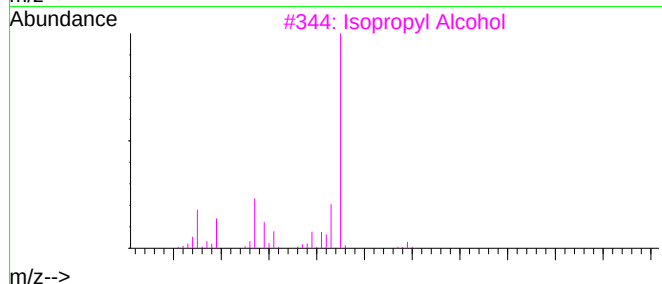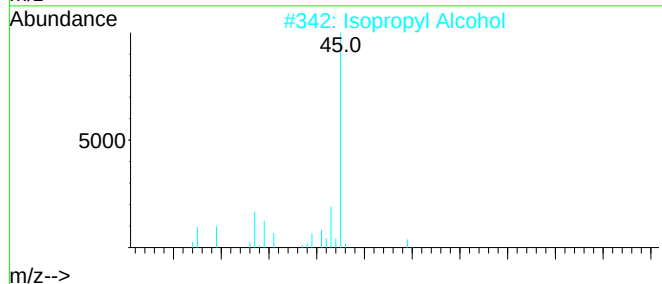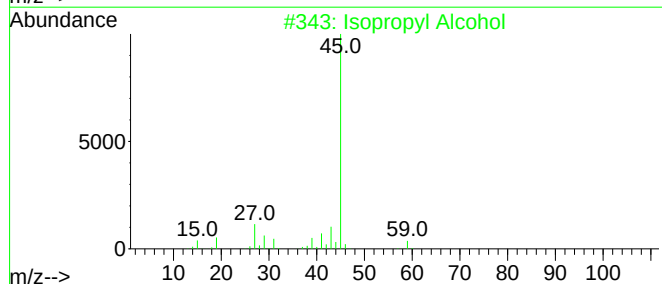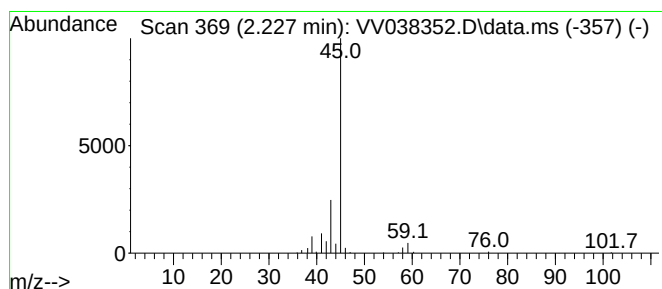

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112524\
Data File : VV038352.D
Acq On : 25 Nov 2024 18:53
Operator : SY/MD
Sample : P4930-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG447

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.227	1.3	ug/L	124848	1	5.529	472002	5.0