
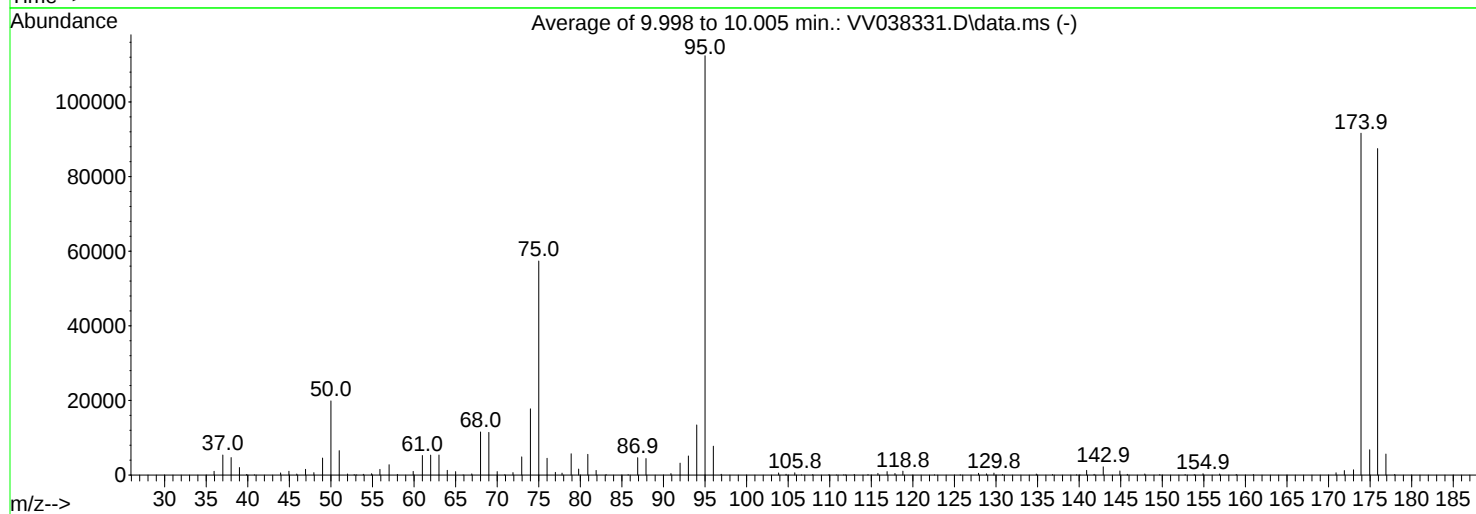


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112524\
Data File : VV038331.D
Acq On : 25 Nov 2024 07:59
Operator : SY/MD
Sample : BFB293
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB293

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Nov 26 00:39:03 2024

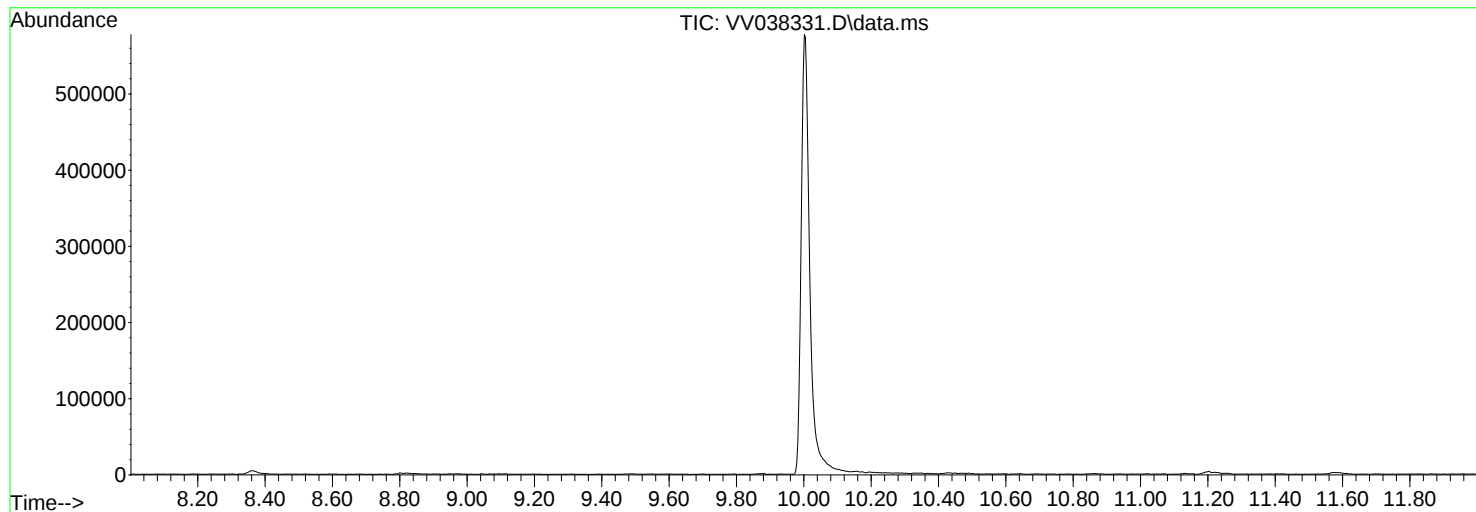

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	19883	PASS
75	95	30	80	51.0	57373	PASS
95	95	100	100	100.0	112392	PASS
96	95	5	9	6.9	7747	PASS
173	174	0.00	2	1.6	1423	PASS
174	95	50	120	81.5	91632	PASS
175	174	5	9	7.4	6784	PASS
176	174	95	105	95.5	87504	PASS
177	176	5	10	6.4	5638	PASS

m/z	Abundance
35.80	102.0
39.80	380.0
43.90	456.0

Instrument :
MSVOA_V
ClientSampleId :
BFB293

m/z	Abundance
36.00	1031.0
37.00	5093.0
38.00	4505.0
39.00	2019.0
39.90	518.0
40.80	111.0
44.00	969.0
45.00	1077.0
45.90	353.0
47.00	1455.0
47.90	690.0
49.00	4222.0
50.00	19304.0
51.00	6166.0
52.00	298.0
53.10	173.0
53.80	205.0
54.90	323.0
55.90	1524.0
57.00	2733.0
58.00	170.0
59.90	879.0
61.00	5011.0
62.00	5070.0
63.00	5428.0
64.00	1244.0
65.00	841.0
66.90	377.0
68.00	11151.0
69.00	10959.0
70.00	817.0
71.90	607.0
72.90	4688.0
74.00	16784.0
75.00	54504.0
76.00	4382.0
77.00	617.0
77.80	495.0
78.90	5296.0
79.80	1313.0
80.90	5413.0
81.90	1138.0
83.20	156.0
86.90	4572.0
87.90	4175.0
90.90	371.0
92.00	3092.0
93.00	4773.0
94.00	12578.0
95.00	106456.0
96.00	7668.0
96.90	192.0
103.90	521.0
104.90	195.0
105.80	592.0
108.00	107.0
111.70	134.0
112.90	178.0
114.50	127.0
115.80	487.0
116.90	842.0
117.90	420.0
118.80	970.0
122.60	103.0
127.90	461.0
128.80	268.0
129.80	535.0
130.80	123.0
134.90	273.0
136.90	125.0
140.10	130.0
140.90	1176.0
141.80	117.0
142.90	1915.0
144.90	1115.0
145.90	205.0
147.80	246.0
149.70	189.0
152.70	127.0
153.90	123.0
154.90	291.0
156.90	296.0
158.90	137.0
160.90	127.0
170.90	549.0
171.90	972.0
173.00	1300.0
173.90	84344.0
175.00	6436.0
175.90	81488.0
176.90	5320.0
178.10	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB293

m/z	Abundance
36.00	1178.0
37.00	5640.0
38.00	4881.0
39.00	2095.0
39.90	533.0
40.80	114.0
44.00	1040.0
44.90	1065.0
45.90	296.0
46.90	1596.0
48.00	674.0
49.00	4713.0
50.00	20336.0
51.00	6799.0
52.00	290.0
52.80	185.0
53.90	224.0
54.90	387.0
55.90	1555.0
57.00	2896.0
58.00	189.0
59.90	1003.0
61.00	5332.0
62.00	5507.0
63.00	5613.0
64.00	1351.0
65.00	944.0
66.90	315.0
68.00	12074.0
69.00	11940.0
70.00	1005.0
70.90	121.0
71.90	707.0
73.00	4901.0
74.00	18264.0
75.00	59288.0
76.00	4656.0
77.00	792.0
77.80	562.0
78.90	5882.0
79.80	1662.0
80.90	5721.0
81.90	1320.0
83.10	134.0
85.70	162.0
86.90	4803.0
87.90	4441.0
90.90	407.0
92.00	3267.0
93.00	5238.0
94.00	13766.0
95.00	115464.0
96.00	8059.0
96.90	226.0
103.90	598.0
104.70	256.0
105.80	655.0
108.00	124.0
109.90	120.0
111.70	129.0
112.90	185.0
114.60	166.0
115.80	435.0
116.90	950.0
117.80	419.0
118.80	1110.0
122.60	115.0
125.70	121.0
127.90	498.0
128.90	351.0
129.80	554.0
130.80	142.0
134.90	305.0
136.80	126.0
139.70	114.0
140.90	1304.0
141.80	229.0
142.90	2271.0
144.90	1158.0
145.80	211.0
147.90	317.0
149.70	171.0
152.70	159.0
153.80	118.0
154.90	397.0
156.90	285.0
158.90	178.0
160.90	167.0
170.90	675.0
171.90	1287.0
173.00	1506.0
173.90	95088.0

Instrument :
MSVOA_V
ClientSampleId :
BFB293

175.00	7006.0
175.90	90360.0
176.90	5836.0
177.90	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB293

m/z	Abundance
36.00	1143.0
37.00	5418.0
38.00	4703.0
39.00	1933.0
40.00	525.0
44.00	1095.0
44.90	976.0
45.90	220.0
46.90	1600.0
48.00	623.0
49.00	4761.0
50.00	20008.0
51.00	6694.0
52.00	299.0
52.80	186.0
54.00	218.0
54.90	419.0
55.90	1511.0
57.00	2708.0
58.00	178.0
59.90	1110.0
61.00	5392.0
62.00	5498.0
63.00	5089.0
64.00	1248.0
65.00	987.0
65.90	109.0
67.00	255.0
68.00	11437.0
69.00	11426.0
70.00	1002.0
70.90	131.0
71.90	705.0
73.00	5045.0
74.00	18200.0
75.00	58328.0
76.00	4494.0
77.00	808.0
77.80	533.0
78.90	5956.0
79.80	1841.0
80.90	5552.0
81.90	1297.0
83.00	109.0
85.80	179.0
86.90	4603.0
87.90	4680.0
90.90	442.0
92.00	3242.0
93.00	5341.0
94.00	13962.0
95.00	115256.0
96.00	7514.0
97.00	257.0
103.80	598.0
104.70	255.0
105.80	633.0
106.60	111.0
107.90	139.0
109.90	114.0
110.80	158.0
111.90	131.0
113.00	157.0
114.70	174.0
115.80	433.0
116.90	1030.0
117.80	425.0
118.80	1102.0
125.70	127.0
127.90	460.0
128.90	380.0
129.70	547.0
130.80	159.0
134.80	265.0
136.70	169.0
139.70	150.0
140.90	1307.0
141.80	273.0
142.90	2470.0
144.90	1039.0
145.70	216.0
148.00	321.0
149.70	109.0
152.80	138.0
153.80	105.0
154.90	437.0
156.90	265.0
158.90	182.0
161.00	158.0
170.90	655.0
171.90	1399.0
173.00	1463.0

Instrument :
MSVOA_V
ClientSampleId :
BFB293

173.90	95464.0
174.90	6911.0
175.90	90664.0
176.90	5757.0
177.80	162.0

Instrument :
MSVOA_V
ClientSampleId :
BFB293