

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112624\
 Data File : VV038369.D
 Acq On : 26 Nov 2024 17:05
 Operator : SY/MD
 Sample : P4930-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG445

Quant Time: Nov 27 00:24:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 27 00:19:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	206564	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	223272	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	90258	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	58790	3.713	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.200%
7) Chloroethane-d5	1.529	69	64171	5.011	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.200%
11) 1,1-Dichloroethene-d2	2.053	65	29396	4.314	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.200%
20) 2-Butanone-d5	3.780	46	241645	76.294	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	152.580%#
24) Chloroform-d	4.243	84	179582	5.844	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	116.800%
26) 1,2-Dichloroethane-d4	4.937	65	93109	6.753	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	135.000%#
32) Benzene-d6	4.953	84	299773	5.195	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.800%
36) 1,2-Dichloropropane-d6	5.982	67	106580	6.002	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	120.000%
41) Toluene-d8	7.239	98	219874	4.118	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.400%
43) trans-1,3-Dichloroprop...	7.558	79	34069	5.161	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	103.200%
46) 2-Hexanone-d5	8.018	63	172739	67.312	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	134.620%#
56) 1,1,2,2-Tetrachloroeth...	10.146	84	96899	6.428	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	128.600%#
66) 1,2-Dichlorobenzene-d4	11.554	152	92426	6.010	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	120.200%#
Target Compounds				Qvalue		
2) Dichlorodifluoromethane	1.105	85	21924	1.122	ug/L	99
5) Vinyl chloride	1.278	62	9600	0.503	ug/L	92
10) 1,1,2-Trichloro-1,2,2-...	2.060	101	5513	0.356	ug/L #	65
12) 1,1-Dichloroethene	2.063	96	903899	61.266	ug/L #	67
16) Methylene chloride	2.442	84	5809	0.345	ug/L	83
17) Methyl tert-butyl Ether	2.699	73	35975	1.078	ug/L	94
18) trans-1,2-Dichloroethene	2.696	96	4357	0.280	ug/L	98
19) 1,1-Dichloroethane	3.101	63	451257	15.995	ug/L	99
22) cis-1,2-Dichloroethene	3.802	96	284670	17.713	ug/L	98
25) Chloroform	4.272	83	8084	0.268	ug/L	80
29) 1,1,1-Trichloroethane	4.503	97	341500	12.753	ug/L	98
34) Trichloroethene	5.821	95	363733	21.275	ug/L	99
47) Tetrachloroethene	7.899	164	63395	4.615	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112624\
Data File : VV038369.D
Acq On : 26 Nov 2024 17:05
Operator : SY/MD
Sample : P4930-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG445

Quant Time: Nov 27 00:24:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 27 00:19:46 2024
Response via : Initial Calibration




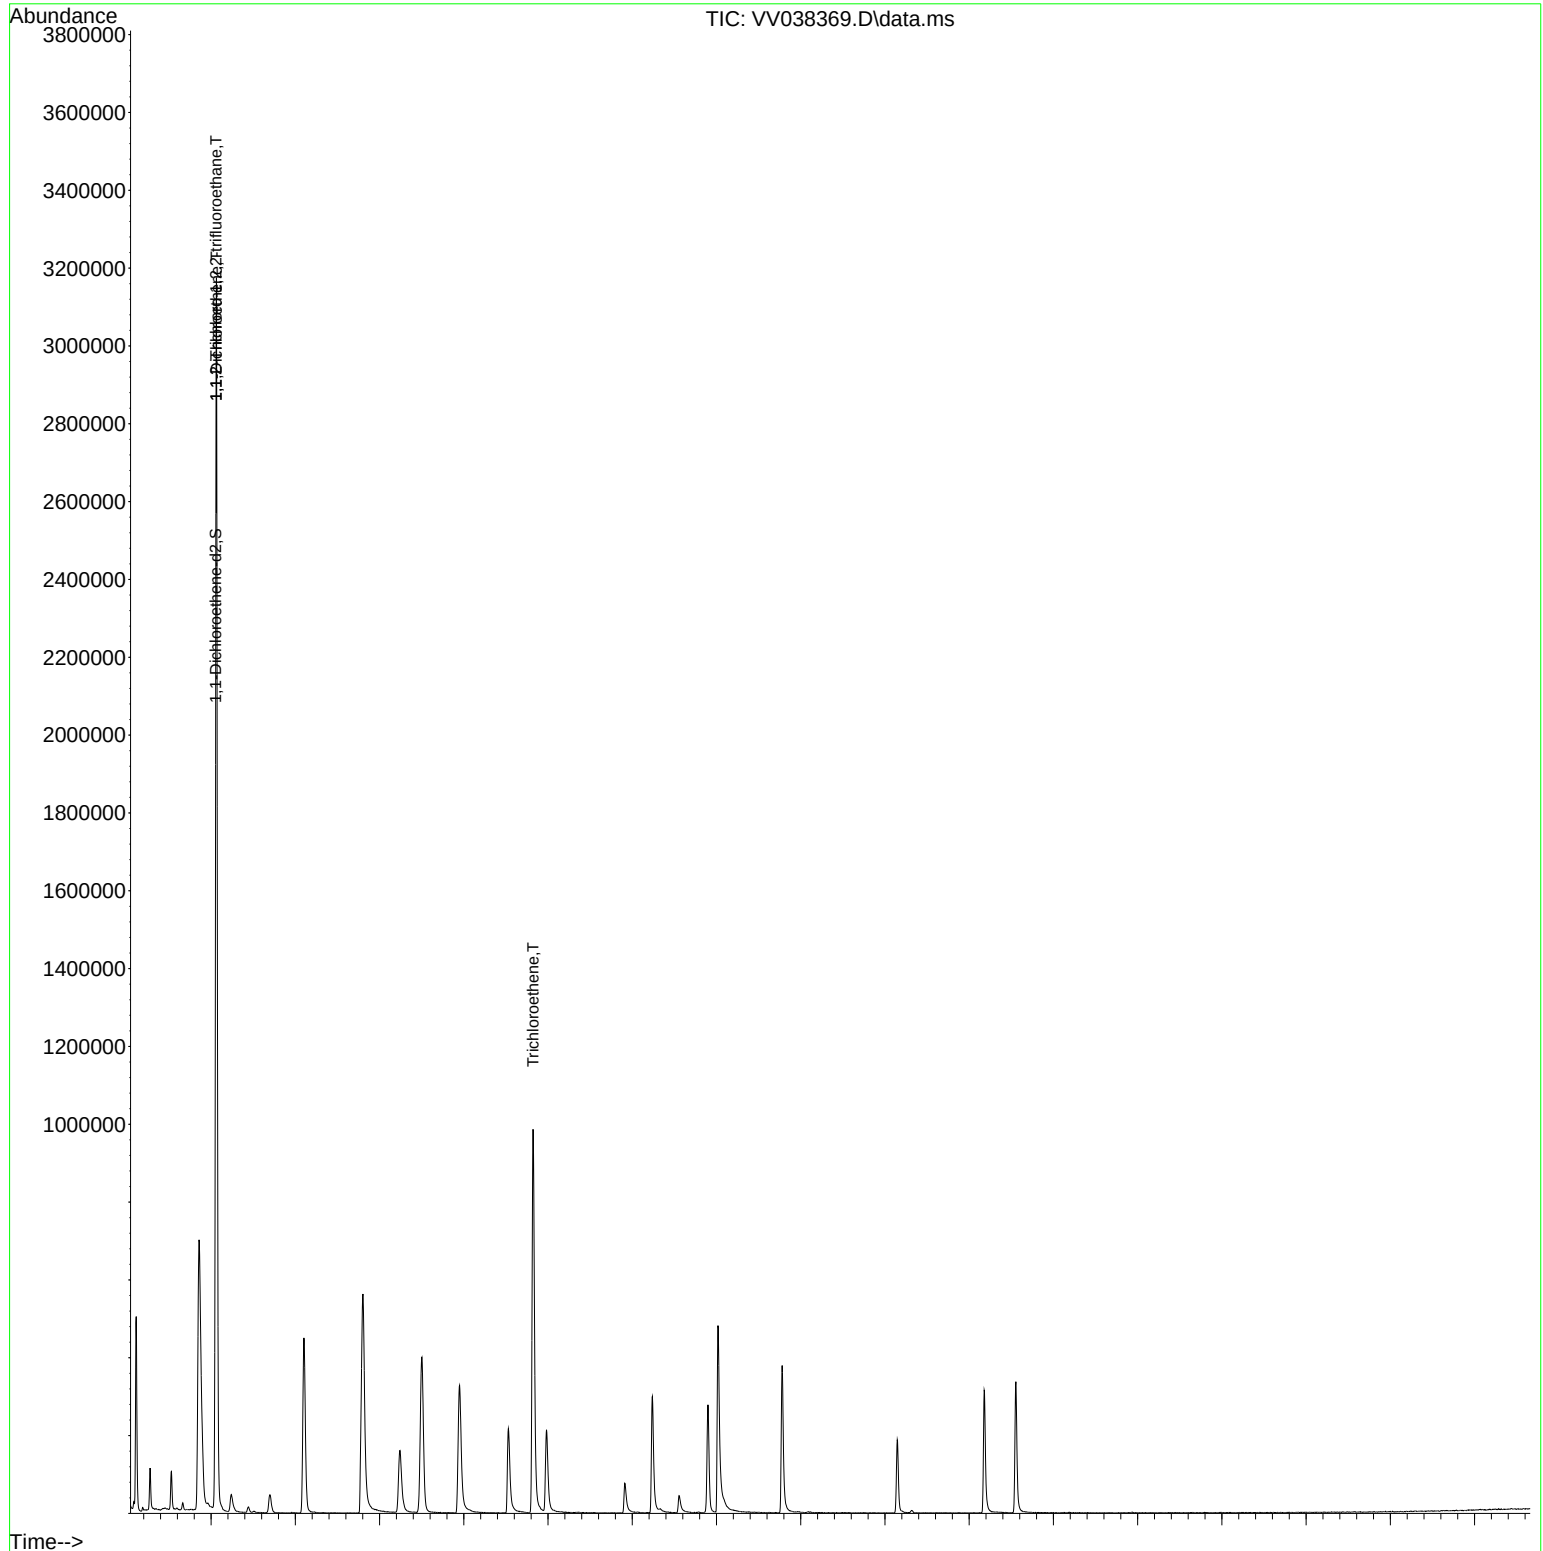


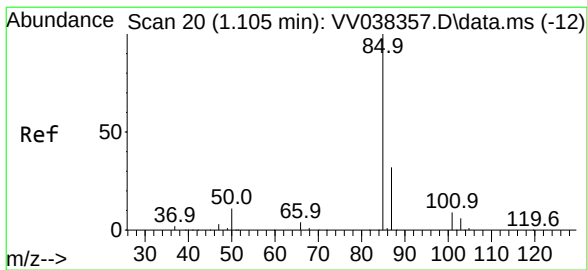

#2
 Dichlorodifluoromethane
 Concen: 1.122 ug/L
 RT: 1.105 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: VV038369.D
 Acq: 26 Nov 2024 17:05




Instrument :
 MSVOA_V
 ClientSampleId :
 BG445


Tgt Ion: 85 Resp: 21924
 Ion Ratio Lower Upper
 85 100
 87 32.3 26.5 39.7

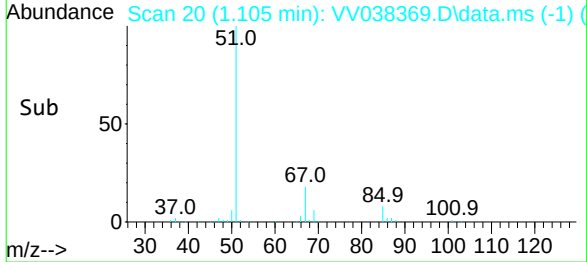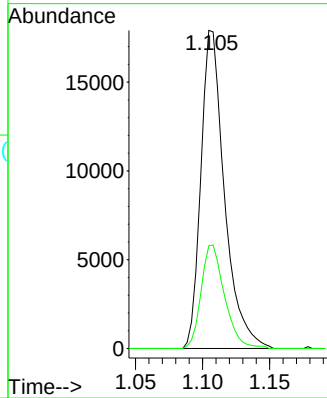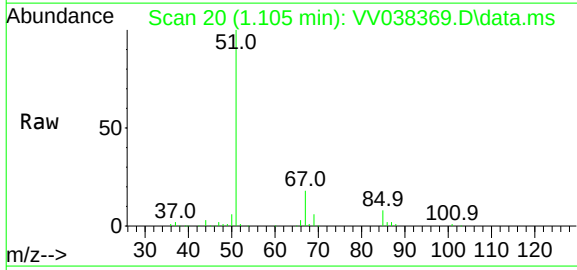

#5
 Vinyl chloride
 Concen: 0.503 ug/L
 RT: 1.278 min Scan# 74
 Delta R.T. -0.003 min
 Lab File: VV038369.D
 Acq: 26 Nov 2024 17:05

Tgt Ion: 62 Resp: 9600
 Ion Ratio Lower Upper
 62 100
 64 39.7 24.4 45.4


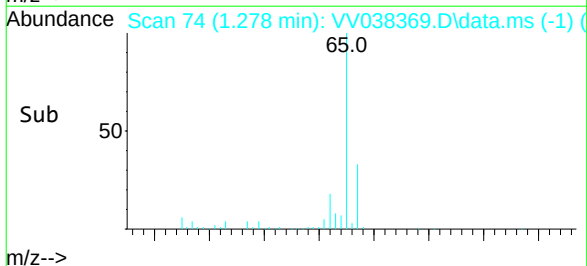
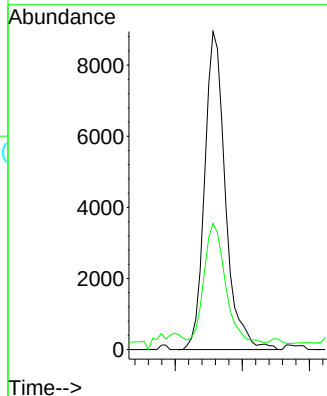
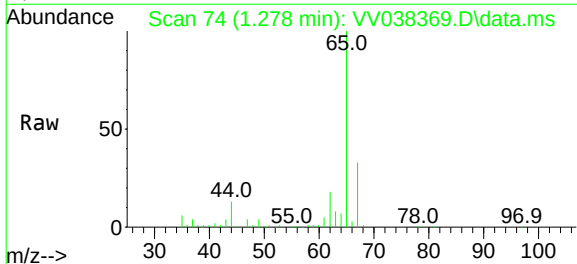




#10
1,1,2-Trichloro-1,2,2-trifluoroethane
Concen: 0.356 ug/L
RT: 2.060 min Scan# 317
Delta R.T. -0.003 min
Lab File: VV038369.D
Acq: 26 Nov 2024 17:05




Instrument :
MSVOA_V
ClientSampleId :
BG445


Tgt Ion: 101 Resp: 5513
Ion Ratio Lower Upper
101 100
85 34.5 33.4 50.0
151 33.1 58.8 88.2#

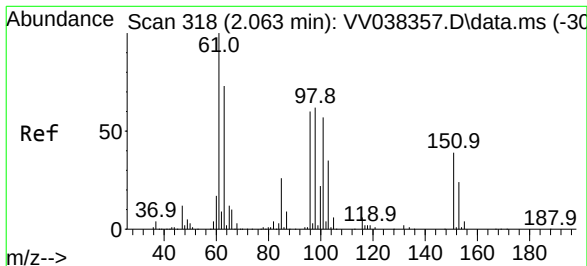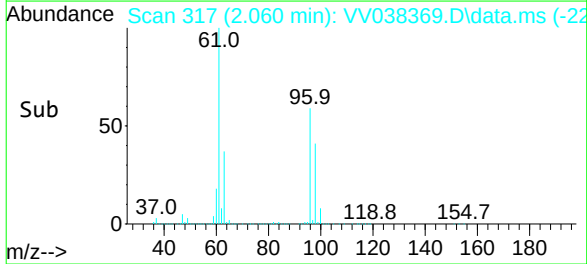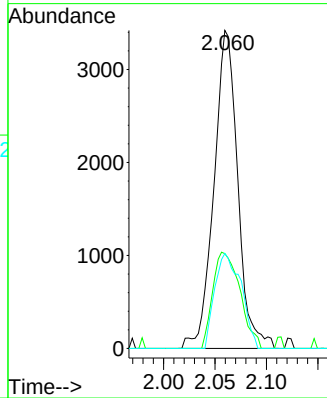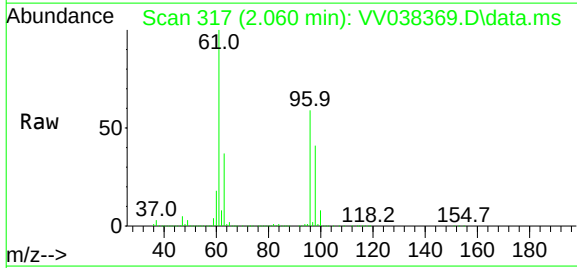

#12
1,1-Dichloroethene
Concen: 61.266 ug/L
RT: 2.063 min Scan# 318
Delta R.T. -0.000 min
Lab File: VV038369.D
Acq: 26 Nov 2024 17:05


Tgt Ion: 96 Resp: 903899
Ion Ratio Lower Upper
96 100
61 165.8 115.7 214.9
63 58.4 101.1 187.7#

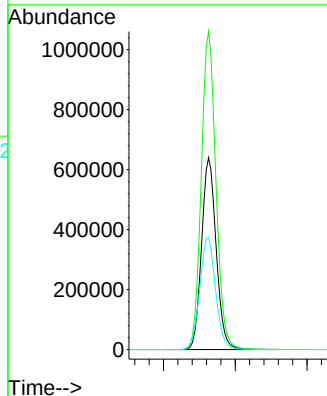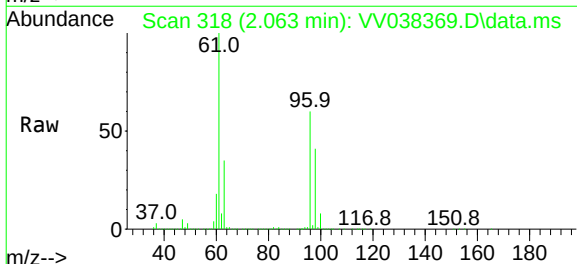






#16
Methylene chloride
Concen: 0.345 ug/L
RT: 2.442 min Scan# 43
Delta R.T. 0.003 min
Lab File: VV038369.D
Acq: 26 Nov 2024 17:05

Instrument :
MSVOA_V
ClientSampleId :
BG445



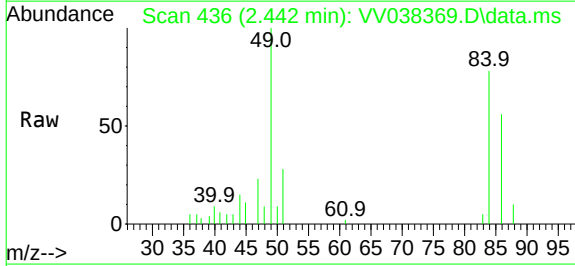



Tgt Ion: 84 Resp: 5809
Ion Ratio Lower Upper
84 100
86 72.0 44.2 82.2
49 127.7 74.9 139.1

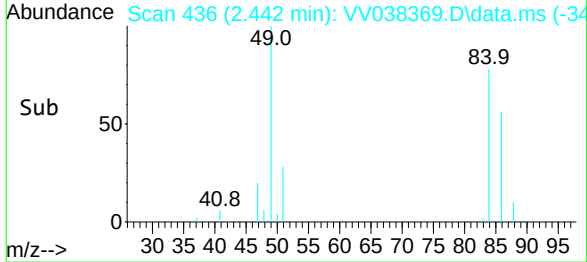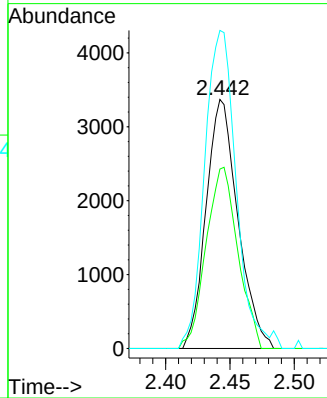

#17
Methyl tert-butyl Ether
Concen: 1.078 ug/L
RT: 2.699 min Scan# 516
Delta R.T. 0.003 min
Lab File: VV038369.D
Acq: 26 Nov 2024 17:05

Tgt Ion: 73 Resp: 35975
Ion Ratio Lower Upper
73 100
43 20.1 14.2 21.2
57 24.7 17.6 26.4

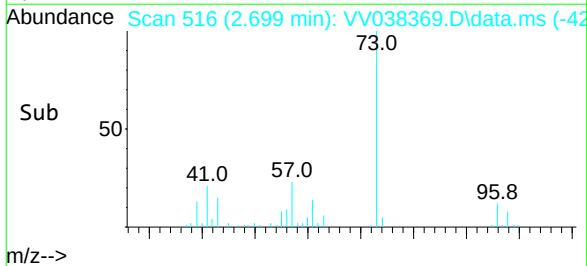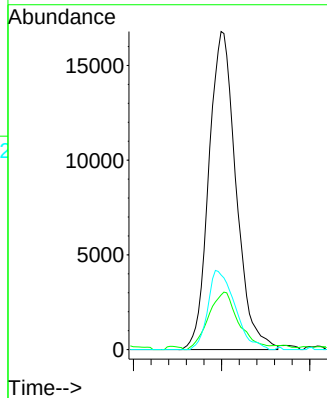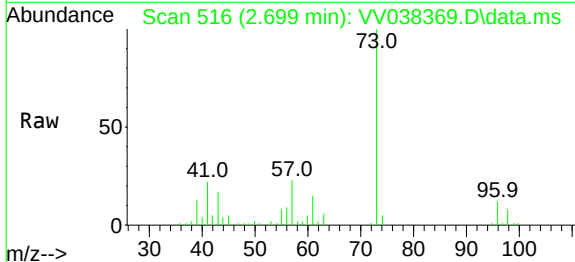



#18

trans-1,2-Dichloroethene

Concen: 0.280 ug/L

RT: 2.696 min Scan# 51

Delta R.T. 0.009 min

Lab File: VV038369.D


Acq: 26 Nov 2024 17:05

Instrument :

MSVOA_V

ClientSampleId :

BG445

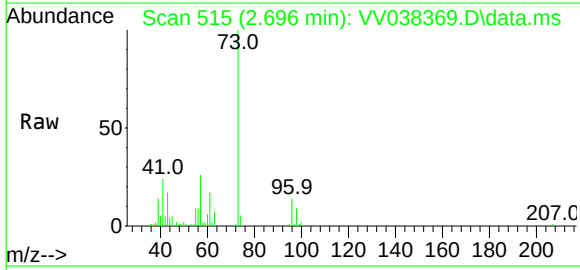




Tgt Ion: 96 Resp: 4357

Ion Ratio Lower Upper

96 100

61 122.9 88.5 164.4

98 62.6 43.9 81.5

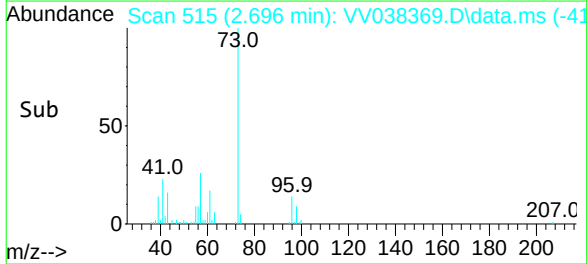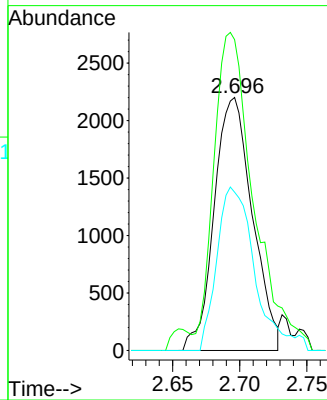

#19

1,1-Dichloroethane

Concen: 15.995 ug/L

RT: 3.101 min Scan# 641

Delta R.T. -0.000 min

Lab File: VV038369.D

Acq: 26 Nov 2024 17:05




Tgt Ion: 63 Resp: 451257


Ion Ratio Lower Upper

63 100

65 32.3 22.5 41.7

83 13.8 10.1 18.9



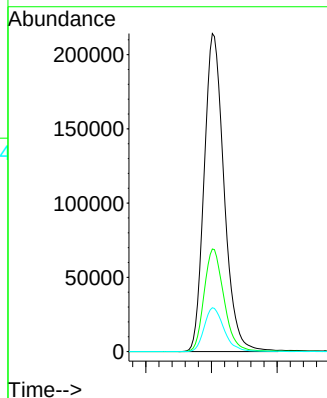
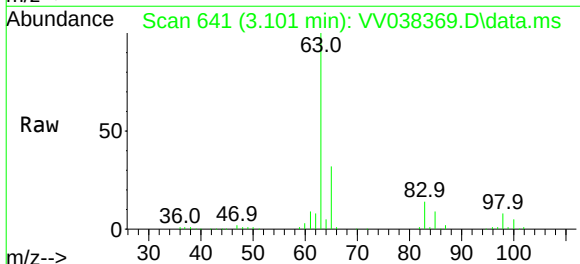




#22
cis-1,2-Dichloroethene
Concen: 17.713 ug/L
RT: 3.802 min Scan# 85
Delta R.T. -0.003 min
Lab File: VV038369.D
Acq: 26 Nov 2024 17:05




Instrument :
MSVOA_V
ClientSampleId :
BG445


Tgt Ion: 96 Resp: 284670
Ion Ratio Lower Upper
96 100
61 119.7 82.7 153.5
98 64.0 46.3 85.9

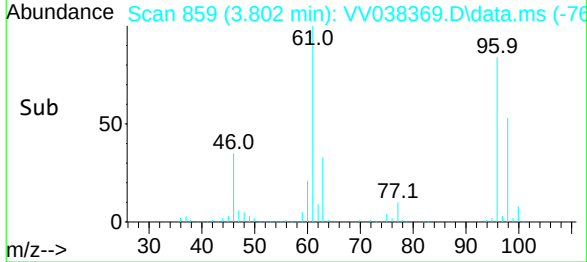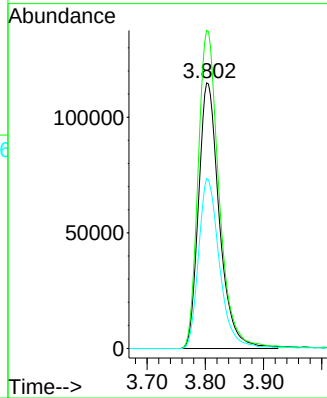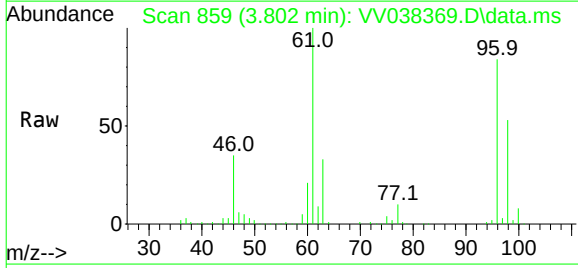

#25
Chloroform
Concen: 0.268 ug/L
RT: 4.272 min Scan# 1005
Delta R.T. 0.009 min
Lab File: VV038369.D
Acq: 26 Nov 2024 17:05

Tgt Ion: 83 Resp: 8084
Ion Ratio Lower Upper
83 100
85 82.1 46.5 86.3

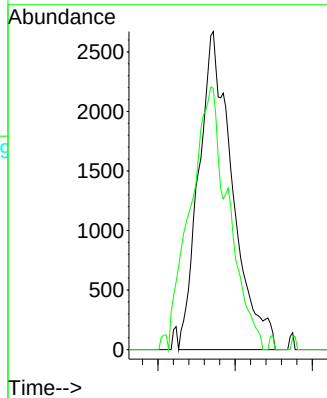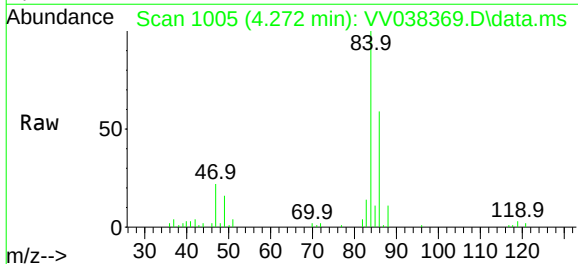



#29

1,1,1-Trichloroethane

Concen: 12.753 ug/L

RT: 4.503 min Scan# 1076

Delta R.T. 0.003 min

Lab File: VV038369.D

Acq: 26 Nov 2024 17:05

Instrument :

MSVOA_V

ClientSampleId :

BG445





Tgt Ion: 97 Resp: 341500

Ion Ratio Lower Upper

97 100

99 64.3 51.8 77.8

61 42.8 32.2 48.2

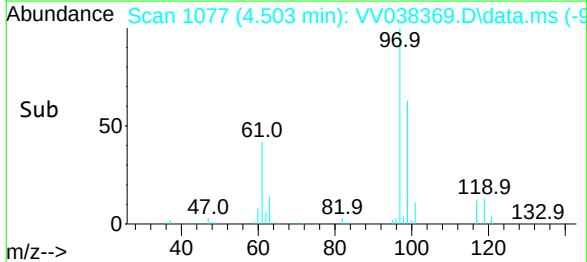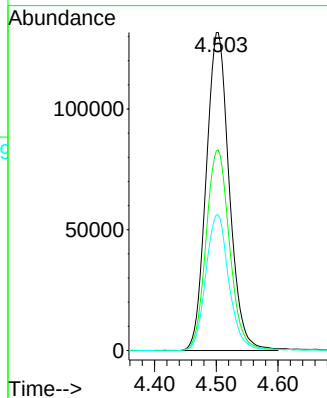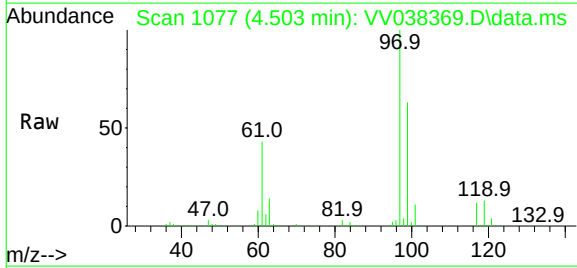

#34

Trichloroethene

Concen: 21.275 ug/L

RT: 5.821 min Scan# 1487

Delta R.T. -0.003 min

Lab File: VV038369.D

Acq: 26 Nov 2024 17:05

Tgt Ion: 95 Resp: 363733




Ion Ratio Lower Upper


95 100

97 65.2 44.8 83.2

132 96.2 68.3 126.8


130 100.2 70.2 130.4

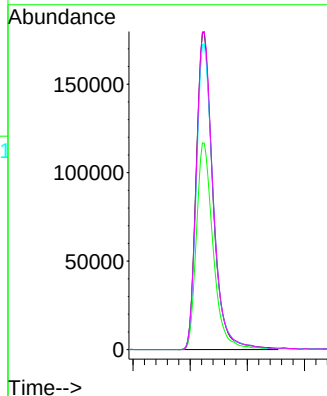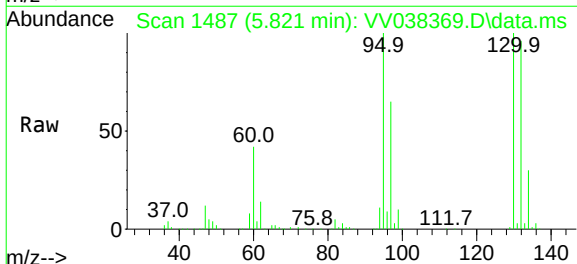

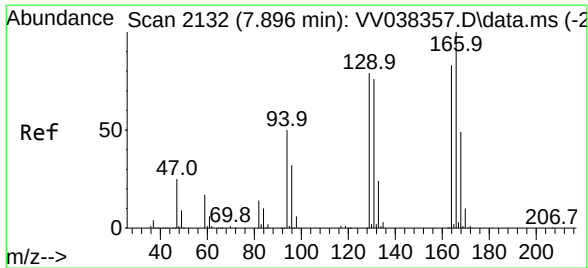

#47
Tetrachloroethene
Concen: 4.615 ug/L
RT: 7.899 min Scan# 21
Delta R.T. 0.003 min
Lab File: VV038369.D
Acq: 26 Nov 2024 17:05

Instrument :
MSVOA_V
ClientSampleId :
BG445

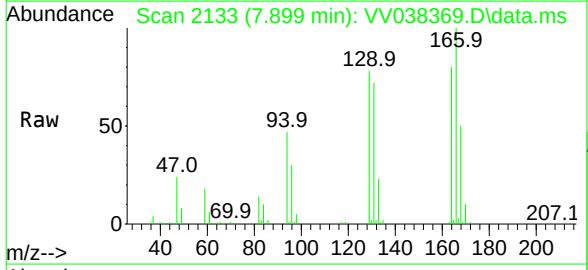

Tgt Ion:	164	Resp:	63395
Ion	Ratio	Lower	Upper
164	100		
129	98.3	68.5	127.1
131	90.0	64.8	120.4
166	125.3	88.3	163.9

