

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112624\
 Data File : VV038360.D
 Acq On : 26 Nov 2024 13:03
 Operator : SY/MD
 Sample : VIBLK205
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK205

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV038360.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	86	rBV	77304	85754	11.91%	1.577%
2	1.413	112	116	125	rVB6	5933	8018	1.11%	0.147%
3	1.529	144	152	165	rBV	76407	92686	12.87%	1.705%
4	1.831	237	246	258	rBV2	25523	42617	5.92%	0.784%
5	2.053	304	315	329	rBV	146608	214536	29.79%	3.946%
6	3.780	841	852	887	rBV2	108028	332446	46.16%	6.115%
7	4.243	977	996	1021	rBV	113411	305899	42.48%	5.627%
8	4.950	1203	1216	1250	rBV3	235222	629100	87.36%	11.572%
9	5.529	1387	1396	1416	rBV2	172964	375562	52.15%	6.908%
10	5.982	1526	1537	1566	rBV2	143755	327391	45.46%	6.022%
11	6.915	1816	1827	1856	rBV2	52199	120125	16.68%	2.210%
12	7.240	1917	1928	1955	rBV	221199	418620	58.13%	7.700%
13	7.558	2018	2027	2049	rBV2	31870	74614	10.36%	1.373%
14	7.863	2114	2122	2137	rBV3	4764	10042	1.39%	0.185%
15	8.018	2161	2170	2223	rBV	293524	720128	100.00%	13.247%
16	8.780	2397	2407	2442	rBV	311597	556689	77.30%	10.240%
17	10.146	2821	2832	2854	rBV	147899	249561	34.66%	4.591%
18	10.317	2877	2885	2896	rBV4	7326	11377	1.58%	0.209%
19	11.182	3144	3154	3179	rBV	258367	446530	62.01%	8.214%
20	11.554	3259	3270	3292	rBV	243171	414597	57.57%	7.626%

Sum of corrected areas: 5436292




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112624\
Data File : VV038360.D
Acq On : 26 Nov 2024 13:03
Operator : SY/MD
Sample : VIBLK205
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK205

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

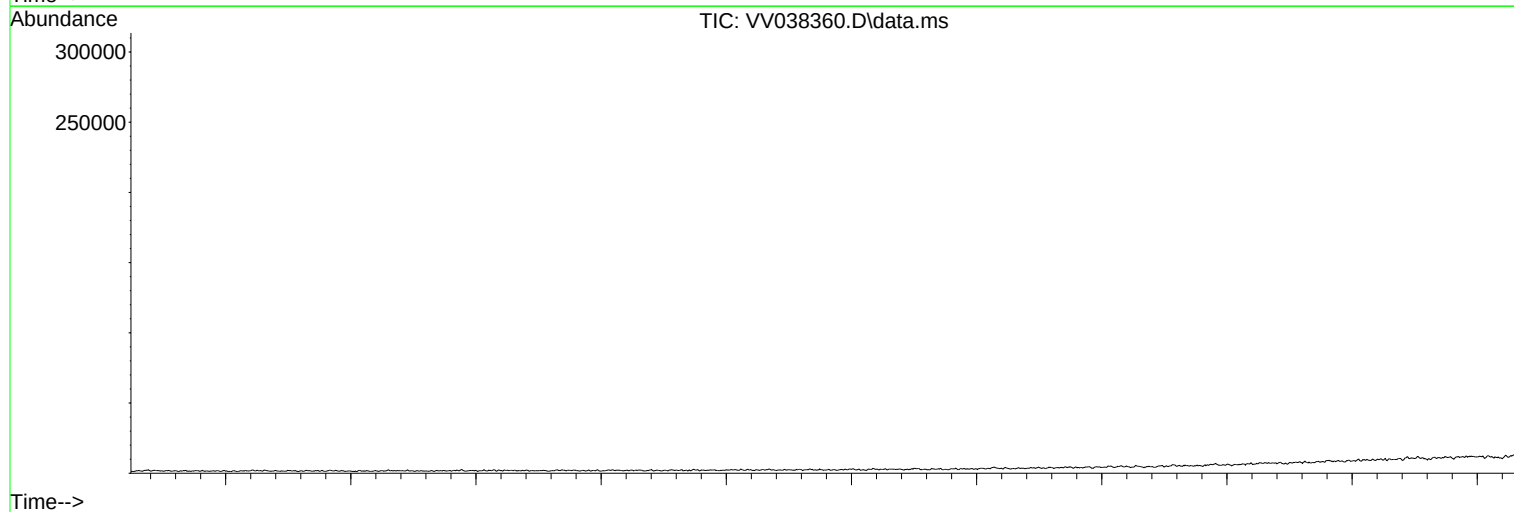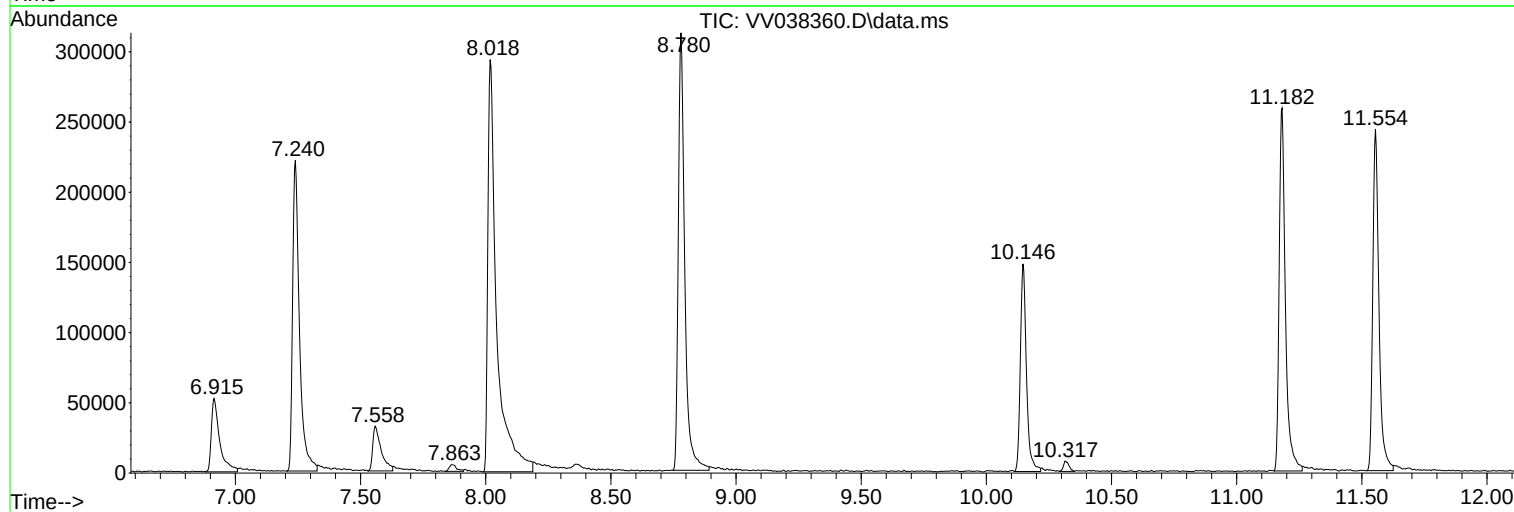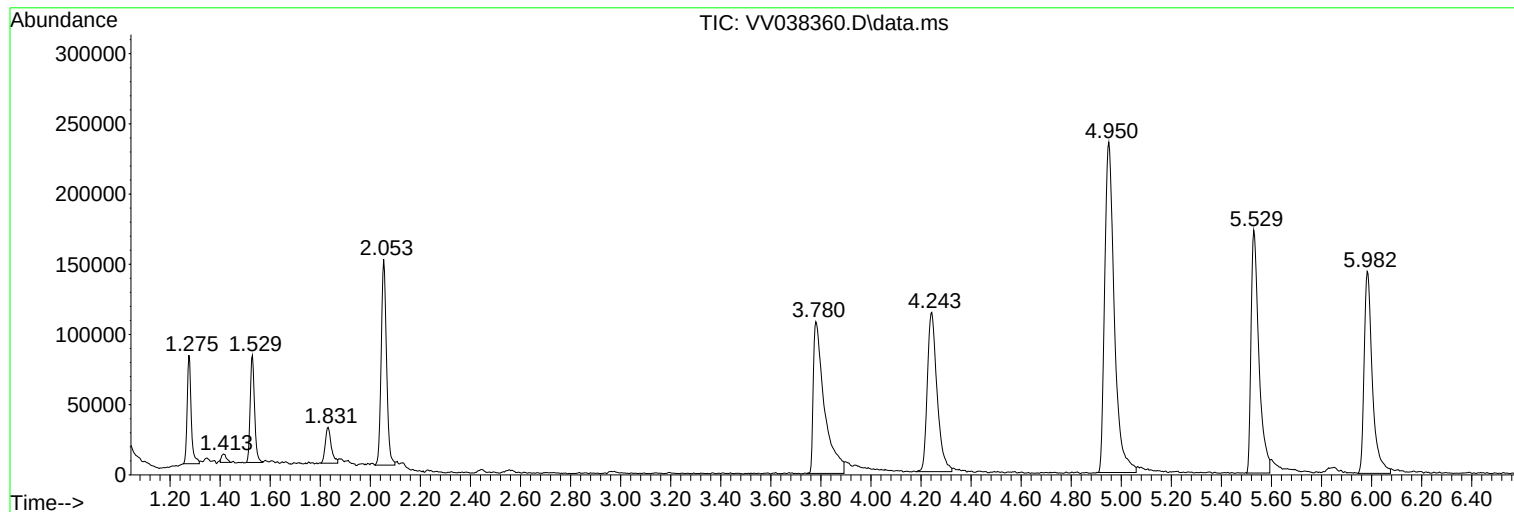

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112624\
Data File : VV038360.D
Acq On : 26 Nov 2024 13:03
Operator : SY/MD
Sample : VIBLK205
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK205

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112624\
Data File : VV038360.D
Acq On : 26 Nov 2024 13:03
Operator : SY/MD
Sample : VIBLK205
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK205

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc