

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112624\
 Data File : VV038363.D
 Acq On : 26 Nov 2024 14:40
 Operator : SY/MD
 Sample : VIBLK206
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK206

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	84	rVB	33877	36102	12.38%	1.699%
2	1.413	109	116	120	rBV6	4131	5688	1.95%	0.268%
3	1.529	144	152	160	rBV	29294	36463	12.50%	1.716%
4	2.053	306	315	332	rVB	60184	91436	31.35%	4.304%
5	2.449	426	438	446	rVB8	2552	4703	1.61%	0.221%
6	3.789	842	855	882	rBV2	49762	156991	53.82%	7.389%
7	4.243	980	996	1019	rBV	42284	119797	41.07%	5.638%
8	4.953	1203	1217	1242	rBV4	86604	235495	80.73%	11.084%
9	5.532	1388	1397	1422	rBV2	59209	143248	49.11%	6.742%
10	5.985	1523	1538	1564	rBV3	50054	122287	41.92%	5.756%
11	6.921	1820	1829	1853	rBV2	16540	43737	14.99%	2.059%
12	7.243	1920	1929	1947	rBV	69510	138929	47.63%	6.539%
13	7.567	2023	2030	2047	rBV4	9760	23534	8.07%	1.108%
14	7.866	2115	2123	2131	rBV5	7023	10710	3.67%	0.504%
15	7.908	2131	2136	2145	rVB8	3309	5436	1.86%	0.256%
16	8.024	2164	2172	2210	rBV	109377	291704	100.00%	13.729%
17	8.783	2399	2408	2435	rBV	108871	206579	70.82%	9.723%
18	10.149	2821	2833	2860	rBV2	65344	116028	39.78%	5.461%
19	10.316	2877	2885	2895	rBV3	9026	15324	5.25%	0.721%
20	11.185	3145	3155	3180	rBV	92006	171367	58.75%	8.066%
21	11.558	3260	3271	3295	rBV2	79239	149119	51.12%	7.018%

Sum of corrected areas: 2124677




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112624\
Data File : VV038363.D
Acq On : 26 Nov 2024 14:40
Operator : SY/MD
Sample : VIBLK206
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK206

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

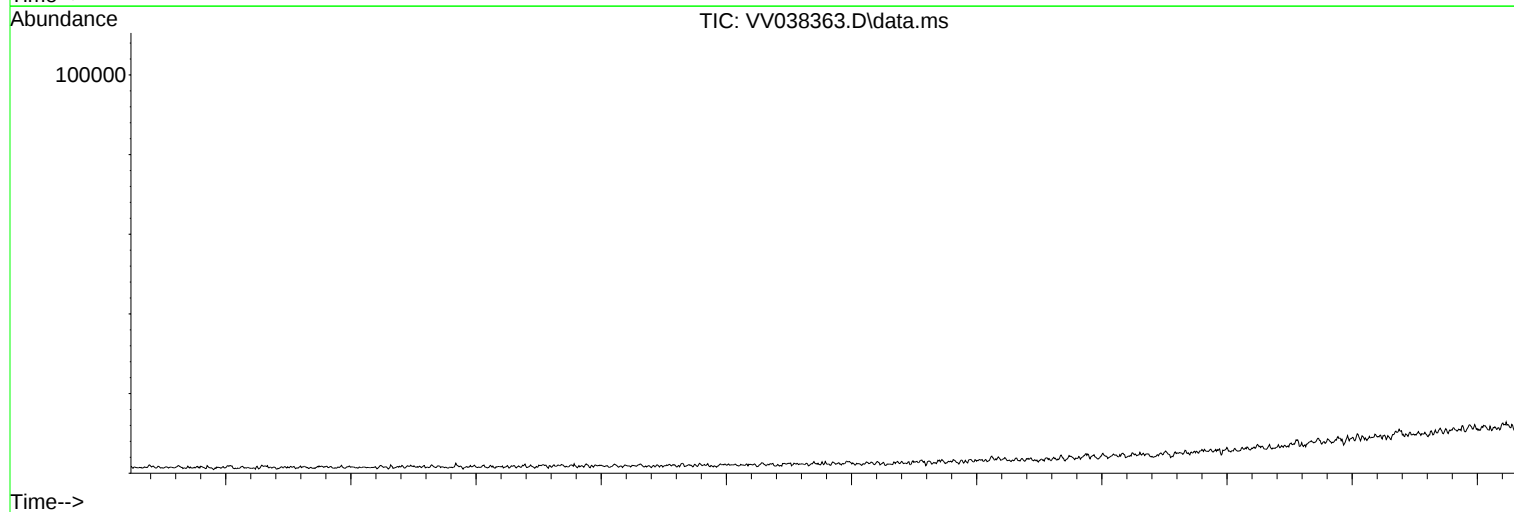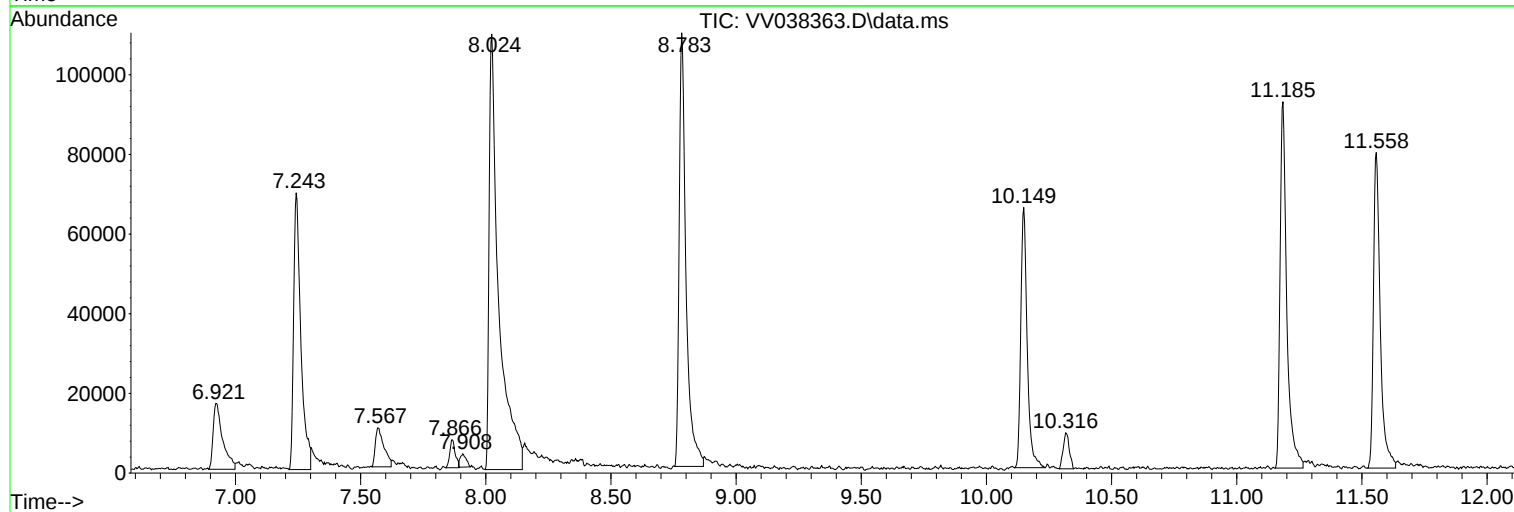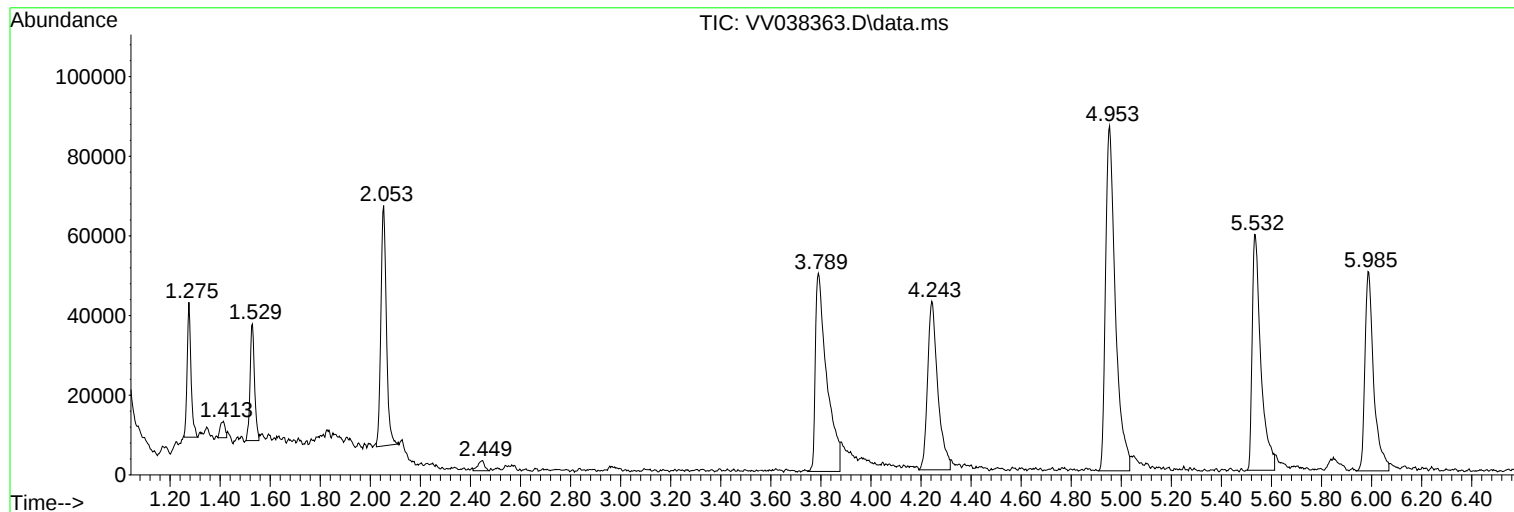

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112624\
Data File : VV038363.D
Acq On : 26 Nov 2024 14:40
Operator : SY/MD
Sample : VIBLK206
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK206

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112624\
Data File : VV038363.D
Acq On : 26 Nov 2024 14:40
Operator : SY/MD
Sample : VIBLK206
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK206

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc