

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112624\
 Data File : VV038365.D
 Acq On : 26 Nov 2024 15:28
 Operator : SY/MD
 Sample : P4930-02
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG440RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038365.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	16	22	33	rVB	81008	90930	4.90%	0.873%
2	1.275	65	73	88	rBV	82603	90486	4.88%	0.869%
3	1.529	144	152	164	rBV	86303	100962	5.44%	0.970%
4	1.902	250	268	283	rBV4	40130	163424	8.81%	1.570%
5	2.059	305	317	330	rBV3	299275	507587	27.37%	4.876%
6	2.265	367	381	419	rVB2	32846	127903	6.90%	1.229%
7	2.442	425	436	453	rVB	93786	155657	8.39%	1.495%
8	3.108	632	643	662	rBV2	15618	33564	1.81%	0.322%
9	3.802	847	859	892	rBV2	193306	630720	34.01%	6.058%
10	4.243	979	996	1029	rBV3	141250	424757	22.90%	4.080%
11	4.503	1062	1077	1094	rBV3	38178	100107	5.40%	0.962%
12	4.728	1135	1147	1163	rVB4	9365	22994	1.24%	0.221%
13	4.950	1203	1216	1241	rBV2	265420	701129	37.81%	6.735%
14	5.529	1386	1396	1424	rBV	221817	490706	26.46%	4.713%
15	5.825	1475	1488	1524	rBV	899876	1854522	100.00%	17.814%
16	5.982	1527	1537	1561	rVB	167116	361400	19.49%	3.471%
17	6.915	1817	1827	1851	rBV2	60164	133654	7.21%	1.284%
18	7.239	1917	1928	1947	rBV	244024	463895	25.01%	4.456%
19	7.323	1949	1954	1975	rVB2	16725	39860	2.15%	0.383%
20	7.558	2020	2027	2046	rBV2	33703	72562	3.91%	0.697%
21	7.895	2115	2132	2157	rBV	533679	945092	50.96%	9.078%
22	8.021	2162	2171	2210	rBV	376306	837569	45.16%	8.045%
23	8.779	2397	2407	2433	rBV	394598	726383	39.17%	6.977%
24	10.146	2822	2832	2855	rBV2	154212	270730	14.60%	2.600%
25	11.181	3143	3154	3180	rBV	322546	558083	30.09%	5.361%
26	11.554	3250	3270	3297	rBV	284115	506077	27.29%	4.861%




Sum of corrected areas: 10410753

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112624\
Data File : VV038365.D
Acq On : 26 Nov 2024 15:28
Operator : SY/MD
Sample : P4930-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG440RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

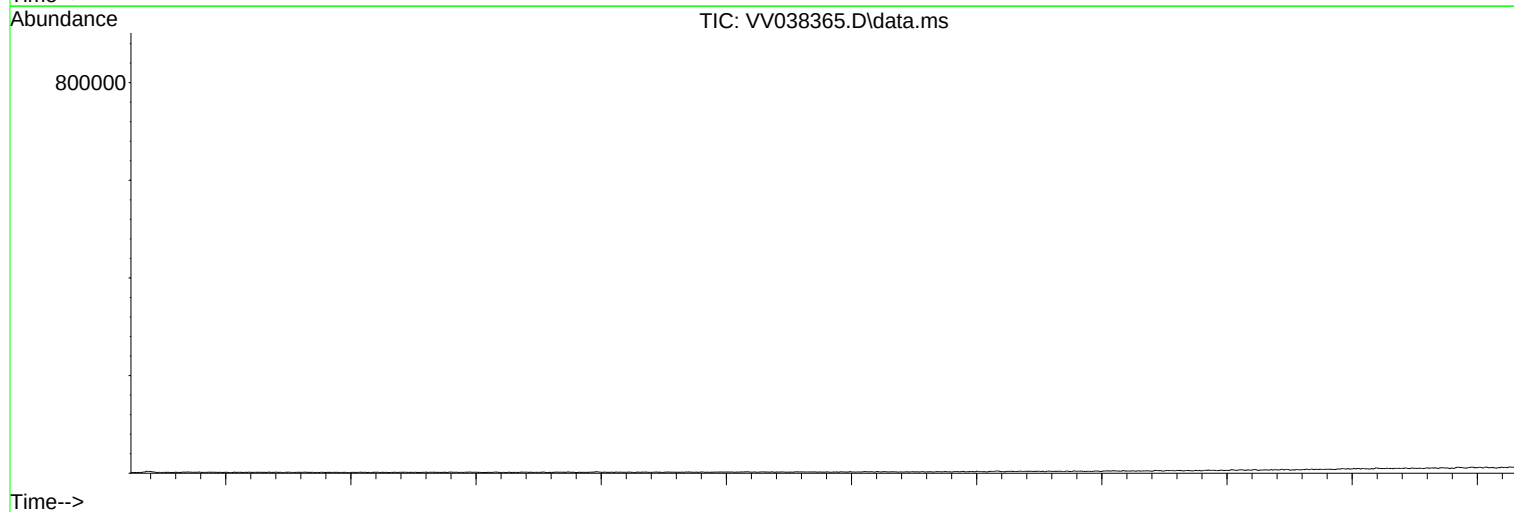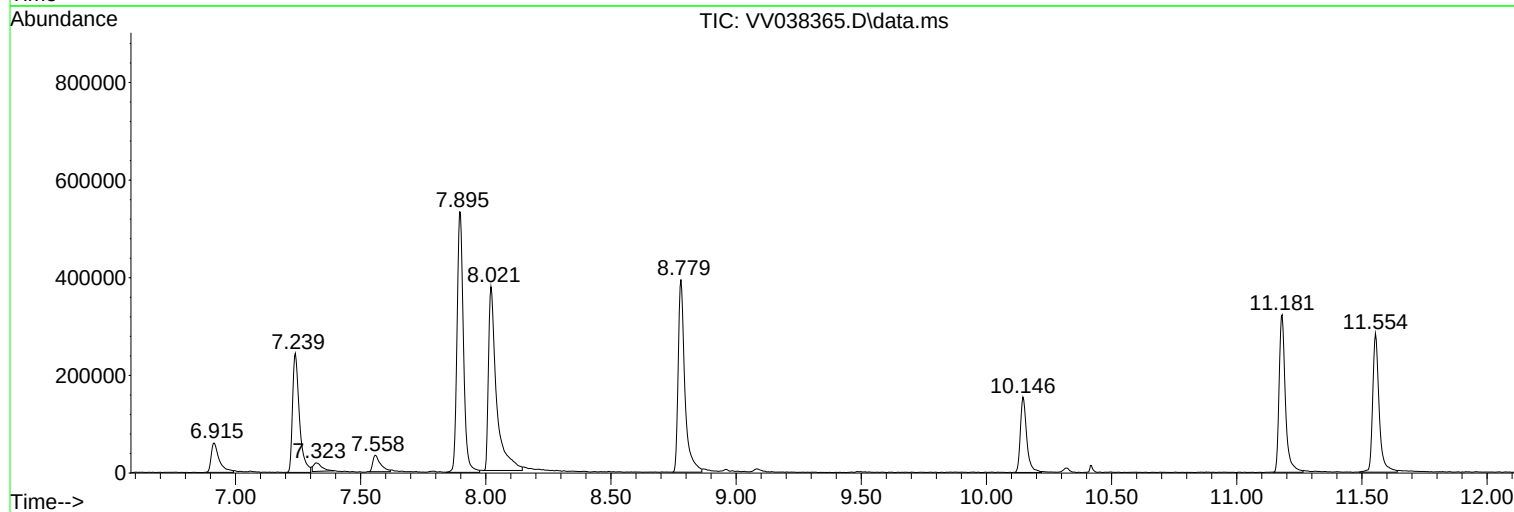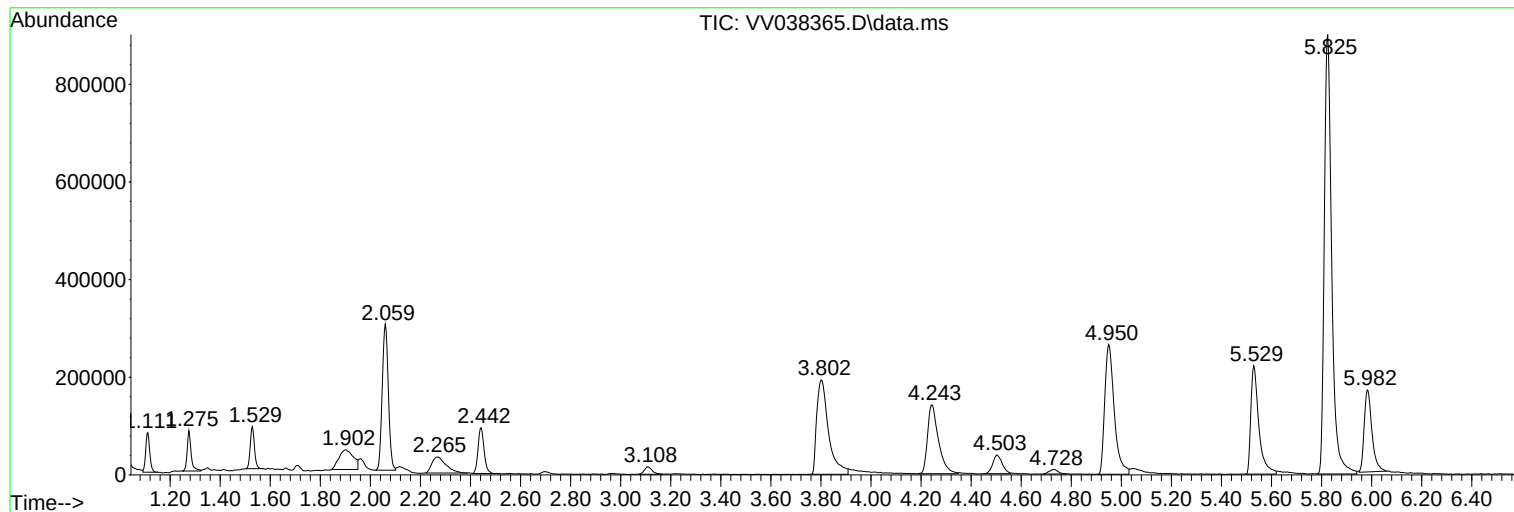

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112624\
Data File : VV038365.D
Acq On : 26 Nov 2024 15:28
Operator : SY/MD
Sample : P4930-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG440RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112624\
Data File : VV038365.D
Acq On : 26 Nov 2024 15:28
Operator : SY/MD
Sample : P4930-02
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG440RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc