

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112724\
 Data File : VV038381.D
 Acq On : 27 Nov 2024 13:25
 Operator : SY/MD
 Sample : P4884-21
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Nov 28 00:31:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 28 00:29:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	93804	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	104402	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	42132	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	29559	4.111	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.200%
7) Chloroethane-d5	1.529	69	30322	5.214	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.200%
11) 1,1-Dichloroethene-d2	2.056	65	14424	4.662	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	93.200%
20) 2-Butanone-d5	3.786	46	99674	69.299	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	138.600%#
24) Chloroform-d	4.246	84	75388	5.403	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.000%
26) 1,2-Dichloroethane-d4	4.940	65	41143	6.571	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	131.400%#
32) Benzene-d6	4.957	84	120769	4.476	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.600%
36) 1,2-Dichloropropane-d6	5.985	67	43893	5.286	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.800%
41) Toluene-d8	7.239	98	89493	3.584	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.600%
43) trans-1,3-Dichloroprop...	7.564	79	13394	4.339	ug/L	0.01
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.800%
46) 2-Hexanone-d5	8.021	63	59530	49.609	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.220%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	48339	6.858	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	137.200%#
66) 1,2-Dichlorobenzene-d4	11.558	152	38149	5.314	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.200%
Target Compounds						
					Qvalue	
61) 1,2,3-Trichloropropane	11.185	75	4832	1.340	ug/L #	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112724\
Data File : VV038381.D
Acq On : 27 Nov 2024 13:25
Operator : SY/MD
Sample : P4884-21
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Nov 28 00:31:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 28 00:29:54 2024
Response via : Initial Calibration

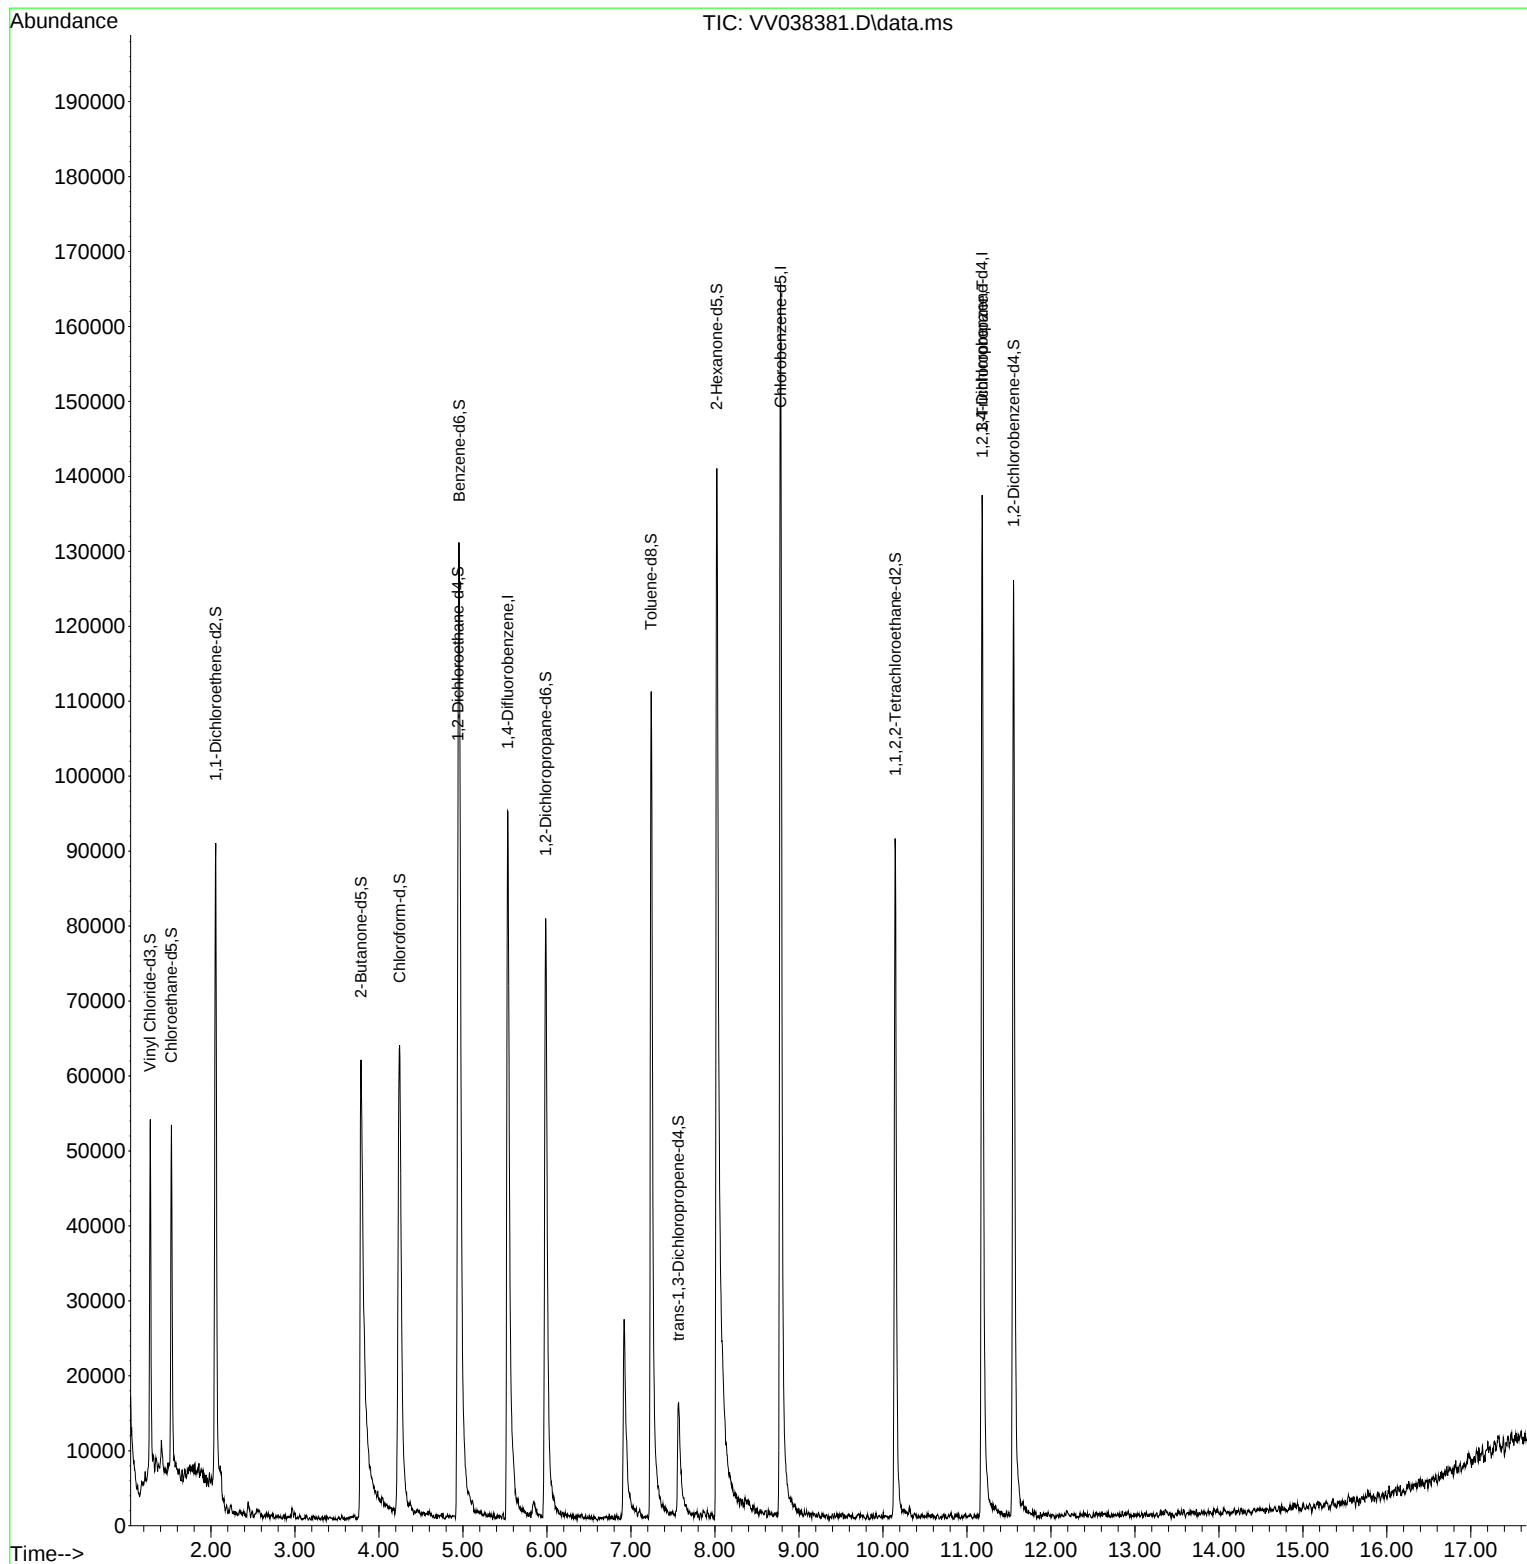

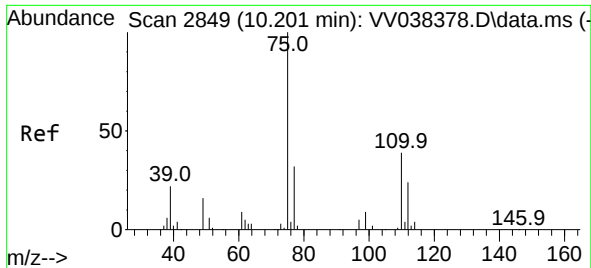

#61

1,2,3-Trichloropropane

Concen: 1.340 ug/L

RT: 11.185 min Scan# 31

Delta R.T. 0.984 min


Lab File: VV038381.D

Acq: 27 Nov 2024 13:25

Instrument :

MSVOA_V

ClientSampleId :

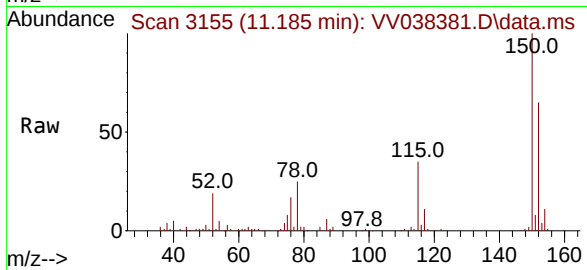

Tgt Ion: 75 Resp: 4832

Ion Ratio Lower Upper

75 100

77 37.5 26.4 39.6

110 0.9 32.3 48.5#

