
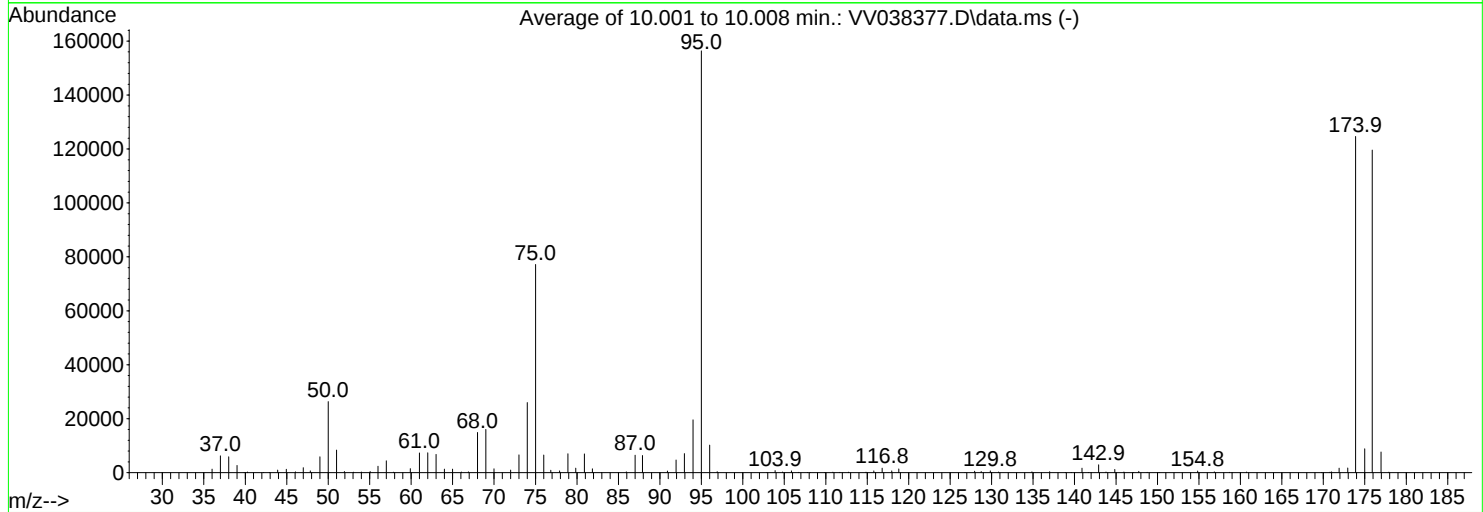


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV112724\
Data File : VV038377.D
Acq On : 27 Nov 2024 07:59
Operator : SY/MD
Sample : BFB295
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB295

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Nov 28 00:29:54 2024

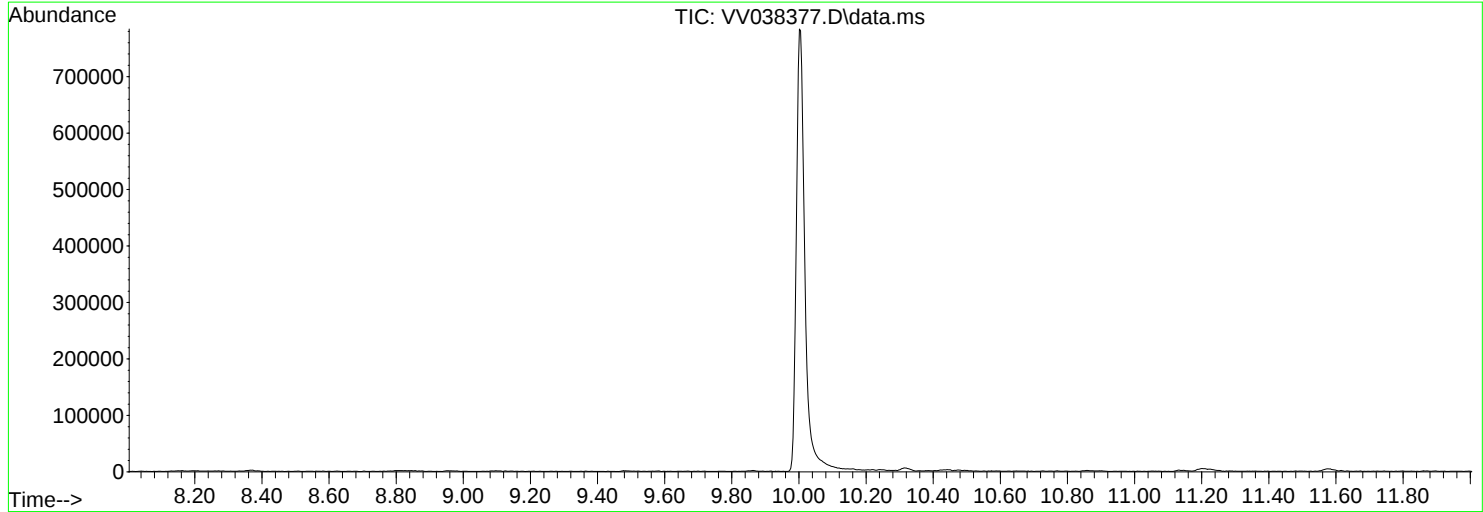

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2775

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.8	26312	PASS
75	95	30	80	49.3	77173	PASS
95	95	100	100	100.0	156395	PASS
96	95	5	9	6.5	10181	PASS
173	174	0.00	2	1.4	1729	PASS
174	95	50	120	79.7	124669	PASS
175	174	5	9	7.1	8852	PASS
176	174	95	105	95.9	119608	PASS
177	176	5	10	6.4	7656	PASS

m/z	Abundance
39.80	237.0
40.90	148.0
43.90	573.0

Instrument :
MSVOA_V
ClientSampleId :
BFB295

m/z	Abundance
36.00	1373.0
37.00	6610.0
38.00	6396.0
39.00	2934.0
39.90	307.0
42.30	102.0
42.90	129.0
44.00	1549.0
45.00	1313.0
46.00	394.0
47.00	2076.0
47.80	662.0
49.00	6387.0
50.00	28560.0
51.00	9032.0
52.00	405.0
53.00	234.0
54.00	250.0
55.10	497.0
56.00	2517.0
57.00	4476.0
57.90	292.0
59.90	1456.0
61.00	7560.0
62.00	7661.0
63.00	7264.0
64.00	1306.0
65.00	1311.0
66.10	203.0
67.00	473.0
68.00	15711.0
69.00	16192.0
70.00	1693.0
72.00	871.0
73.00	6696.0
74.00	26840.0
75.00	80304.0
76.00	6827.0
76.80	1058.0
77.90	622.0
78.90	7253.0
79.90	1690.0
80.90	7326.0
81.90	1528.0
83.00	137.0
86.00	435.0
87.00	6914.0
87.90	6895.0
90.90	565.0
91.90	4693.0
93.00	7333.0
94.00	20744.0
95.00	159424.0
96.00	10798.0
96.90	392.0
103.90	790.0
104.80	250.0
105.90	724.0
106.80	120.0
108.10	101.0
109.90	117.0
110.90	191.0
111.70	142.0
112.70	242.0
114.90	177.0
115.80	720.0
116.80	1732.0
118.00	636.0
118.80	1297.0
126.80	114.0
127.90	587.0
128.80	488.0
129.80	663.0
130.90	274.0
134.80	411.0
137.00	346.0
140.00	104.0
140.90	1592.0
141.70	178.0
142.90	3165.0
143.80	366.0
144.90	1119.0
146.00	257.0
147.10	102.0
147.80	487.0
148.80	150.0
154.90	621.0
156.90	322.0
159.00	135.0
160.80	233.0
169.80	105.0
170.80	532.0

Instrument :
MSVOA_V
ClientSampleId :
BFB295

171.90	1687.0
172.90	1949.0
173.90	125896.0
175.00	9294.0
175.90	120888.0
176.90	8087.0
177.90	226.0

Instrument :
MSVOA_V
ClientSampleId :
BFB295

m/z	Abundance
36.00	1353.0
37.00	6375.0
38.00	6055.0
39.00	2690.0
39.90	322.0
40.20	337.0
40.80	163.0
43.90	1633.0
45.00	1307.0
46.10	320.0
47.00	1918.0
47.80	666.0
49.00	6015.0
50.00	27032.0
51.00	8544.0
51.90	444.0
53.00	205.0
54.00	232.0
55.10	394.0
56.00	2412.0
57.00	4538.0
57.90	217.0
59.90	1541.0
61.00	7581.0
62.00	7484.0
63.00	6965.0
64.00	1423.0
65.00	1321.0
66.10	241.0
66.90	311.0
68.00	15281.0
69.00	16496.0
70.00	1496.0
72.00	982.0
73.00	6752.0
74.00	26480.0
75.00	79320.0
76.00	6616.0
76.80	926.0
77.90	667.0
78.90	7261.0
79.90	1717.0
80.90	7041.0
81.90	1442.0
82.90	119.0
85.90	300.0
87.00	6791.0
87.90	6500.0
90.90	635.0
92.00	4743.0
93.00	7290.0
94.00	20064.0
95.00	160512.0
96.00	10502.0
96.90	298.0
102.90	104.0
103.90	826.0
104.80	254.0
105.90	661.0
106.70	152.0
110.80	207.0
111.70	140.0
112.70	229.0
114.90	202.0
115.80	697.0
116.80	1770.0
117.90	652.0
118.80	1425.0
126.80	107.0
128.00	544.0
128.80	450.0
129.80	715.0
130.90	229.0
134.90	318.0
137.00	402.0
140.00	130.0
140.90	1730.0
142.90	3014.0
143.80	276.0
144.80	1235.0
145.90	278.0
147.70	465.0
148.80	149.0
154.80	678.0
156.90	340.0
158.70	181.0
160.70	209.0
171.00	483.0
171.90	1786.0
173.00	1788.0
173.90	128088.0
175.00	8997.0

Instrument :
MSVOA_V
ClientSampleId :
BFB295

175.90

177.00

177.90

122968.0

7915.0

212.0

Instrument :

MSVOA_V

ClientSampleId :

BFB295

m/z	Abundance
36.00	1287.0
37.00	5648.0
38.00	5182.0
39.00	2370.0
39.90	362.0
40.30	396.0
42.10	104.0
43.90	1485.0
44.90	1128.0
46.10	272.0
47.00	1574.0
47.90	633.0
49.00	5194.0
50.00	23344.0
51.00	7462.0
51.90	404.0
53.10	155.0
54.00	204.0
55.00	301.0
56.00	2168.0
57.00	4104.0
57.80	121.0
59.90	1455.0
61.00	6694.0
62.00	6888.0
63.00	5992.0
64.00	1293.0
65.00	1252.0
66.00	208.0
66.80	215.0
68.00	13695.0
69.00	15324.0
70.00	1152.0
72.00	944.0
73.00	6316.0
74.00	24616.0
75.00	71896.0
76.00	6072.0
76.90	746.0
77.90	676.0
78.90	6497.0
79.80	1679.0
80.90	6453.0
81.80	1283.0
85.90	235.0
87.00	5777.0
87.90	5744.0
90.90	678.0
92.00	4569.0
92.90	6625.0
94.00	17968.0
95.00	149248.0
96.00	9244.0
96.90	198.0
97.00	193.0
102.90	113.0
103.90	738.0
104.80	257.0
105.80	634.0
106.70	175.0
107.80	143.0
110.80	207.0
111.70	105.0
112.80	173.0
114.80	187.0
115.80	611.0
116.80	1524.0
117.90	635.0
118.80	1347.0
128.00	483.0
128.70	332.0
129.90	635.0
130.80	216.0
134.90	277.0
137.00	372.0
138.90	136.0
139.60	110.0
140.90	1674.0
142.00	216.0
142.90	2563.0
143.90	151.0
144.80	1191.0
145.90	267.0
147.70	398.0
148.70	109.0
150.20	122.0
154.80	510.0
156.80	308.0
158.70	175.0
160.70	217.0
171.00	492.0
171.90	1602.0

Instrument :
MSVOA_V
ClientSampleId :
BFB295

172.90	1449.0
173.90	120024.0
175.00	8266.0
175.90	114968.0
177.00	6965.0
177.90	185.0

Instrument :
MSVOA_V
ClientSampleId :
BFB295