

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120224\
 Data File : VV038392.D
 Acq On : 02 Dec 2024 16:37
 Operator : SY/MD
 Sample : VV1202WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK256

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120224WMA.M
 Title : VOC Analysis

Signal : TIC: VV038392.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	67	73	87	rBV	316270	342038	15.05%	2.054%
2	1.529	145	152	165	rVB	268279	310277	13.65%	1.863%
3	2.053	306	315	330	rBV	547827	802434	35.31%	4.818%
4	2.786	541	543	547	rBV2	512	281	0.01%	0.002%
5	2.838	557	559	561	rBV3	525	285	0.01%	0.002%
6	2.896	575	577	579	rBV	549	190	0.01%	0.001%
7	3.056	626	627	628	rBV	498	162	0.01%	0.001%
8	3.085	634	636	638	rBV2	424	183	0.01%	0.001%
9	3.101	638	641	643	rBV4	548	317	0.01%	0.002%
10	3.150	653	656	657	rBV	372	190	0.01%	0.001%
11	3.201	667	672	674	rBV3	578	564	0.02%	0.003%
12	3.243	682	685	688	rVB2	715	460	0.02%	0.003%
13	3.269	688	693	698	rBV4	554	671	0.03%	0.004%
14	3.288	698	699	702	rVB	474	135	0.01%	0.001%
15	3.307	702	705	709	rBV4	477	522	0.02%	0.003%
16	3.339	712	715	717	rBV	433	223	0.01%	0.001%
17	3.423	737	741	743	rBV3	755	495	0.02%	0.003%
18	3.452	748	750	753	rBV	377	202	0.01%	0.001%
19	3.468	753	755	763	rVB3	439	436	0.02%	0.003%
20	3.507	763	767	770	rBV3	535	475	0.02%	0.003%
21	3.564	784	785	790	rBV2	405	226	0.01%	0.001%
22	3.648	809	811	813	rVB2	562	261	0.01%	0.002%
23	3.661	813	815	819	rBV3	324	227	0.01%	0.001%
24	3.680	819	821	825	rVB3	430	330	0.01%	0.002%
25	3.699	825	827	829	rBV2	407	204	0.01%	0.001%
26	3.719	829	833	835	rBV	581	348	0.02%	0.002%
27	3.783	845	853	888	rBV2	119768	374981	16.50%	2.251%
28	4.240	980	995	1033	rBV	348118	907194	39.92%	5.447%
29	4.947	1200	1215	1258	rBV2	846466	2272617	100.00%	13.645%
30	5.526	1384	1395	1435	rBV	585386	1272061	55.97%	7.637%
31	5.979	1524	1536	1573	rBV	483899	1024891	45.10%	6.153%
32	6.429	1674	1676	1679	rBV3	869	598	0.03%	0.004%
33	6.519	1700	1704	1705	rBV3	464	311	0.01%	0.002%
34	6.584	1721	1724	1726	rBV3	775	498	0.02%	0.003%
35	6.635	1738	1740	1741	rBV	402	166	0.01%	0.001%
36	6.674	1749	1752	1754	rBV3	700	381	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120224\
 Data File : VV038392.D
 Acq On : 02 Dec 2024 16:37
 Operator : SY/MD
 Sample : VV1202WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK256

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120224WMA.M
 Title : VOC Analysis

37	6.722	1763	1767	1771	rVB4	696	549	0.02%	0.003%
38	6.773	1781	1783	1785	rBV	451	172	0.01%	0.001%
39	6.905	1814	1824	1851	rBV	242732	484487	21.32%	2.909%
40	7.233	1916	1926	1966	rBV	978384	1785443	78.56%	10.720%
41	7.548	2015	2024	2061	rBV	169231	337984	14.87%	2.029%
42	7.908	2131	2136	2147	rBV9	1662	3231	0.14%	0.019%
43	8.018	2161	2170	2205	rBV	375633	824582	36.28%	4.951%
44	8.776	2395	2406	2439	rBV	970209	1648174	72.52%	9.896%
45	9.336	2578	2580	2582	rBV2	492	233	0.01%	0.001%
46	9.429	2606	2609	2610	rBV	591	315	0.01%	0.002%
47	9.468	2620	2621	2622	rBV	318	108	0.00%	0.001%
48	9.481	2622	2625	2628	rVV4	1054	794	0.03%	0.005%
49	9.545	2643	2645	2646	rBV3	623	233	0.01%	0.001%
50	9.567	2650	2652	2654	rBV3	654	377	0.02%	0.002%
51	9.632	2668	2672	2674	rBV2	1172	940	0.04%	0.006%
52	9.648	2674	2677	2679	rVV2	547	316	0.01%	0.002%
53	9.799	2721	2724	2725	rBV	596	322	0.01%	0.002%
54	9.834	2732	2735	2736	rBV2	521	243	0.01%	0.001%
55	9.937	2765	2767	2769	rVB	1040	383	0.02%	0.002%
56	9.953	2769	2772	2773	rBV2	805	503	0.02%	0.003%
57	9.985	2780	2782	2786	rBV3	493	389	0.02%	0.002%
58	10.046	2798	2801	2806	rVB3	771	572	0.03%	0.003%
59	10.069	2806	2808	2811	rBV2	458	306	0.01%	0.002%
60	10.143	2820	2831	2856	rBV	662703	1068951	47.04%	6.418%
61	10.487	2930	2938	2941	rBV5	1694	1889	0.08%	0.011%
62	10.522	2948	2949	2954	rBV2	559	248	0.01%	0.001%
63	10.587	2965	2969	2972	rBV3	614	528	0.02%	0.003%
64	10.693	2998	3002	3004	rBV	534	485	0.02%	0.003%
65	10.786	3028	3031	3032	rBV3	1034	514	0.02%	0.003%
66	10.860	3048	3054	3056	rBV3	1823	1712	0.08%	0.010%
67	10.995	3094	3096	3099	rVB4	781	431	0.02%	0.003%
68	11.011	3099	3101	3102	rBV	544	242	0.01%	0.001%
69	11.088	3121	3125	3128	rBV4	617	581	0.03%	0.003%
70	11.130	3132	3138	3142	rBV6	2883	3789	0.17%	0.023%
71	11.178	3142	3153	3185	rVV	901081	1485187	65.35%	8.917%
72	11.551	3257	3269	3297	rBV	996971	1649995	72.60%	9.906%
73	12.230	3478	3480	3483	rBV2	447	276	0.01%	0.002%
74	12.435	3542	3544	3546	rBV3	806	357	0.02%	0.002%
75	12.860	3674	3676	3679	rBV2	461	322	0.01%	0.002%
76	13.333	3821	3823	3825	rBV2	743	308	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120224\
Data File : VV038392.D
Acq On : 02 Dec 2024 16:37
Operator : SY/MD
Sample : VV1202WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK256

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120224WMA.M
Title : VOC Analysis

77	13.381	3835	3838	3839	rBV	733	386	0.02%	0.002%
78	13.448	3851	3859	3873	rBV2	11002	24901	1.10%	0.150%
79	13.680	3924	3931	3933	rBV7	5971	6742	0.30%	0.040%
80	13.751	3951	3953	3955	rBV2	792	497	0.02%	0.003%
81	13.808	3968	3971	3975	rBV4	919	850	0.04%	0.005%

Sum of corrected areas: 16655681




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120224\
Data File : VV038392.D
Acq On : 02 Dec 2024 16:37
Operator : SY/MD
Sample : VV1202WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK256

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

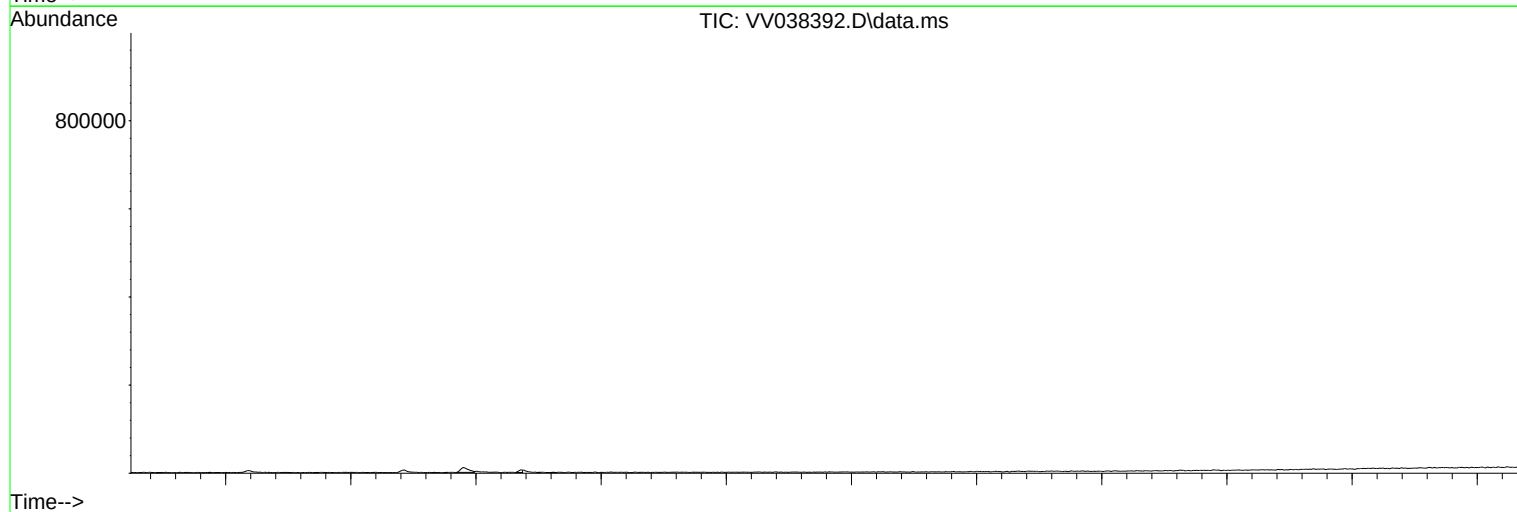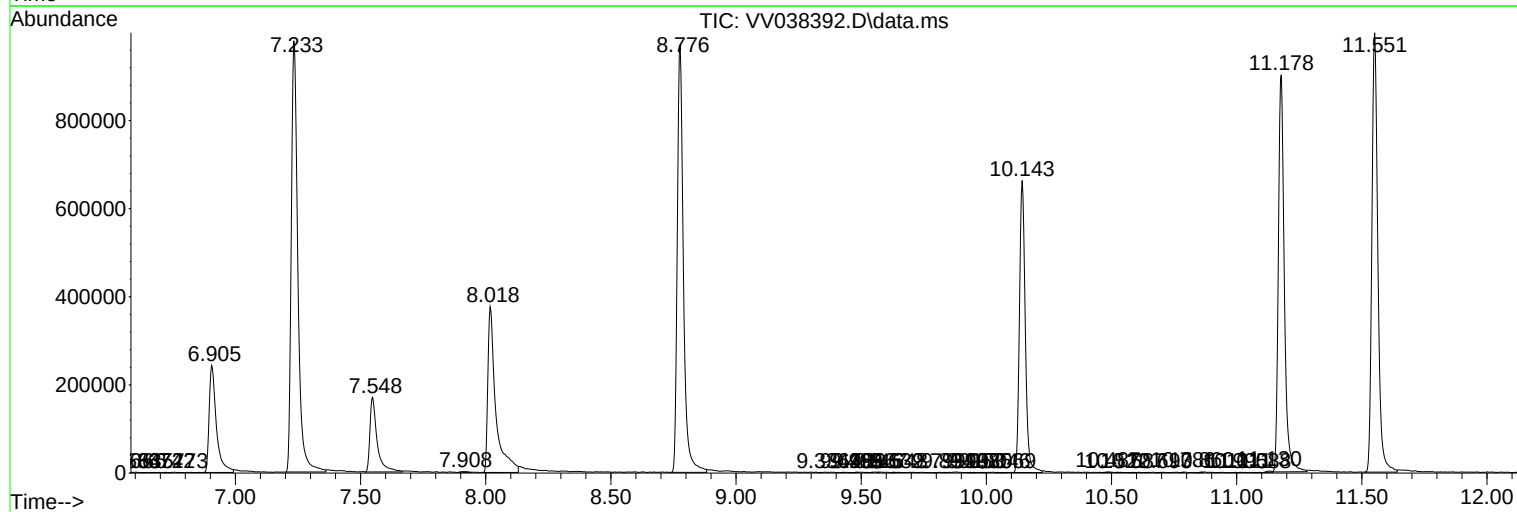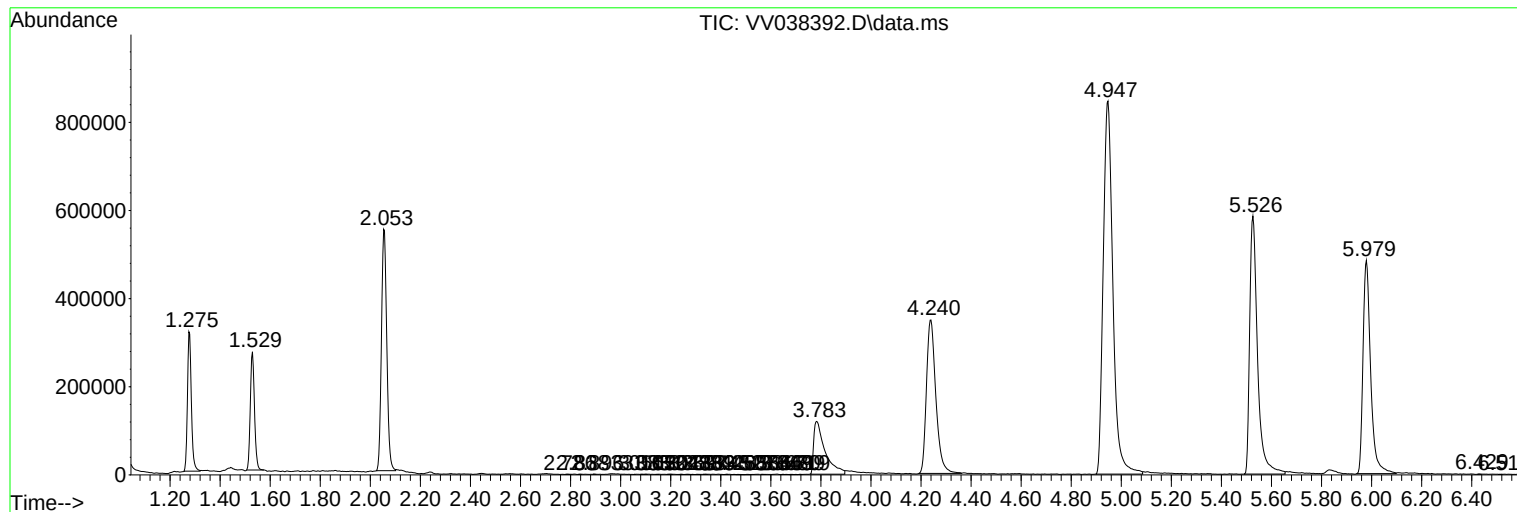

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120224\
Data File : VV038392.D
Acq On : 02 Dec 2024 16:37
Operator : SY/MD
Sample : VV1202WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK256

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120224\
Data File : VV038392.D
Acq On : 02 Dec 2024 16:37
Operator : SY/MD
Sample : VV1202WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK256

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc