
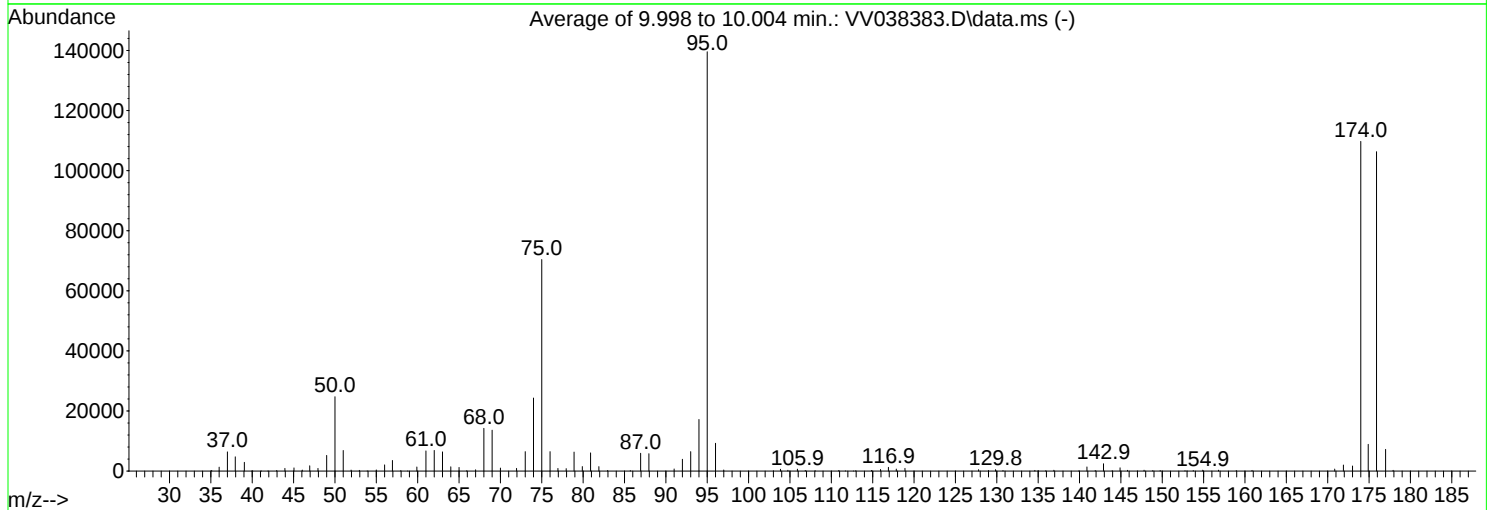


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120224\
Data File : VV038383.D
Acq On : 02 Dec 2024 08:12
Operator : SY/MD
Sample : BFB399
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB399

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120224WMA.M
Title : VOC Analysis
Last Update : Mon Dec 02 21:19:32 2024

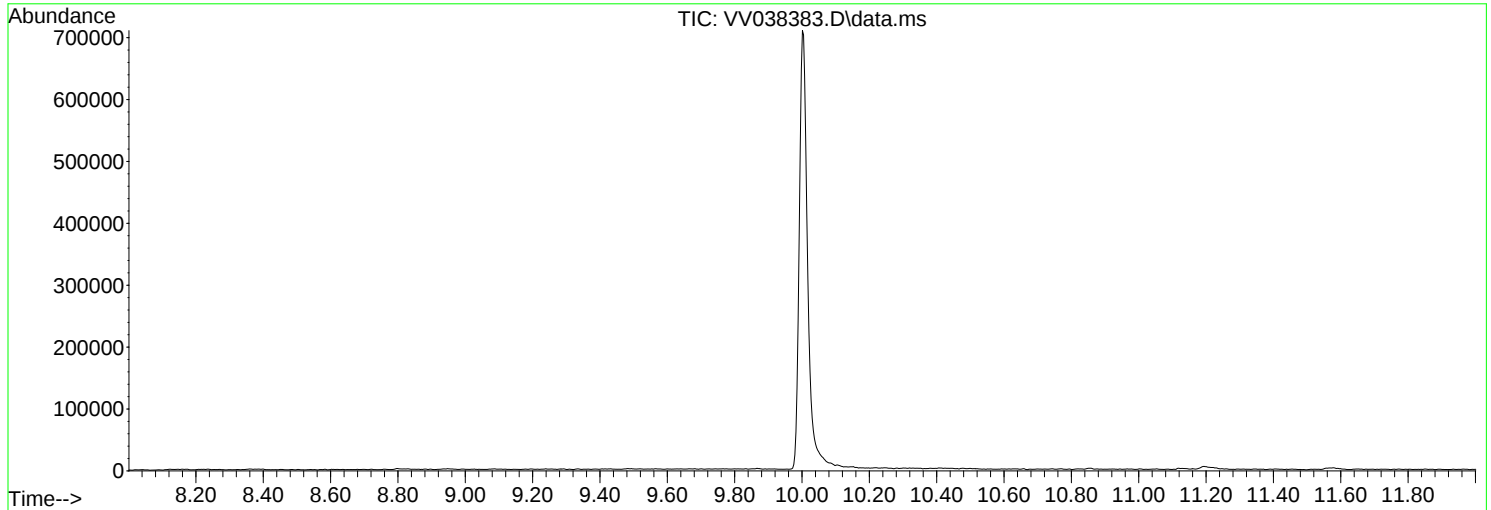

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2774

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	24757	PASS
75	95	30	80	50.4	70411	PASS
95	95	100	100	100.0	139584	PASS
96	95	5	9	6.6	9257	PASS
173	174	0.00	2	1.5	1691	PASS
174	95	50	120	78.6	109731	PASS
175	174	5	9	8.1	8902	PASS
176	174	95	105	96.9	106325	PASS
177	176	5	10	6.8	7218	PASS

m/z	Abundance
36.00	1307.0
37.10	171.0
37.90	453.0
40.10	434.0
43.90	361.0

Instrument :
MSVOA_V
ClientSampleId :
BFB399

m/z	Abundance
36.00	2553.0
37.00	6322.0
38.00	4992.0
39.00	2917.0
39.90	431.0
41.90	107.0
42.90	162.0
44.00	1096.0
45.10	991.0
46.10	292.0
46.90	1718.0
48.00	945.0
49.00	5212.0
50.00	23832.0
51.00	6414.0
51.90	316.0
52.90	198.0
55.00	347.0
56.00	1971.0
57.00	3232.0
58.00	133.0
59.90	1288.0
61.00	6824.0
62.00	6402.0
63.00	6090.0
64.00	1305.0
65.00	1155.0
67.00	431.0
68.00	13721.0
69.00	12890.0
70.00	1026.0
72.00	883.0
73.00	6242.0
74.00	23248.0
75.00	66344.0
76.00	6242.0
76.90	784.0
78.00	801.0
78.90	6133.0
79.90	1534.0
80.90	5576.0
81.90	1249.0
83.00	227.0
85.70	136.0
87.00	5903.0
88.00	5123.0
91.00	558.0
92.00	3671.0
93.00	6147.0
94.00	16358.0
95.00	132544.0
96.00	8925.0
97.00	323.0
103.90	555.0
104.80	285.0
105.90	607.0
106.90	184.0
108.00	106.0
111.00	221.0
111.70	122.0
112.70	120.0
114.90	237.0
115.90	510.0
116.90	1212.0
117.90	537.0
118.90	869.0
127.80	506.0
129.00	151.0
129.80	495.0
130.70	194.0
134.50	213.0
135.00	219.0
135.90	130.0
136.90	301.0
140.90	1173.0
141.90	171.0
142.90	2271.0
143.90	166.0
144.80	1244.0
145.80	183.0
147.00	116.0
147.90	314.0
148.80	124.0
149.80	184.0
152.70	105.0
153.00	106.0
153.70	169.0
154.90	292.0
156.80	261.0
158.90	122.0
160.90	265.0
170.90	653.0

Instrument :
MSVOA_V
ClientSampleId :
BFB399

171.90	1992.0
173.00	1600.0
174.00	101552.0
174.90	8433.0
175.90	98136.0
177.00	6536.0
177.90	279.0

Instrument :
MSVOA_V
ClientSampleId :
BFB399

m/z	Abundance
35.10	326.0
36.00	2697.0
37.00	6849.0
38.00	5338.0
39.10	2995.0
39.90	438.0
43.00	193.0
44.00	1288.0
45.00	1082.0
46.10	333.0
46.90	1809.0
48.00	911.0
49.00	5392.0
50.00	25816.0
51.00	6950.0
52.00	363.0
53.00	238.0
55.00	394.0
56.00	2132.0
56.90	3655.0
57.90	133.0
59.90	1374.0
61.00	6806.0
62.00	7081.0
63.00	6680.0
64.00	1487.0
65.00	1241.0
65.90	104.0
67.00	430.0
68.00	14824.0
69.00	14100.0
70.00	1045.0
71.90	938.0
73.00	6714.0
74.00	25072.0
75.00	72840.0
76.00	6821.0
77.00	873.0
77.90	838.0
78.90	6579.0
79.90	1551.0
80.90	6230.0
81.90	1555.0
83.00	197.0
85.70	176.0
87.00	6080.0
88.00	6054.0
91.00	710.0
92.00	4066.0
93.00	6699.0
94.00	17672.0
95.00	144384.0
96.00	9441.0
97.00	425.0
103.00	121.0
103.90	590.0
104.70	293.0
105.90	667.0
106.90	227.0
108.00	112.0
110.90	213.0
111.70	103.0
112.90	129.0
114.90	223.0
116.00	544.0
116.90	1287.0
117.80	725.0
118.90	944.0
127.80	486.0
129.00	185.0
129.90	486.0
130.70	196.0
134.60	235.0
135.00	237.0
135.90	110.0
136.90	289.0
140.90	1419.0
141.90	204.0
142.90	2538.0
144.00	124.0
144.90	1073.0
145.80	263.0
147.80	320.0
148.90	179.0
149.80	177.0
152.80	141.0
153.70	201.0
154.90	333.0
156.80	314.0
159.00	154.0
160.80	244.0
170.90	722.0

Instrument :
MSVOA_V
ClientSampleId :
BFB399

171.90	2120.0
173.00	1752.0
174.00	113256.0
174.90	9129.0
175.90	110136.0
177.00	7453.0
177.90	303.0

Instrument :
MSVOA_V
ClientSampleId :
BFB399

m/z	Abundance
35.10	316.0
36.00	2593.0
37.00	6537.0
38.00	5277.0
39.00	2837.0
39.90	445.0
41.10	128.0
43.00	219.0
44.00	1374.0
45.00	1107.0
46.00	402.0
47.00	1751.0
47.90	820.0
49.00	5040.0
50.00	24624.0
51.00	7189.0
52.00	365.0
53.00	287.0
53.90	144.0
55.00	423.0
56.00	2083.0
56.90	3714.0
57.90	128.0
58.80	109.0
59.90	1418.0
61.00	6523.0
62.00	7132.0
63.00	6421.0
64.00	1472.0
65.00	1259.0
65.90	139.0
67.00	420.0
68.00	14127.0
69.00	13871.0
70.00	932.0
71.90	852.0
73.00	6445.0
74.00	24616.0
75.00	72048.0
76.00	6367.0
77.00	960.0
77.90	830.0
78.90	6271.0
79.90	1439.0
80.90	6368.0
81.90	1646.0
82.90	149.0
85.70	196.0
86.90	5803.0
87.90	6198.0
91.00	838.0
92.00	4073.0
93.00	6558.0
94.00	17520.0
95.00	141824.0
96.00	9406.0
97.00	353.0
103.00	105.0
103.80	673.0
104.80	276.0
105.90	666.0
106.80	229.0
108.10	119.0
110.80	228.0
113.00	169.0
114.70	177.0
116.00	524.0
116.90	1223.0
117.90	749.0
118.90	930.0
127.80	438.0
129.00	196.0
129.90	463.0
130.80	204.0
134.70	243.0
136.90	273.0
139.90	132.0
140.90	1519.0
141.90	183.0
142.90	2542.0
145.00	930.0
145.80	334.0
147.70	289.0
148.90	189.0
149.70	173.0
152.80	167.0
153.80	195.0
154.90	331.0
156.80	339.0
159.00	172.0
160.80	174.0
170.80	627.0

Instrument :
MSVOA_V
ClientSampleId :
BFB399

171.90	1954.0
173.00	1722.0
174.00	114384.0
174.90	9143.0
175.90	110704.0
177.00	7666.0
177.90	219.0

Instrument :
MSVOA_V
ClientSampleId :
BFB399