
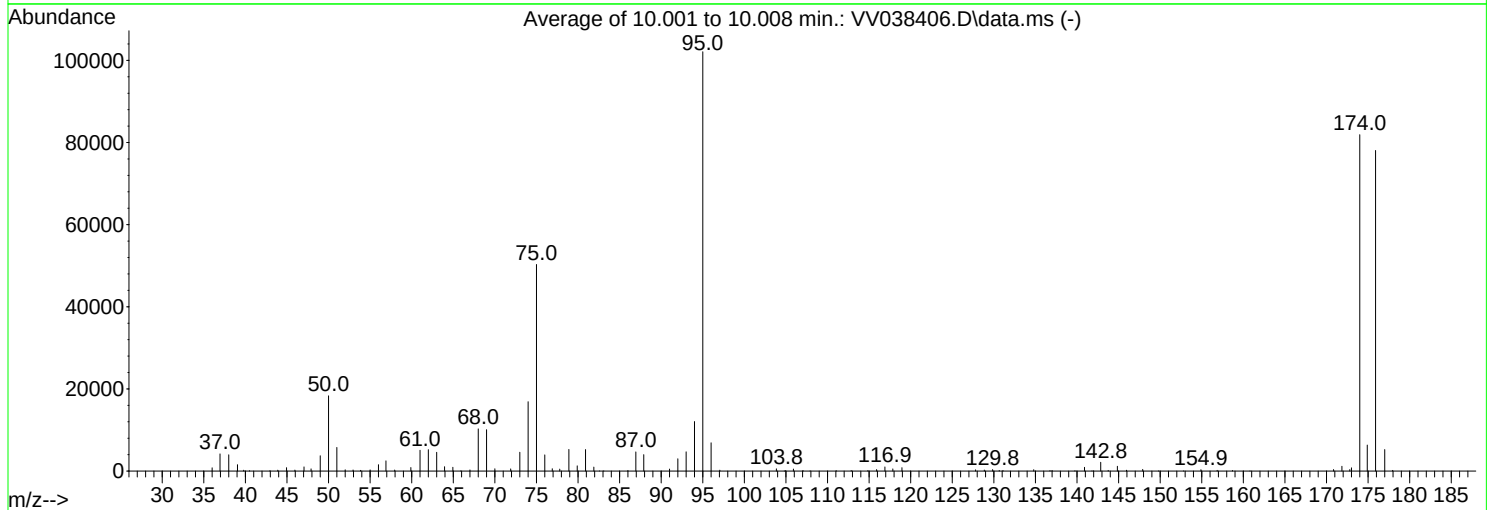


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120424\
Data File : VV038406.D
Acq On : 04 Dec 2024 08:21
Operator : SY/MD
Sample : BFB227
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB227

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM120324.M
Title : TRACE VOA SOM01.0
Last Update : Tue Dec 03 21:43:44 2024

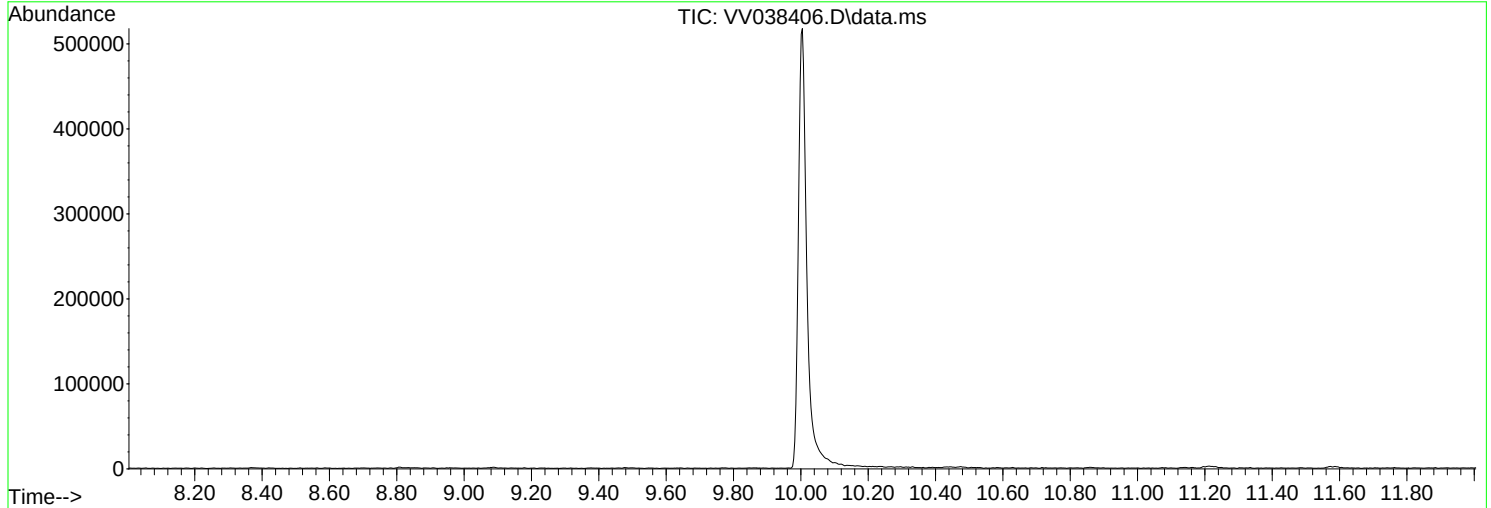

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	18331	PASS
75	95	30	80	49.3	50301	PASS
95	95	100	100	100.0	102109	PASS
96	95	5	9	6.7	6881	PASS
173	174	0.00	2	1.0	803	PASS
174	95	50	120	80.2	81904	PASS
175	174	5	9	7.7	6338	PASS
176	174	95	101	95.3	78067	PASS
177	176	5	9	6.7	5236	PASS

Scan 2775 (9.963 min): VV038406.D\data.ms
BFB227

m/z	Abundance
36.90	120.0
39.90	271.0
43.90	621.0
76.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

m/z	Abundance
36.00	909.0
37.00	4569.0
38.00	4178.0
39.10	1641.0
39.80	444.0
43.90	986.0
44.90	814.0
46.00	304.0
47.10	1072.0
47.90	587.0
49.00	3697.0
50.00	18776.0
51.00	5833.0
52.00	360.0
52.90	257.0
53.80	148.0
55.00	307.0
56.00	1609.0
56.90	2442.0
57.90	263.0
59.90	961.0
61.00	5188.0
62.00	5339.0
63.00	4830.0
63.90	1032.0
65.00	877.0
67.00	346.0
68.00	10435.0
69.00	9986.0
70.00	659.0
71.90	527.0
73.00	4806.0
74.00	17832.0
75.00	52960.0
76.00	4127.0
76.90	683.0
77.80	553.0
78.90	5499.0
79.90	1363.0
80.90	5398.0
81.90	1015.0
86.00	115.0
87.00	4558.0
87.90	4242.0
91.00	484.0
92.00	3097.0
93.00	4729.0
94.00	12474.0
95.00	104832.0
96.00	7095.0
97.00	191.0
103.80	565.0
104.80	150.0
105.90	464.0
107.10	141.0
112.80	141.0
114.80	123.0
115.90	427.0
116.90	1006.0
117.90	553.0
118.90	899.0
127.90	310.0
128.80	268.0
129.80	329.0
130.60	177.0
131.10	129.0
134.80	256.0
136.80	199.0
140.90	970.0
141.80	165.0
142.90	2088.0
143.80	174.0
144.80	1194.0
146.00	202.0
147.90	349.0
154.90	326.0
156.90	192.0
158.70	141.0
170.90	327.0
171.90	1298.0
172.80	1108.0
174.00	81920.0
174.90	6409.0
175.90	77736.0
177.00	5248.0
177.90	182.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

m/z	Abundance
36.00	808.0
37.00	4328.0
38.00	4096.0
39.10	1623.0
39.80	497.0
43.00	121.0
43.90	841.0
45.00	859.0
46.00	236.0
47.10	1014.0
47.90	535.0
49.00	3871.0
50.00	19040.0
51.00	5976.0
52.00	328.0
52.90	288.0
53.80	176.0
55.00	309.0
56.00	1618.0
56.90	2608.0
58.00	278.0
59.90	883.0
61.00	5335.0
62.00	5400.0
63.00	4745.0
63.90	1082.0
65.00	987.0
65.90	102.0
67.00	284.0
68.00	10627.0
69.00	10489.0
70.00	558.0
71.90	564.0
73.00	4692.0
74.00	17448.0
75.00	51744.0
76.00	4012.0
77.00	720.0
77.80	517.0
78.90	5444.0
79.90	1286.0
80.90	5365.0
81.90	1023.0
83.10	106.0
86.00	134.0
86.90	4774.0
87.90	4141.0
91.00	531.0
92.00	3110.0
93.00	4881.0
94.00	12505.0
95.00	105040.0
96.00	7219.0
97.00	227.0
103.80	594.0
105.00	145.0
105.90	520.0
107.10	137.0
111.10	116.0
112.80	131.0
114.90	111.0
115.90	378.0
116.90	1062.0
117.80	539.0
118.90	857.0
127.80	313.0
128.90	281.0
129.90	393.0
130.60	155.0
131.10	138.0
134.80	366.0
137.00	200.0
139.80	112.0
140.90	905.0
142.00	130.0
142.90	2215.0
143.80	156.0
144.90	1225.0
146.00	215.0
147.90	457.0
154.90	363.0
156.90	186.0
158.70	154.0
170.80	383.0
171.90	1194.0
173.00	1218.0
174.00	84288.0
174.90	6589.0
175.90	80768.0
177.00	5435.0
178.00	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

m/z	Abundance
36.00	679.0
37.00	4034.0
38.00	3633.0
39.00	1423.0
39.80	495.0
40.50	241.0
42.90	148.0
44.00	723.0
45.00	835.0
45.90	191.0
47.00	965.0
47.90	495.0
49.00	3637.0
50.00	17176.0
51.00	5440.0
52.00	267.0
53.00	261.0
53.90	195.0
55.00	273.0
56.00	1452.0
56.90	2432.0
58.00	249.0
59.90	749.0
61.00	4714.0
62.00	4918.0
63.00	4149.0
64.00	1091.0
64.90	906.0
66.90	209.0
68.00	9772.0
69.00	9761.0
70.00	471.0
71.90	493.0
73.00	4253.0
74.00	15376.0
75.00	46200.0
76.00	3677.0
76.90	673.0
77.80	358.0
78.90	4876.0
79.90	1200.0
80.90	4962.0
81.90	900.0
82.60	118.0
86.00	120.0
87.00	4677.0
87.90	3613.0
91.00	479.0
92.00	2785.0
93.00	4446.0
94.00	11212.0
95.00	96456.0
96.00	6328.0
97.10	269.0
103.90	500.0
104.90	123.0
105.90	503.0
107.00	113.0
107.90	128.0
111.00	128.0
112.90	113.0
114.90	115.0
115.90	309.0
116.90	962.0
117.80	480.0
119.00	737.0
127.70	288.0
128.90	215.0
129.90	368.0
130.70	123.0
131.10	117.0
134.80	415.0
136.70	174.0
137.00	190.0
139.70	138.0
140.90	879.0
142.80	2121.0
143.70	154.0
144.90	1084.0
145.90	237.0
147.90	430.0
149.80	103.0
152.80	108.0
154.90	335.0
156.80	170.0
158.70	144.0
160.80	105.0
170.80	413.0
171.80	1021.0
173.00	1192.0
174.00	79504.0
174.90	6015.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

175.90

177.00

178.00

75696.0

5025.0

127.0

Instrument :

MSVOA_V

ClientSampleId :

BFB227