

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120524\
 Data File : VV038414.D
 Acq On : 05 Dec 2024 11:34
 Operator : SY/MD
 Sample : VV1205WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK258

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120224WMA.M
 Title : VOC Analysis

Signal : TIC: VV038414.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.211	49	53	55	rBV3	2864	2447	0.11%	0.015%
2	1.275	66	73	87	rBV	310191	330354	14.62%	1.975%
3	1.526	144	151	166	rVB	257525	309399	13.69%	1.850%
4	2.053	305	315	333	rBV	536859	777587	34.41%	4.649%
5	2.233	366	371	383	rVB2	3677	5518	0.24%	0.033%
6	2.439	430	435	436	rBV4	1799	1488	0.07%	0.009%
7	2.506	453	456	458	rVB4	1043	592	0.03%	0.004%
8	2.613	480	489	491	rBV3	809	1237	0.05%	0.007%
9	2.693	509	514	517	rBV5	1264	1179	0.05%	0.007%
10	2.969	590	600	602	rBV5	1746	2028	0.09%	0.012%
11	3.027	615	618	622	rBV4	753	614	0.03%	0.004%
12	3.162	658	660	666	rVB4	839	700	0.03%	0.004%
13	3.204	666	673	676	rBV2	1118	1136	0.05%	0.007%
14	3.368	721	724	728	rVB2	891	678	0.03%	0.004%
15	3.477	749	758	759	rBV4	678	856	0.04%	0.005%
16	3.532	772	775	780	rVB3	734	622	0.03%	0.004%
17	3.786	845	854	882	rBV	144357	428087	18.94%	2.560%
18	4.240	979	995	1031	rBV	353406	926086	40.98%	5.537%
19	4.436	1053	1056	1060	rBV4	1034	664	0.03%	0.004%
20	4.516	1078	1081	1088	rBV8	967	1076	0.05%	0.006%
21	4.693	1133	1136	1139	rBV3	763	608	0.03%	0.004%
22	4.802	1165	1170	1171	rBV2	802	622	0.03%	0.004%
23	4.947	1200	1215	1258	rBV2	843175	2259990	100.00%	13.513%
24	5.297	1320	1324	1326	rBV4	706	517	0.02%	0.003%
25	5.329	1332	1334	1339	rBV3	674	587	0.03%	0.004%
26	5.471	1373	1378	1382	rBV5	1026	1112	0.05%	0.007%
27	5.526	1385	1395	1437	rBV	571606	1232191	54.52%	7.368%
28	5.767	1468	1470	1475	rVB4	963	662	0.03%	0.004%
29	5.831	1480	1490	1506	rBV8	11320	27736	1.23%	0.166%
30	5.979	1524	1536	1577	rVV	480076	1025406	45.37%	6.131%
31	6.182	1597	1599	1604	rVB6	1339	791	0.04%	0.005%
32	6.442	1676	1680	1682	rBV5	1059	746	0.03%	0.004%
33	6.471	1685	1689	1695	rVB6	1335	1233	0.05%	0.007%
34	6.574	1718	1721	1723	rVB3	823	513	0.02%	0.003%
35	6.612	1729	1733	1739	rBV6	643	806	0.04%	0.005%
36	6.815	1791	1796	1799	rBV6	827	815	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120524\
 Data File : VV038414.D
 Acq On : 05 Dec 2024 11:34
 Operator : SY/MD
 Sample : VV1205WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK258

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120224WMA.M
 Title : VOC Analysis

37	6.908	1814	1825	1858	rBV	233300	478416	21.17%	2.861%
38	7.236	1916	1927	1971	rBV	949460	1728808	76.50%	10.337%
39	7.548	2015	2024	2050	rBV	162635	327014	14.47%	1.955%
40	7.812	2103	2106	2108	rBV3	919	488	0.02%	0.003%
41	7.902	2130	2134	2138	rBV4	2002	2215	0.10%	0.013%
42	7.966	2150	2154	2157	rVB4	671	513	0.02%	0.003%
43	8.021	2162	2171	2215	rBV	467653	1030907	45.62%	6.164%
44	8.484	2313	2315	2318	rBV5	610	508	0.02%	0.003%
45	8.522	2323	2327	2330	rBV4	1131	961	0.04%	0.006%
46	8.632	2355	2361	2365	rBV5	1180	1309	0.06%	0.008%
47	8.657	2367	2369	2374	rVV5	877	649	0.03%	0.004%
48	8.776	2396	2406	2445	rBV	918199	1601210	70.85%	9.574%
49	9.043	2483	2489	2494	rBV6	1446	1771	0.08%	0.011%
50	9.291	2562	2566	2567	rBV3	831	525	0.02%	0.003%
51	9.300	2567	2569	2574	rVB3	1080	912	0.04%	0.005%
52	9.426	2603	2608	2614	rBV5	860	892	0.04%	0.005%
53	9.493	2627	2629	2635	rVB4	1466	1011	0.04%	0.006%
54	9.538	2638	2643	2646	rBV4	1201	978	0.04%	0.006%
55	9.651	2675	2678	2681	rBV3	1178	818	0.04%	0.005%
56	9.976	2777	2779	2783	rVB4	774	533	0.02%	0.003%
57	10.008	2783	2789	2792	rBV5	873	946	0.04%	0.006%
58	10.053	2799	2803	2808	rBV5	1030	1124	0.05%	0.007%
59	10.146	2820	2832	2862	rBV	692490	1151845	50.97%	6.887%
60	10.413	2912	2915	2918	rBV3	746	551	0.02%	0.003%
61	10.461	2925	2930	2931	rBV3	742	506	0.02%	0.003%
62	10.538	2950	2954	2956	rBV3	843	522	0.02%	0.003%
63	10.587	2966	2969	2975	rVB6	820	739	0.03%	0.004%
64	10.776	3024	3028	3031	rBV3	1253	932	0.04%	0.006%
65	10.866	3049	3056	3057	rBV4	1838	1862	0.08%	0.011%
66	10.976	3086	3090	3095	rBV5	867	737	0.03%	0.004%
67	11.008	3095	3100	3102	rBV4	732	651	0.03%	0.004%
68	11.130	3130	3138	3142	rBV5	4544	5937	0.26%	0.035%
69	11.178	3142	3153	3187	rVV	830335	1369894	60.62%	8.191%
70	11.464	3237	3242	3244	rBV3	722	700	0.03%	0.004%
71	11.503	3249	3254	3255	rBV4	919	651	0.03%	0.004%
72	11.551	3258	3269	3293	rBV	958403	1565634	69.28%	9.361%
73	12.075	3429	3432	3436	rVB3	884	743	0.03%	0.004%
74	12.194	3465	3469	3472	rVV5	605	574	0.03%	0.003%
75	12.371	3521	3524	3529	rBV5	732	554	0.02%	0.003%
76	12.403	3532	3534	3536	rVB2	1072	502	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120524\
 Data File : VV038414.D
 Acq On : 05 Dec 2024 11:34
 Operator : SY/MD
 Sample : VV1205WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK258

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120224WMA.M
 Title : VOC Analysis

77	12.590	3585	3592	3594	rBV5	4213	4879	0.22%	0.029%
78	12.670	3613	3617	3622	rVB5	857	765	0.03%	0.005%
79	12.786	3649	3653	3657	rVB3	755	628	0.03%	0.004%
80	12.840	3664	3670	3678	rBV6	1033	1440	0.06%	0.009%
81	12.924	3693	3696	3699	rBV2	741	502	0.02%	0.003%
82	13.024	3724	3727	3730	rVV4	1018	600	0.03%	0.004%
83	13.104	3749	3752	3756	rVB5	663	576	0.03%	0.003%
84	13.204	3776	3783	3799	rBV5	7060	13970	0.62%	0.084%
85	13.262	3799	3801	3806	rVB4	639	498	0.02%	0.003%
86	13.339	3822	3825	3828	rBV4	938	608	0.03%	0.004%
87	13.355	3828	3830	3833	rVB2	1016	576	0.03%	0.003%
88	13.445	3849	3858	3876	rBV2	19768	43209	1.91%	0.258%
89	13.683	3924	3932	3939	rBV5	10001	15755	0.70%	0.094%
90	13.982	4023	4025	4028	rVB2	1116	546	0.02%	0.003%
91	14.065	4048	4051	4054	rVB4	782	519	0.02%	0.003%
92	14.120	4065	4068	4072	rVB4	958	827	0.04%	0.005%
93	14.236	4099	4104	4105	rBV3	704	536	0.02%	0.003%
94	14.364	4141	4144	4148	rBV4	760	502	0.02%	0.003%
95	14.387	4149	4151	4156	rVB5	1251	794	0.04%	0.005%
96	14.577	4208	4210	4216	rVB6	766	565	0.03%	0.003%
97	14.609	4218	4220	4224	rVV3	1132	738	0.03%	0.004%
98	14.644	4228	4231	4233	rBV4	698	515	0.02%	0.003%
99	14.799	4277	4279	4285	rBV5	604	525	0.02%	0.003%
100	15.496	4493	4496	4501	rBV5	1351	1577	0.07%	0.009%




Sum of corrected areas: 16724375

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120524\
Data File : VV038414.D
Acq On : 05 Dec 2024 11:34
Operator : SY/MD
Sample : VV1205WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK258

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

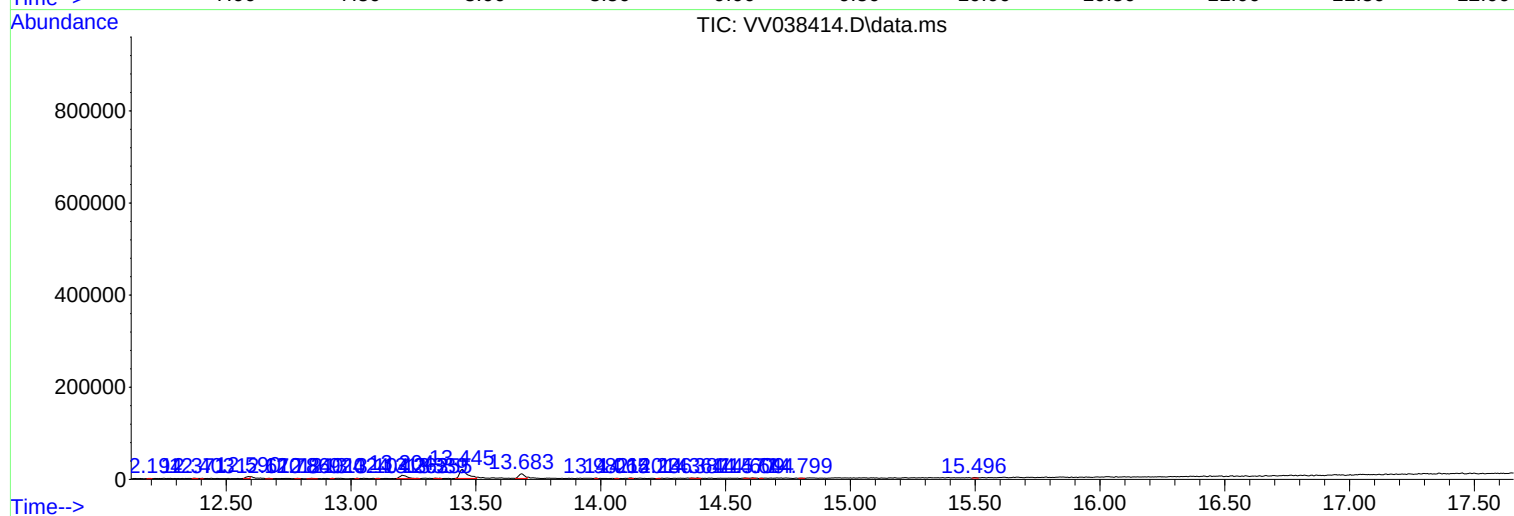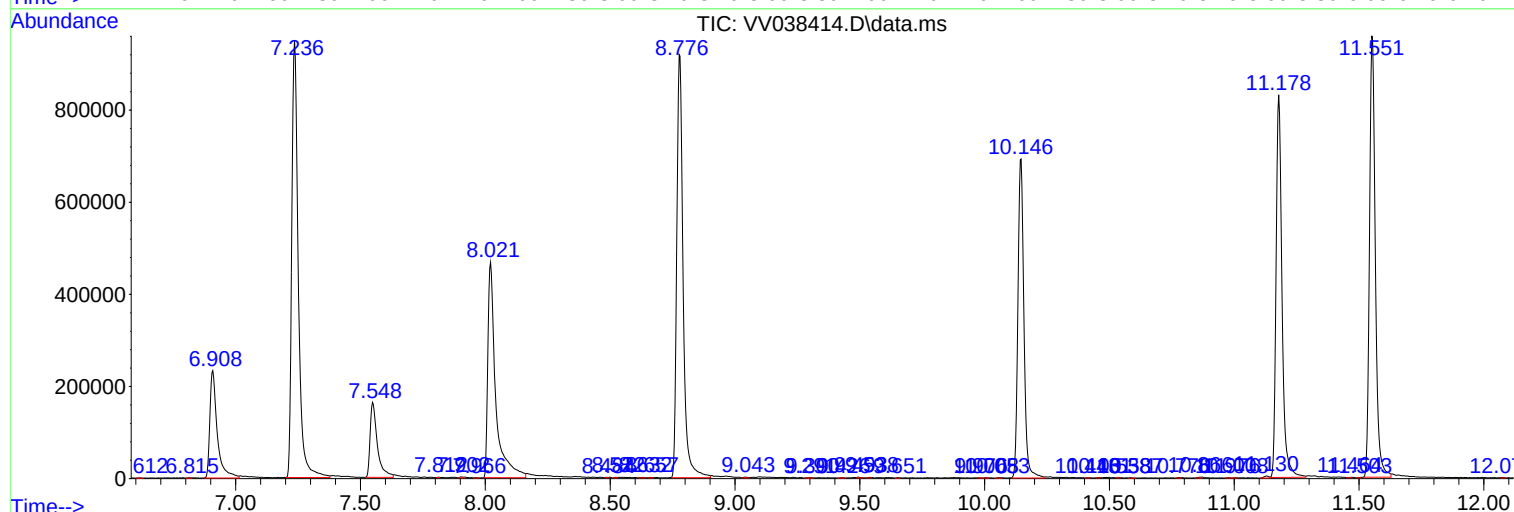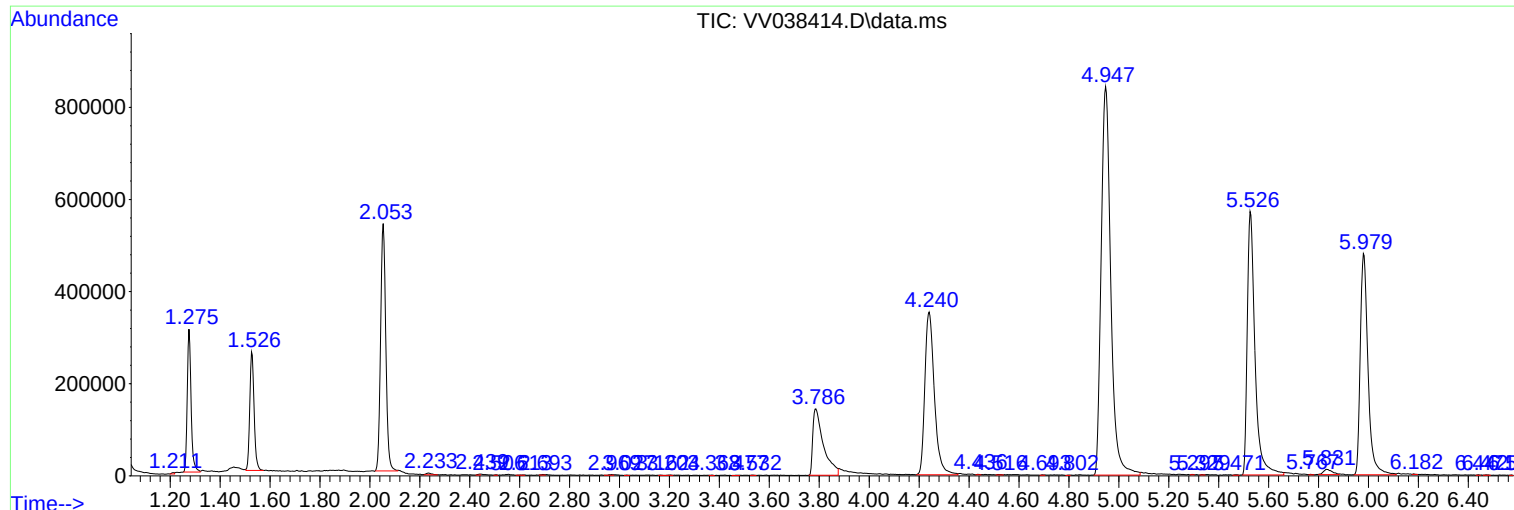

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120524\
Data File : VV038414.D
Acq On : 05 Dec 2024 11:34
Operator : SY/MD
Sample : VV1205WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK258

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120524\
Data File : VV038414.D
Acq On : 05 Dec 2024 11:34
Operator : SY/MD
Sample : VV1205WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK258

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM120224WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc