

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120624\
 Data File : VV038421.D
 Acq On : 05 Dec 2024 17:15
 Operator : SY/MD
 Sample : P5111-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 06 05:40:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 06 05:39:27 2024
 Response via : Initial Calibration


Compound	R.T. QIon		Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	253681	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	283338	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	111571	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	110537	5.685	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	113.600%	
7) Chloroethane-d5	1.529	69	93448	5.941	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	118.800%	
11) 1,1-Dichloroethene-d2	2.053	65	47710	5.702	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	114.000%	
20) 2-Butanone-d5	3.789	46	192199	49.412	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	98.820%	
24) Chloroform-d	4.236	84	197109	5.223	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.400%	
26) 1,2-Dichloroethane-d4	4.934	65	96428	5.695	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	113.800%	
32) Benzene-d6	4.950	84	367487	5.018	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	100.400%	
36) 1,2-Dichloropropane-d6	5.979	67	116238	5.158	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	103.200%	
41) Toluene-d8	7.236	98	292621	4.318	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	86.400%	
43) trans-1,3-Dichloroprop...	7.555	79	38123	4.550	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	91.000%	
46) 2-Hexanone-d5	8.021	63	133340	40.944	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	81.880%	
56) 1,1,2,2-Tetrachloroeth...	10.146	84	85243	4.456	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	89.200%	
66) 1,2-Dichlorobenzene-d4	11.554	152	105322	5.540	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	110.800%	
Target Compounds						Qvalue
13) Acetone	2.124	43	52322	18.187	ug/L	99
15) Methyl Acetate	2.281	43	17217	2.464	ug/L #	48
35) Methylcyclohexane	5.979	83	29752	0.969	ug/L #	19
61) 1,2,3-Trichloropropane	11.178	75	14331	1.500	ug/L #	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120624\
Data File : VV038421.D
Acq On : 05 Dec 2024 17:15
Operator : SY/MD
Sample : P5111-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Dec 06 05:40:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 06 05:39:27 2024
Response via : Initial Calibration

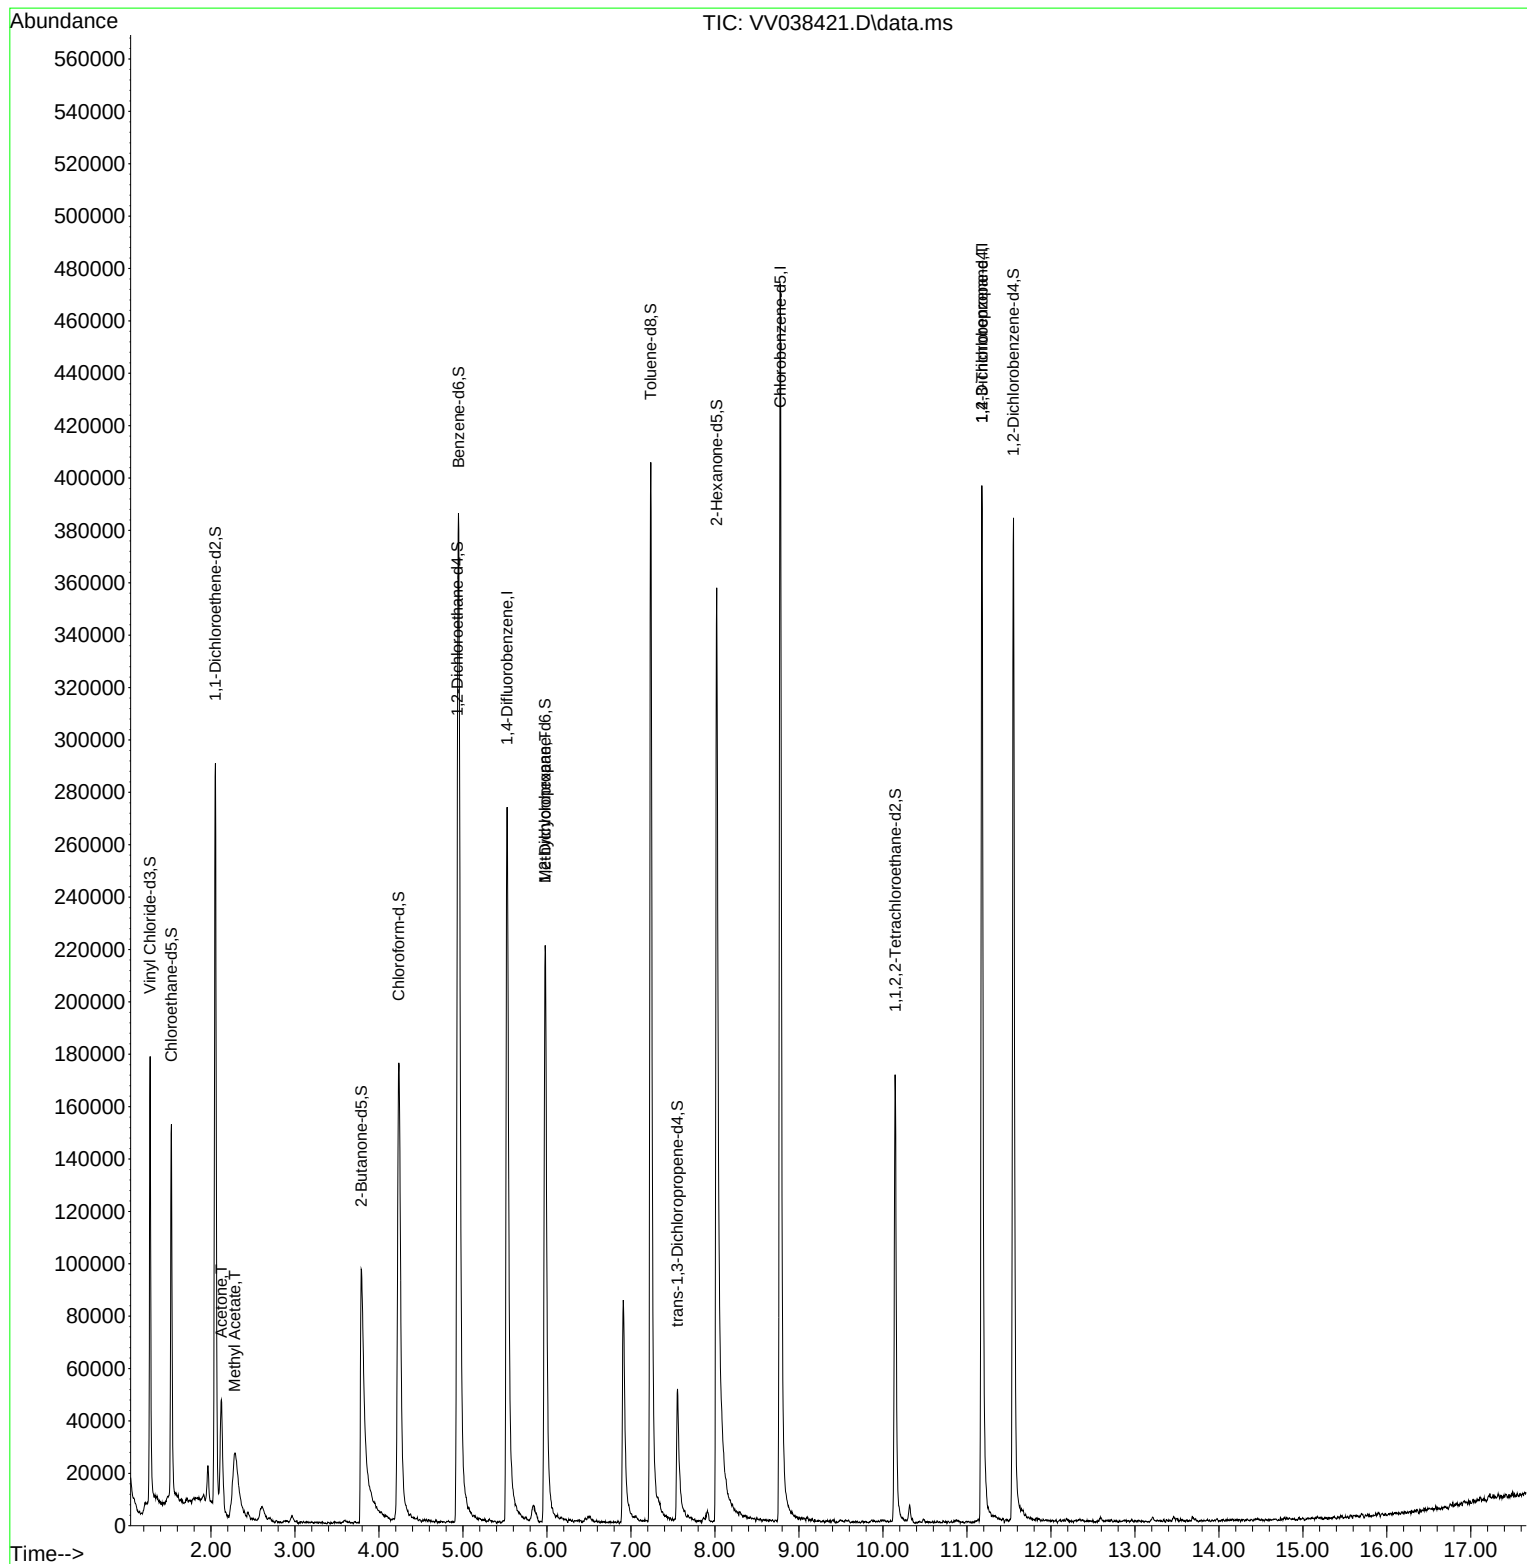



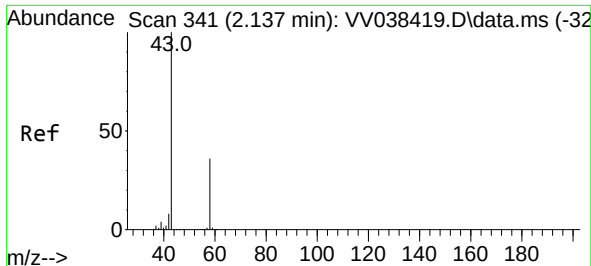


#13
Acetone
Concen: 18.187 ug/L
RT: 2.124 min Scan# 31
Delta R.T. -0.013 min
Lab File: VV038421.D
Acq: 05 Dec 2024 17:15

Instrument :
MSVOA_V
ClientSampleId :



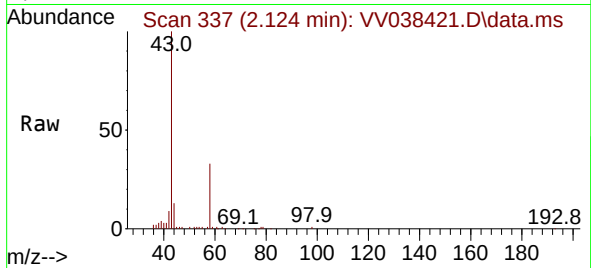



Tgt Ion: 43 Resp: 52322
Ion Ratio Lower Upper
43 100
58 34.0 0.0 67.2

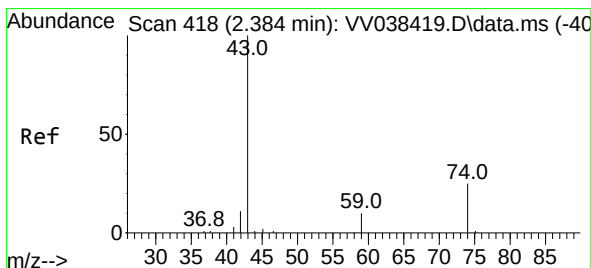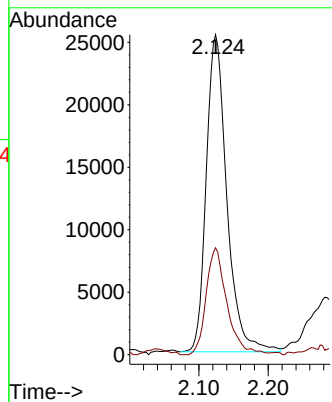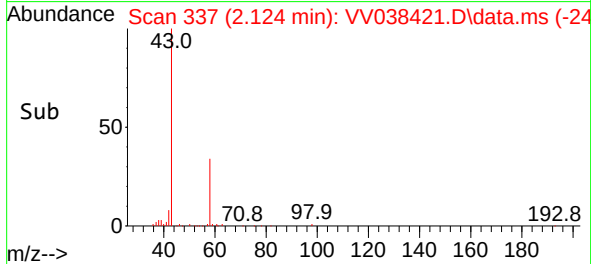

#15
Methyl Acetate
Concen: 2.464 ug/L
RT: 2.281 min Scan# 386
Delta R.T. -0.103 min
Lab File: VV038421.D
Acq: 05 Dec 2024 17:15

Tgt Ion: 43 Resp: 17217
Ion Ratio Lower Upper
43 100
74 0.4 22.4 33.6#

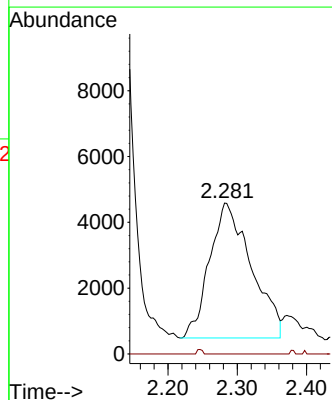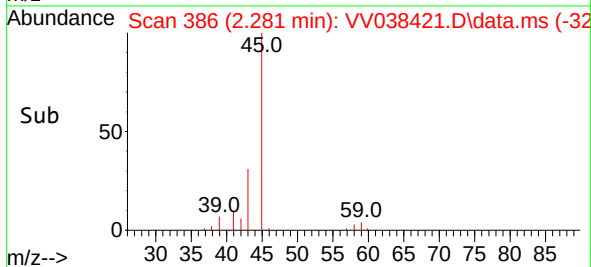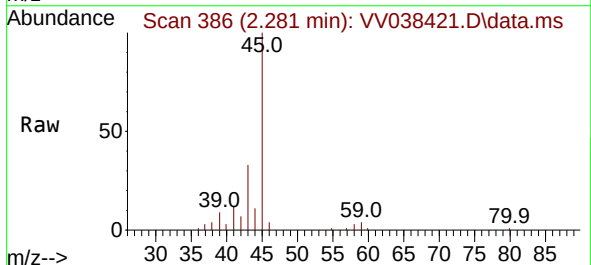

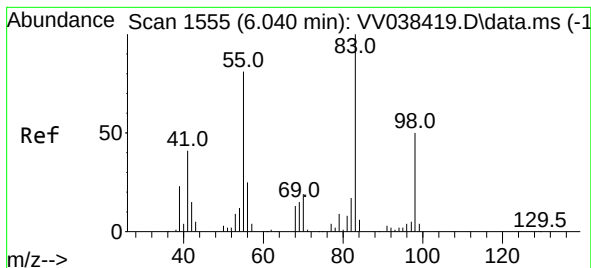

#35

Methylcyclohexane

Concen: 0.969 ug/L

RT: 5.979 min Scan# 1

Delta R.T. -0.061 min


Lab File: VV038421.D

Acq: 05 Dec 2024 17:15




Instrument :

MSVOA_V

ClientSampleId :

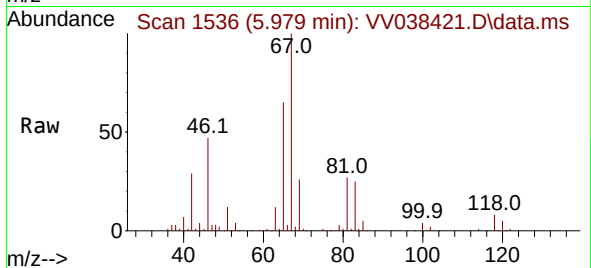

Tgt Ion:	83	Resp:	29752
Ion	Ratio	Lower	Upper
83	100		
55	0.2	59.7	89.5#
98	1.0	39.0	58.4#

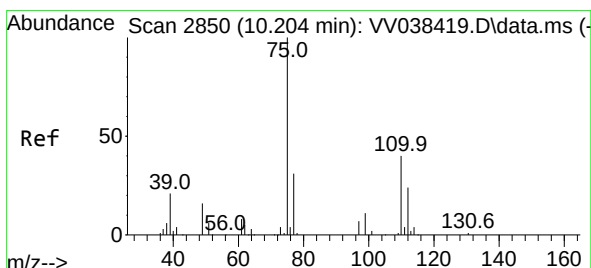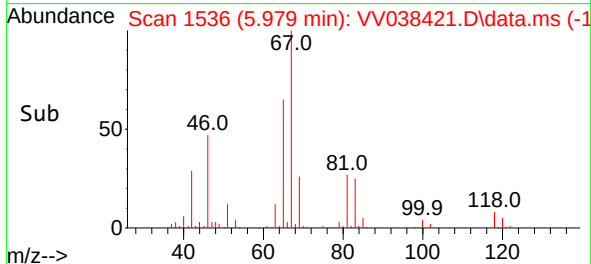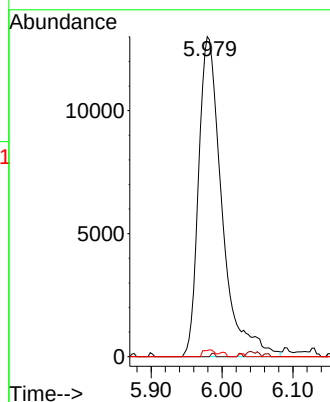

#61

1,2,3-Trichloropropane

Concen: 1.500 ug/L

RT: 11.178 min Scan# 3153

Delta R.T. 0.974 min

Lab File: VV038421.D

Acq: 05 Dec 2024 17:15

Tgt Ion:	75	Resp:	14331
Ion	Ratio	Lower	Upper
75	100		
77	28.8	26.4	39.6
110	3.1	32.3	48.5#

