

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120624\
 Data File : VV038421.D
 Acq On : 05 Dec 2024 17:15
 Operator : SY/MD
 Sample : P5111-12
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG461

Quant Time: Dec 06 05:40:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 06 05:39:27 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		5.526	114	253681	5.000	ug/L	0.00
28) Chlorobenzene-d5		8.776	117	283338	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.178	152	111571	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.275	65	110537	5.685	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	113.600%	
7) Chloroethane-d5		1.529	69	93448	5.941	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	118.800%	
11) 1,1-Dichloroethene-d2		2.053	65	47710	5.702	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	114.000%	
20) 2-Butanone-d5		3.789	46	192199	49.412	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.820%	
24) Chloroform-d		4.236	84	197109	5.223	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.400%	
26) 1,2-Dichloroethane-d4		4.934	65	96428	5.695	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	113.800%	
32) Benzene-d6		4.950	84	367487	5.018	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.400%	
36) 1,2-Dichloropropane-d6		5.979	67	116238	5.158	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	103.200%	
41) Toluene-d8		7.236	98	292621	4.318	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.400%	
43) trans-1,3-Dichloroprop...		7.555	79	38123	4.550	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.000%	
46) 2-Hexanone-d5		8.021	63	133340	40.944	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.880%	
56) 1,1,2,2-Tetrachloroeth...		10.146	84	85243	4.456	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.200%	
66) 1,2-Dichlorobenzene-d4		11.554	152	105322	5.540	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.800%	
Target Compounds							Qvalue
13) Acetone		2.124	43	52322	18.187	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120624\
Data File : VV038421.D
Acq On : 05 Dec 2024 17:15
Operator : SY/MD
Sample : P5111-12
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG461

Quant Time: Dec 06 05:40:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 06 05:39:27 2024
Response via : Initial Calibration

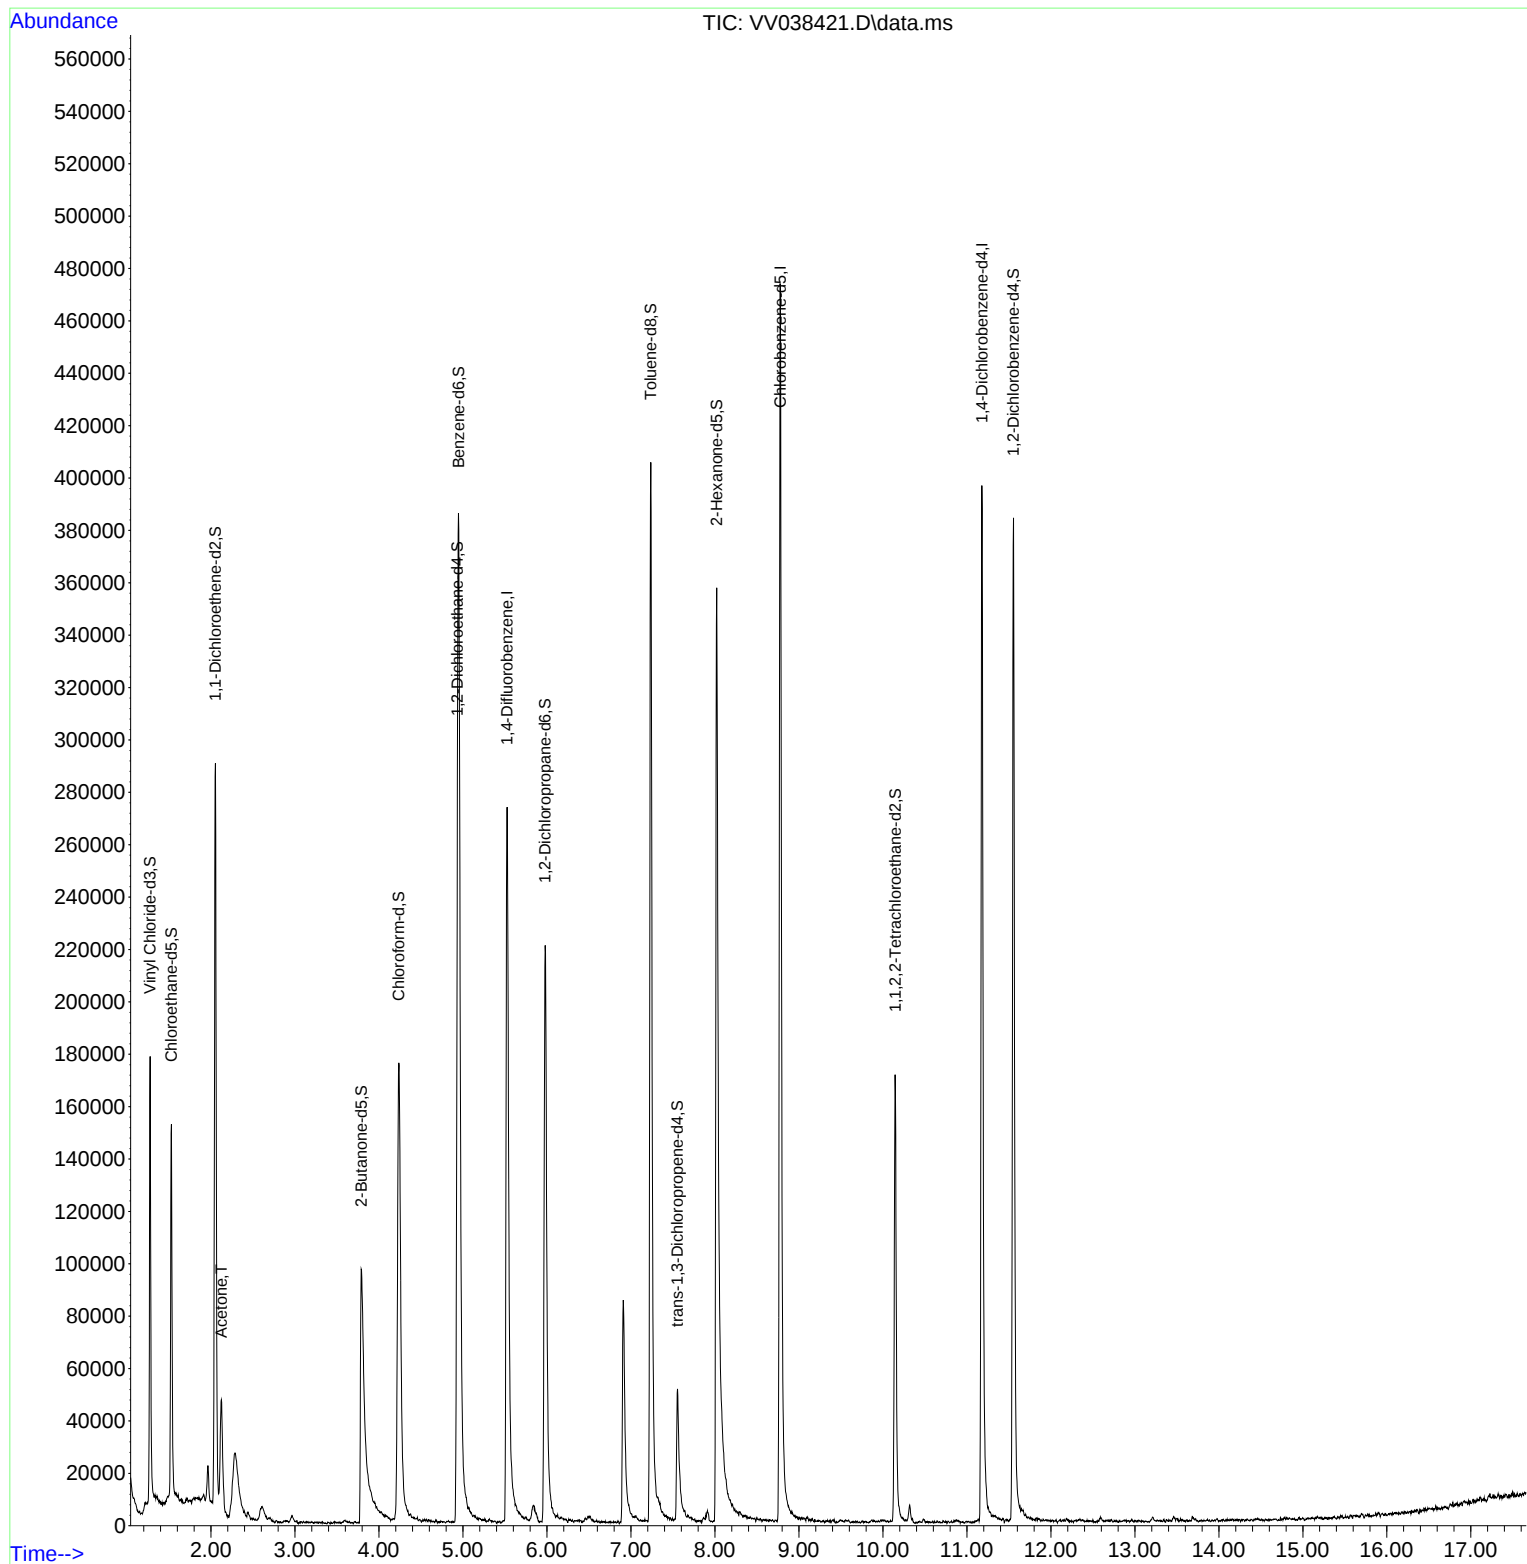

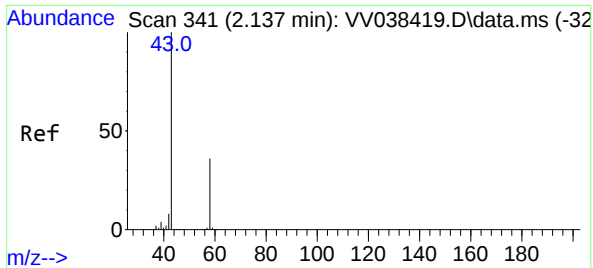

#13
Acetone
Concen: 18.187 ug/L
RT: 2.124 min Scan# 31
Delta R.T. -0.013 min
Lab File: VV038421.D
Acq: 05 Dec 2024 17:15

Instrument :
MSVOA_V
ClientSampleId :
BG461

Tgt Ion: 43 Resp: 52322
Ion Ratio Lower Upper
43 100
58 34.0 0.0 67.2

