

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120624\
 Data File : VV038422.D
 Acq On : 05 Dec 2024 17:40
 Operator : SY/MD
 Sample : P5111-13
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG462

Quant Time: Dec 06 05:40:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 06 05:39:27 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	228519	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	245911	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.182	152	96523	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	101318	5.785	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	115.600%	
7) Chloroethane-d5	1.529	69	83880	5.920	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	118.400%	
11) 1,1-Dichloroethene-d2	2.053	65	43797	5.811	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	116.200%	
20) 2-Butanone-d5	3.793	46	176100	50.258	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	100.520%	
24) Chloroform-d	4.240	84	180009	5.295	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	106.000%	
26) 1,2-Dichloroethane-d4	4.934	65	86270	5.656	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	113.200%	
32) Benzene-d6	4.950	84	331108	5.210	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	104.200%	
36) 1,2-Dichloropropane-d6	5.982	67	105683	5.404	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	108.000%	
41) Toluene-d8	7.236	98	262642	4.466	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	89.400%	
43) trans-1,3-Dichloroprop...	7.558	79	32864	4.520	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.400%	
46) 2-Hexanone-d5	8.021	63	126415	44.726	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	89.460%	
56) 1,1,2,2-Tetrachloroeth...	10.146	84	82339	4.959	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	99.200%	
66) 1,2-Dichlorobenzene-d4	11.555	152	98203	5.971	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	119.400%	
Target Compounds						
13) Acetone	2.121	43	55758	21.516	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120624\
Data File : VV038422.D
Acq On : 05 Dec 2024 17:40
Operator : SY/MD
Sample : P5111-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG462

Quant Time: Dec 06 05:40:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 06 05:39:27 2024
Response via : Initial Calibration

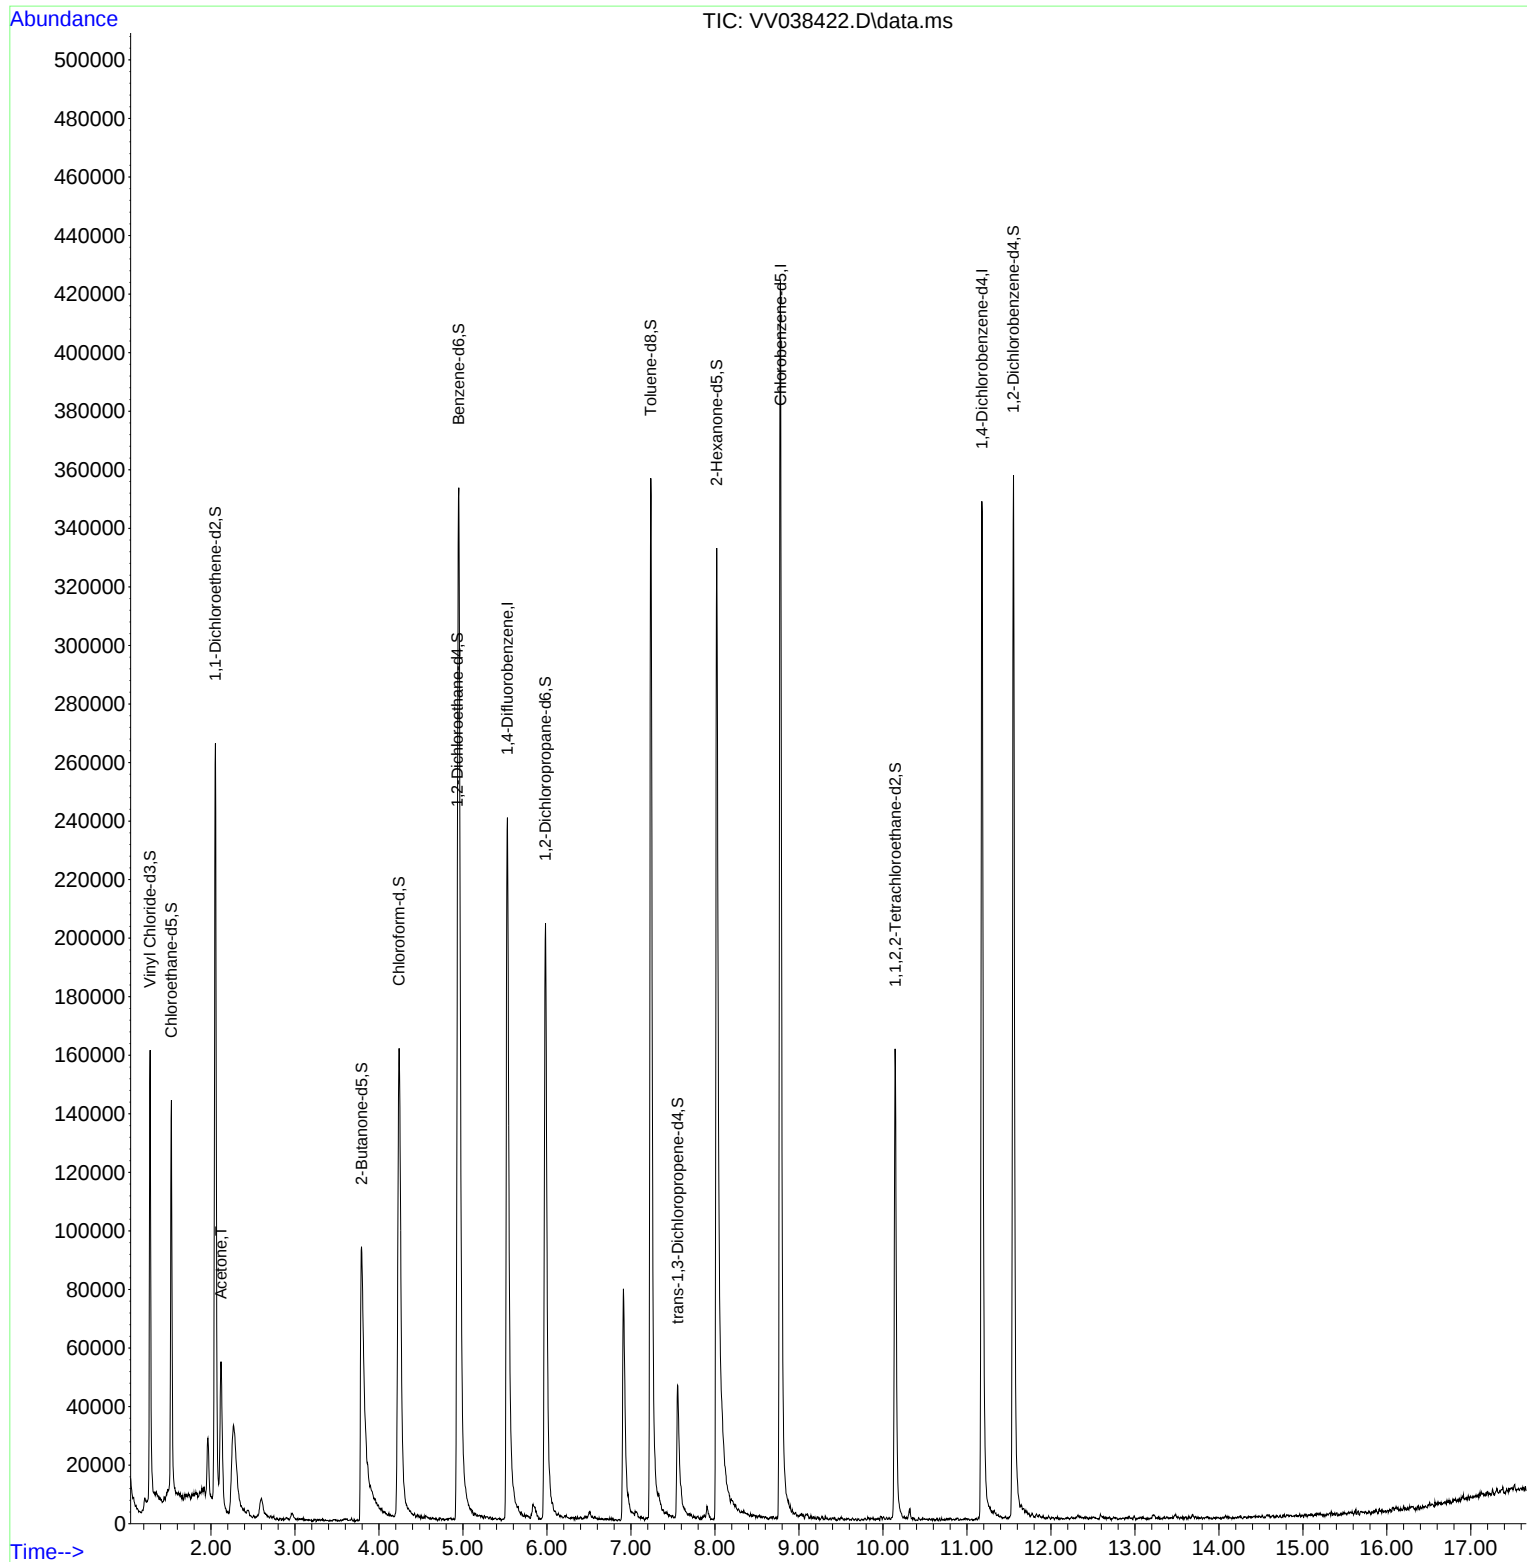

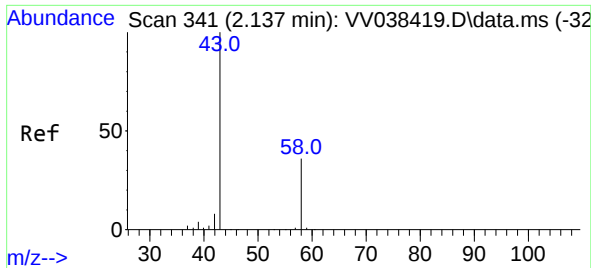

#13

Acetone

Concen: 21.516 ug/L

RT: 2.121 min Scan# 31

Delta R.T. -0.016 min

Lab File: VV038422.D


Acq: 05 Dec 2024 17:40

Instrument :

MSVOA_V

ClientSampleId :

BG462

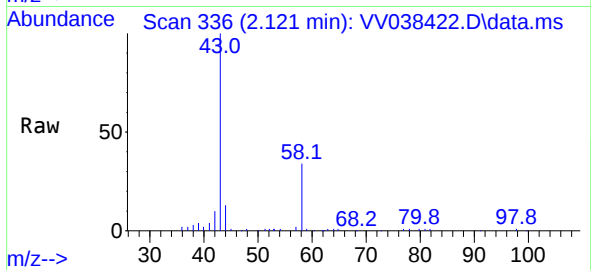

Tgt Ion: 43 Resp: 55758

Ion Ratio Lower Upper

43 100

58 32.1 0.0 67.2

