

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120624\
 Data File : VV038427.D
 Acq On : 05 Dec 2024 19:42
 Operator : SY/MD
 Sample : P5111-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG450

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	13	20	34	rVB	164904	176077	5.88%	1.279%
2	1.275	66	73	88	rBV	152934	168772	5.63%	1.226%
3	1.529	143	152	160	rBV	130981	158012	5.27%	1.148%
4	2.056	305	316	331	rBV3	356275	597565	19.95%	4.342%
5	2.285	365	387	428	rBV2	26056	129942	4.34%	0.944%
6	3.802	848	859	889	rBV2	225229	680212	22.71%	4.943%
7	4.240	980	995	1023	rBV2	161833	450278	15.03%	3.272%
8	4.506	1061	1078	1095	rBV4	15659	41696	1.39%	0.303%
9	4.950	1197	1216	1262	rBV2	351847	950625	31.73%	6.908%
10	5.529	1386	1396	1425	rBV	235951	524419	17.51%	3.811%
11	5.822	1475	1487	1526	rBV	1171985	2426642	81.01%	17.633%
12	5.982	1526	1537	1564	rVV	211690	470783	15.72%	3.421%
13	6.912	1816	1826	1852	rBV2	79572	176632	5.90%	1.283%
14	7.236	1918	1927	1949	rBV	362931	684767	22.86%	4.976%
15	7.555	2016	2026	2045	rBV	46450	101128	3.38%	0.735%
16	7.895	2113	2132	2161	rBV	1750329	2995634	100.00%	21.767%
17	8.021	2163	2171	2223	rVB	363080	849386	28.35%	6.172%
18	8.780	2397	2407	2430	rBV	415976	728198	24.31%	5.291%
19	10.146	2821	2832	2854	rBV	168012	277912	9.28%	2.019%
20	11.178	3143	3153	3177	rBV	338737	579910	19.36%	4.214%
21	11.554	3256	3270	3296	rBV	345894	593531	19.81%	4.313%




Sum of corrected areas: 13762121

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120624\
Data File : VV038427.D
Acq On : 05 Dec 2024 19:42
Operator : SY/MD
Sample : P5111-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG450

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

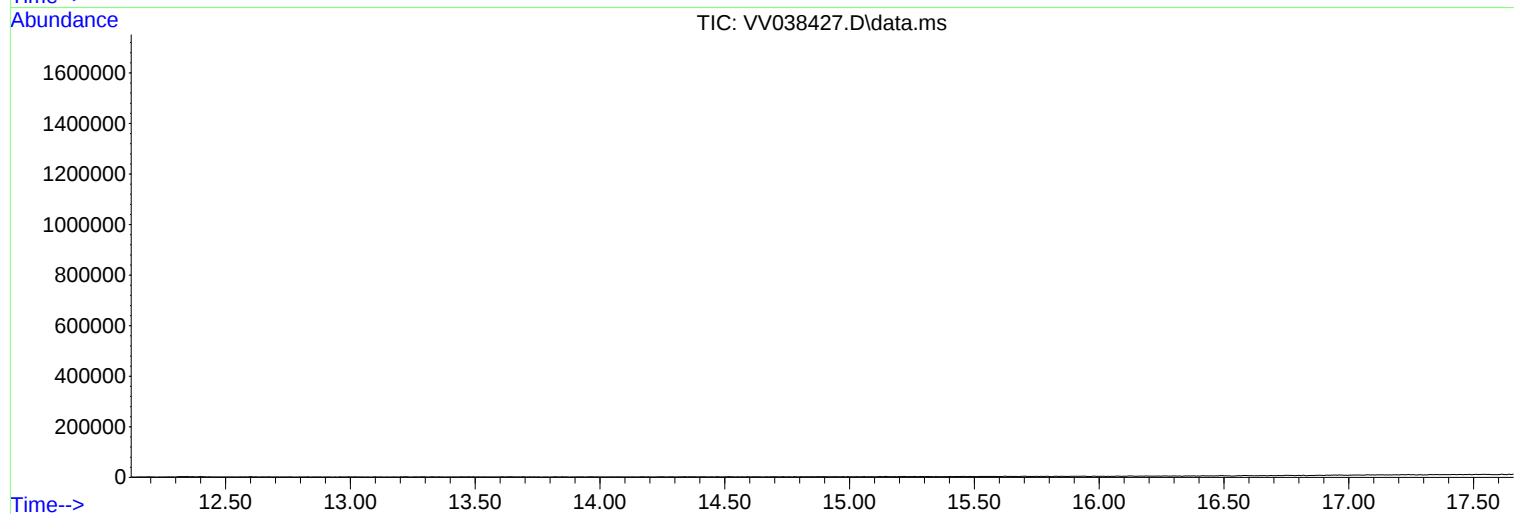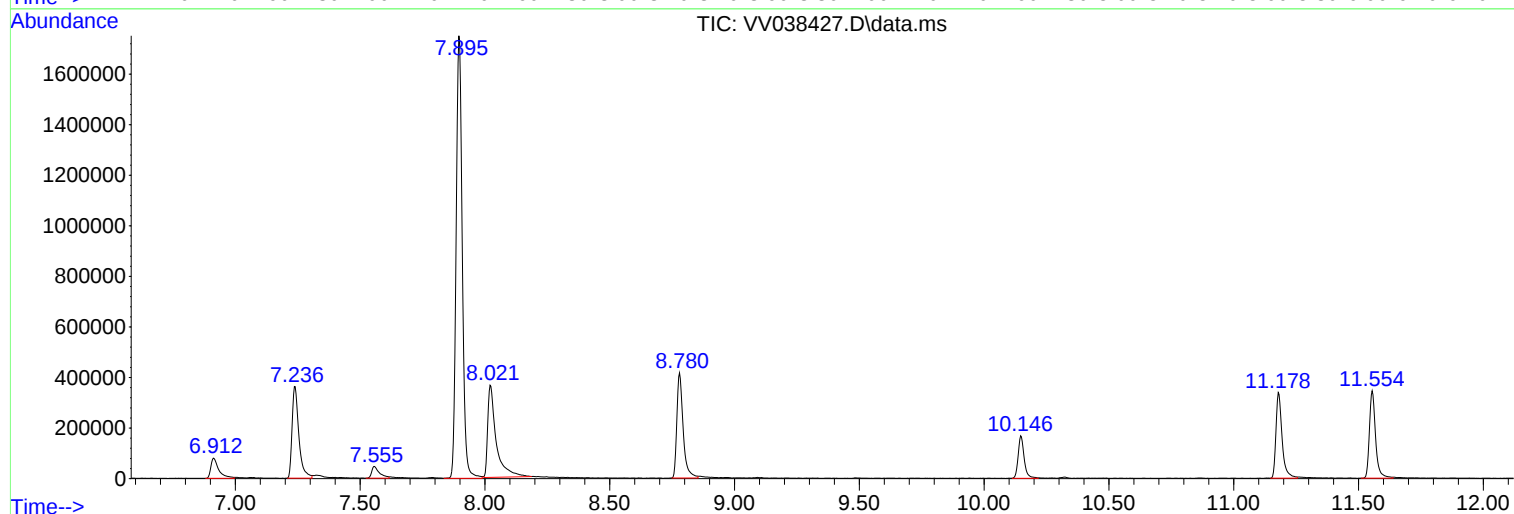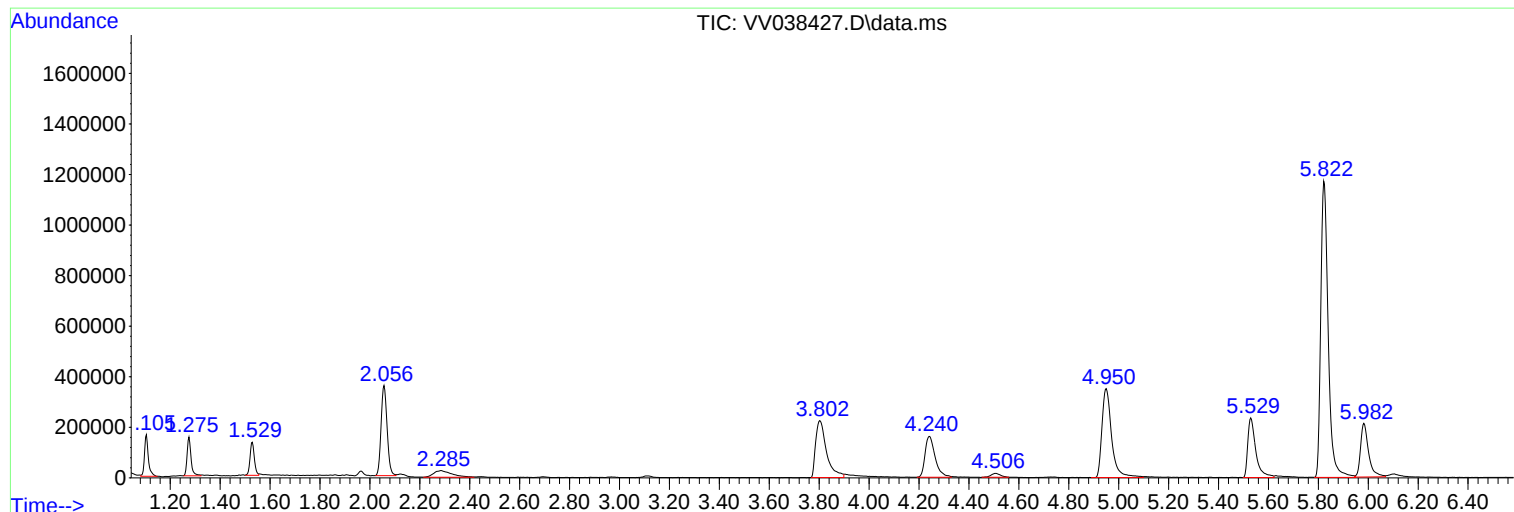

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120624\
Data File : VV038427.D
Acq On : 05 Dec 2024 19:42
Operator : SY/MD
Sample : P5111-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG450

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120624\
Data File : VV038427.D
Acq On : 05 Dec 2024 19:42
Operator : SY/MD
Sample : P5111-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG450

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc