

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120624\
 Data File : VV038431.D
 Acq On : 06 Dec 2024 00:45
 Operator : SY/MD
 Sample : P5111-05
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG454

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV038431.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.204	40	51	66	rBV2	20903	68097	6.85%	0.836%
2	1.275	66	73	85	rVV	160456	176081	17.71%	2.162%
3	1.343	86	94	114	rVV3	23081	77968	7.84%	0.957%
4	1.529	145	152	166	rBV	134233	160825	16.18%	1.974%
5	1.966	282	288	303	rVV	17114	25557	2.57%	0.314%
6	2.053	306	315	332	rVV	274787	419310	42.18%	5.147%
7	2.124	332	337	353	rVB3	9788	22973	2.31%	0.282%
8	2.304	373	393	395	rBV2	19556	42887	4.31%	0.526%
9	3.799	847	858	891	rBV	94748	328833	33.08%	4.037%
10	4.240	980	995	1035	rBV	170400	459614	46.24%	5.642%
11	4.950	1201	1216	1250	rBV2	374618	994056	100.00%	12.203%
12	5.529	1385	1396	1429	rBV	234261	532593	53.58%	6.538%
13	5.838	1480	1492	1518	rBV4	39241	98189	9.88%	1.205%
14	5.982	1522	1537	1572	rBV	216461	482856	48.57%	5.927%
15	6.912	1817	1826	1853	rBV	77925	173319	17.44%	2.128%
16	7.236	1914	1927	1952	rBV	377596	723474	72.78%	8.881%
17	7.558	2018	2027	2047	rBV2	46400	102051	10.27%	1.253%
18	7.902	2122	2134	2152	rBV2	93315	169991	17.10%	2.087%
19	8.021	2163	2171	2217	rBV	348943	860208	86.54%	10.560%
20	8.780	2397	2407	2429	rBV	413929	740550	74.50%	9.091%
21	10.146	2820	2832	2856	rBV	177487	296017	29.78%	3.634%
22	11.178	3143	3153	3179	rBV	341676	576445	57.99%	7.076%
23	11.554	3259	3270	3294	rBV	353072	614184	61.79%	7.540%




Sum of corrected areas: 8146078

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120624\
Data File : VV038431.D
Acq On : 06 Dec 2024 00:45
Operator : SY/MD
Sample : P5111-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG454

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

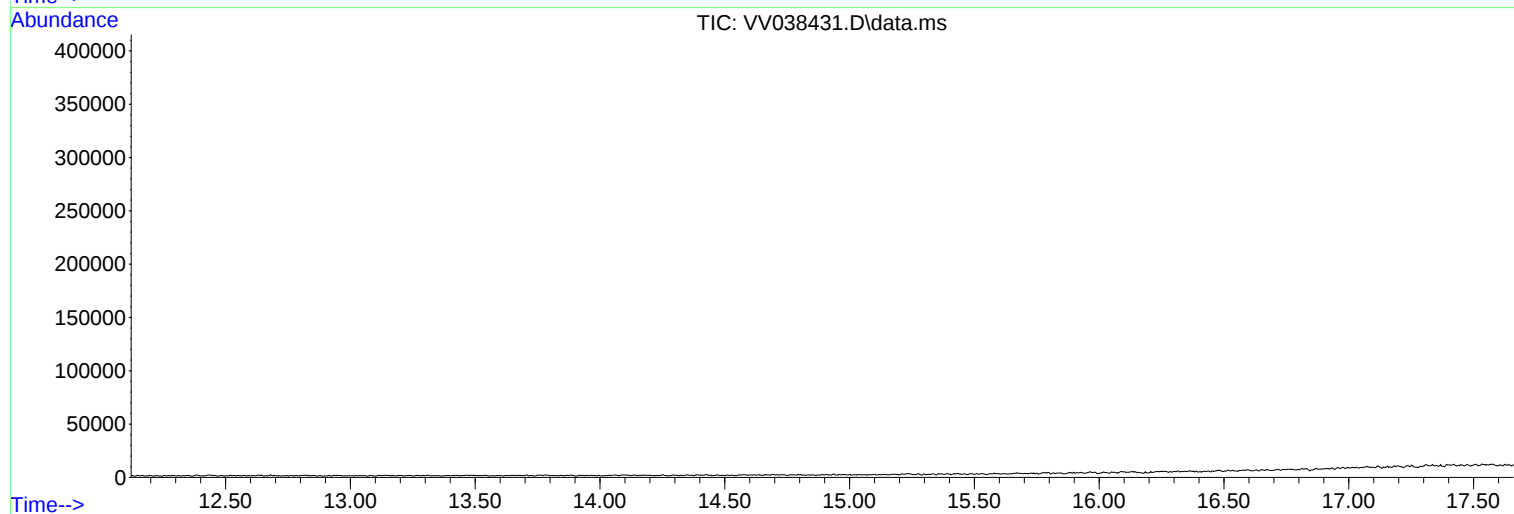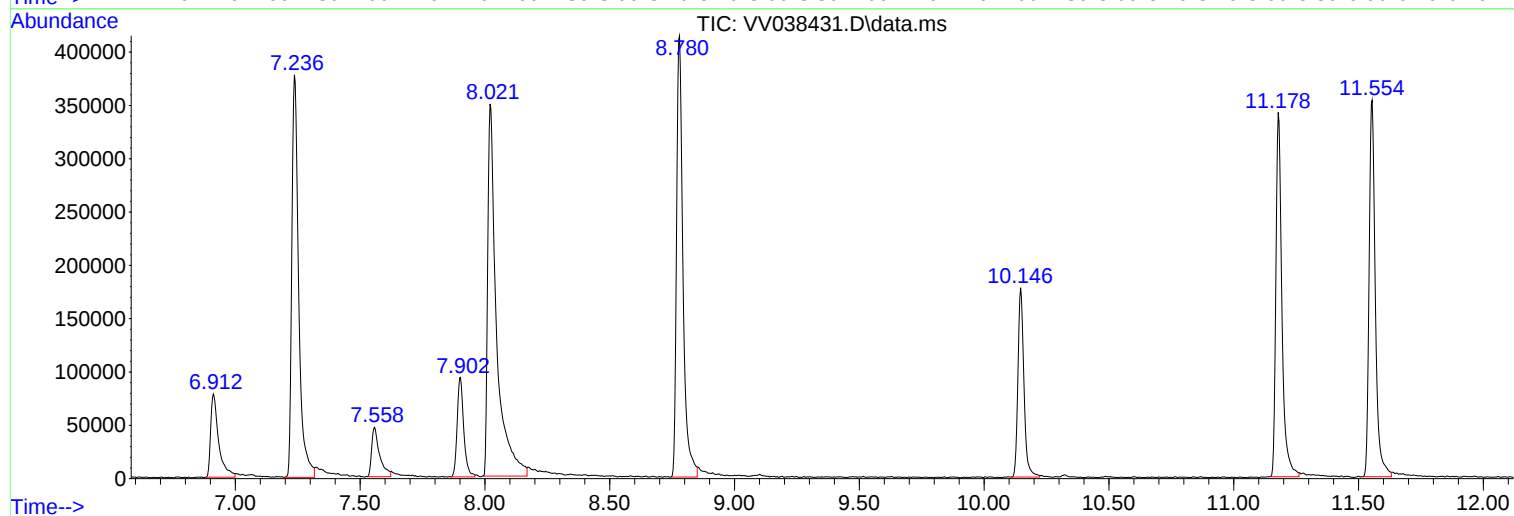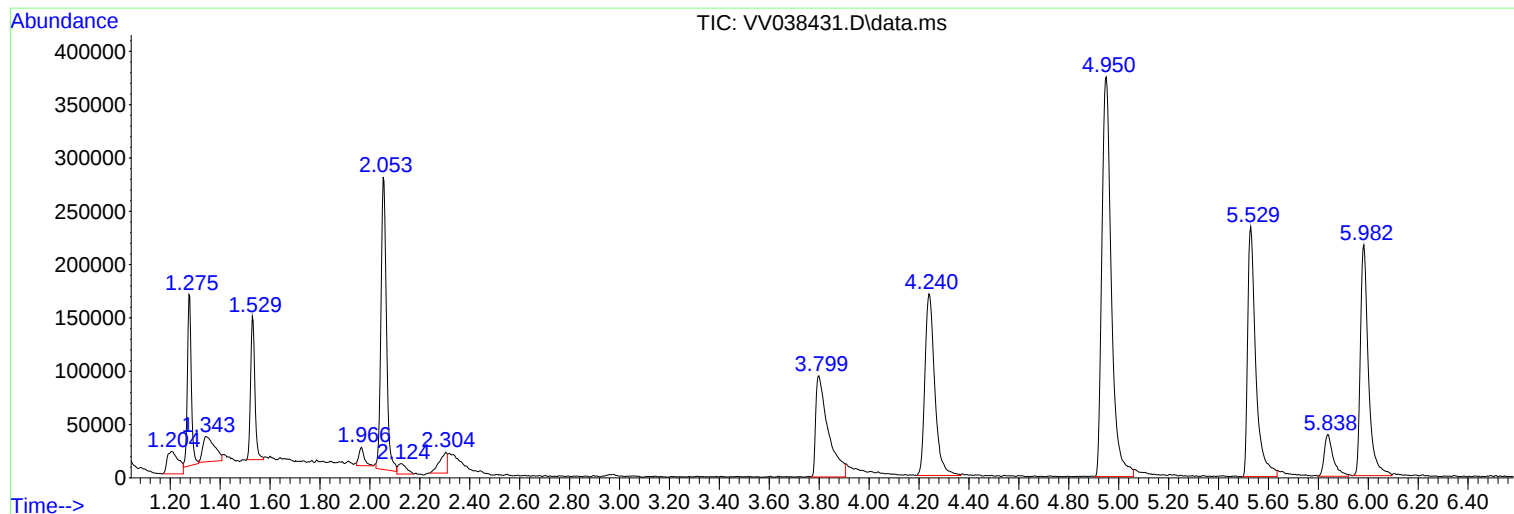

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120624\
Data File : VV038431.D
Acq On : 06 Dec 2024 00:45
Operator : SY/MD
Sample : P5111-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG454

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120624\
Data File : VV038431.D
Acq On : 06 Dec 2024 00:45
Operator : SY/MD
Sample : P5111-05
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG454

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc