


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120624\
Data File : VV038418.D
Acq On : 05 Dec 2024 14:31
Operator : SY/MD
Sample : BFB296
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB296

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Dec 06 21:32:44 2024

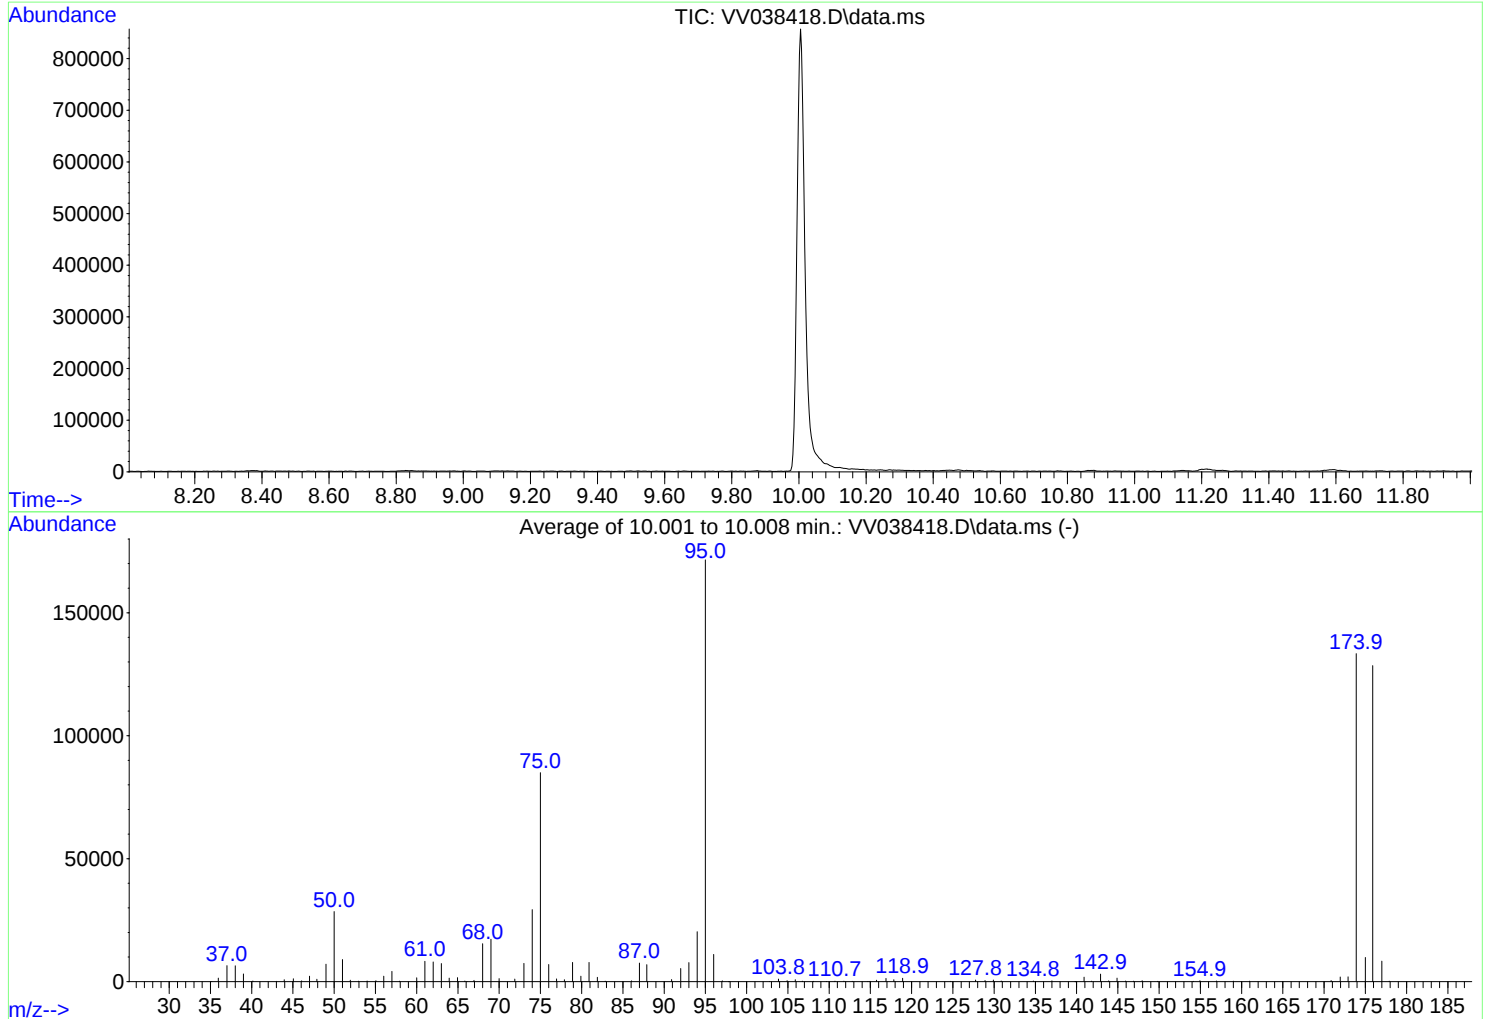

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	28512	PASS
75	95	30	80	49.6	85003	PASS
95	95	100	100	100.0	171520	PASS
96	95	5	9	6.4	11058	PASS
173	174	0.00	2	1.5	1935	PASS
174	95	50	120	77.8	133405	PASS
175	174	5	9	7.4	9840	PASS
176	174	95	105	96.3	128523	PASS
177	176	5	10	6.5	8355	PASS

m/z	Abundance
35.80	127.0
39.90	287.0
43.90	761.0
77.00	128.0
206.80	108.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296

m/z	Abundance
35.10	138.0
36.00	1402.0
37.00	6696.0
38.00	6483.0
39.00	3092.0
39.90	431.0
43.00	175.0
44.00	1598.0
45.10	1227.0
46.10	337.0
47.00	2205.0
47.90	877.0
49.00	6848.0
50.00	28288.0
51.00	8989.0
52.00	578.0
52.90	204.0
54.00	276.0
55.10	350.0
56.00	2233.0
57.00	4148.0
57.90	161.0
60.00	1594.0
61.00	8488.0
62.00	7898.0
63.00	7371.0
64.00	1566.0
65.00	1648.0
65.90	228.0
66.10	225.0
67.00	429.0
68.00	15250.0
69.00	16976.0
70.00	1191.0
71.90	1017.0
73.00	7360.0
74.00	28472.0
75.00	84208.0
76.00	6729.0
77.00	1150.0
77.80	721.0
78.90	7904.0
79.90	2336.0
80.90	7539.0
81.90	1658.0
82.90	197.0
86.00	355.0
87.00	7558.0
87.90	6971.0
90.90	820.0
92.00	5181.0
93.00	7459.0
94.00	20064.0
95.00	168128.0
96.00	11298.0
97.10	266.0
97.80	111.0
103.90	979.0
104.90	349.0
105.90	784.0
106.80	152.0
108.10	147.0
110.70	186.0
112.00	162.0
112.70	119.0
114.70	181.0
115.80	603.0
117.00	1365.0
117.90	794.0
118.90	1363.0
124.70	110.0
127.80	685.0
128.90	453.0
129.90	666.0
130.90	213.0
134.80	278.0
137.00	271.0
139.80	112.0
140.90	1783.0
141.80	195.0
142.90	3083.0
143.90	321.0
144.90	1375.0
146.00	214.0
146.90	208.0
147.90	392.0
149.80	168.0
154.20	114.0
155.00	433.0
156.90	300.0
159.00	238.0
160.90	194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296

170.80	516.0
171.90	2037.0
172.90	1854.0
173.90	127384.0
175.00	9356.0
175.90	122384.0
177.00	8140.0
177.90	197.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296

m/z	Abundance
35.20	107.0
36.00	1662.0
37.00	6653.0
38.00	6746.0
39.00	3198.0
40.10	356.0
43.00	137.0
44.00	1607.0
45.00	1236.0
46.00	341.0
47.00	2341.0
47.90	1011.0
49.00	7443.0
50.00	29624.0
51.00	9170.0
52.00	638.0
52.90	212.0
54.00	262.0
55.00	371.0
56.00	2312.0
57.00	4364.0
57.90	162.0
60.00	1604.0
61.00	8620.0
62.00	8227.0
63.00	7549.0
64.00	1451.0
65.00	1709.0
65.80	245.0
66.90	514.0
68.00	15733.0
69.00	17904.0
70.00	1292.0
71.90	1091.0
73.00	7790.0
74.00	30264.0
75.00	88384.0
76.00	7251.0
76.90	1308.0
77.90	767.0
78.90	8208.0
79.90	2243.0
80.90	8024.0
81.90	1812.0
82.80	199.0
86.10	333.0
87.00	7721.0
87.90	7125.0
90.90	866.0
92.00	5612.0
93.00	7913.0
94.00	20976.0
95.00	177792.0
96.00	11431.0
97.00	329.0
103.90	1110.0
104.90	396.0
105.90	830.0
106.70	192.0
108.10	142.0
109.70	108.0
110.70	220.0
111.80	165.0
112.80	126.0
114.90	195.0
115.80	639.0
116.90	1324.0
117.90	812.0
118.90	1436.0
124.80	106.0
127.80	677.0
128.90	432.0
129.90	649.0
130.80	238.0
134.70	300.0
137.00	319.0
140.00	126.0
140.90	1872.0
141.80	229.0
142.90	3166.0
143.90	367.0
144.90	1533.0
146.00	313.0
146.90	216.0
148.00	439.0
149.80	157.0
154.20	123.0
154.90	419.0
156.90	286.0
159.00	202.0
160.90	202.0
170.90	461.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296

172.00	1950.0
172.90	2015.0
173.90	138432.0
175.00	10154.0
175.90	132992.0
177.00	8641.0
177.90	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296

m/z	Abundance
36.00	1678.0
37.00	6182.0
38.00	6199.0
39.00	3043.0
40.20	380.0
44.00	1460.0
45.00	1118.0
46.00	270.0
47.00	2082.0
47.90	1081.0
49.00	6994.0
50.00	27624.0
51.00	8755.0
51.90	585.0
53.00	220.0
54.00	224.0
55.10	457.0
56.00	2187.0
57.00	4064.0
57.90	186.0
60.00	1417.0
61.00	7791.0
62.00	7954.0
63.00	7106.0
63.90	1373.0
64.90	1541.0
65.90	234.0
66.90	611.0
68.00	15211.0
69.00	16856.0
70.00	1290.0
71.90	1020.0
73.00	7185.0
74.00	29128.0
75.00	82416.0
76.00	6982.0
76.90	1231.0
78.00	792.0
78.90	7364.0
79.90	1987.0
80.90	7789.0
81.90	1837.0
82.80	179.0
86.10	280.0
87.00	7464.0
87.90	6657.0
90.90	824.0
92.00	5316.0
93.00	7894.0
94.00	19864.0
95.00	168640.0
96.00	10446.0
97.00	386.0
102.80	121.0
103.80	1029.0
104.90	392.0
105.90	821.0
106.70	175.0
108.10	164.0
109.70	128.0
110.70	218.0
111.70	238.0
112.90	135.0
115.00	242.0
115.70	553.0
116.80	1315.0
117.80	765.0
118.90	1337.0
124.80	111.0
127.70	619.0
128.90	419.0
129.90	656.0
130.80	268.0
134.80	286.0
137.00	300.0
139.90	134.0
140.90	1757.0
141.80	207.0
142.90	3036.0
143.90	304.0
144.90	1450.0
145.90	348.0
146.90	212.0
148.00	439.0
149.80	172.0
154.00	112.0
154.90	394.0
157.00	267.0
158.90	117.0
161.00	184.0
170.90	440.0
172.00	1781.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296

172.90	1935.0
173.90	134400.0
175.00	10011.0
175.90	130192.0
177.00	8284.0
177.90	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB296