

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120724\
 Data File : VV038437.D
 Acq On : 06 Dec 2024 14:29
 Operator : SY/MD
 Sample : P5111-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG456

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV038437.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.243	48	63	65	rBV4	8644	18956	1.89%	0.245%
2	1.275	66	73	88	rVB	157959	176533	17.62%	2.284%
3	1.529	145	152	164	rBV	139059	154419	15.42%	1.998%
4	1.963	279	287	296	rBV	20079	28108	2.81%	0.364%
5	2.053	305	315	332	rVB	264729	386467	38.58%	5.000%
6	2.320	374	398	400	rBV	14738	40368	4.03%	0.522%
7	3.799	849	858	894	rBV	90087	332503	33.19%	4.302%
8	4.240	977	995	1023	rBV2	167411	450617	44.99%	5.830%
9	4.947	1202	1215	1259	rBV2	380185	1001679	100.00%	12.959%
10	5.526	1384	1395	1433	rBV	236852	542189	54.13%	7.015%
11	5.841	1482	1493	1509	rBV9	14011	35790	3.57%	0.463%
12	5.979	1524	1536	1566	rBV	216844	469232	46.84%	6.071%
13	6.912	1813	1826	1856	rBV	75836	172893	17.26%	2.237%
14	7.236	1917	1927	1951	rBV	383886	731523	73.03%	9.464%
15	7.558	2017	2027	2047	rBV	43759	100297	10.01%	1.298%
16	7.905	2121	2135	2151	rVB6	13736	27447	2.74%	0.355%
17	8.024	2163	2172	2208	rBV	336491	826722	82.53%	10.696%
18	8.776	2394	2406	2436	rBV	409944	738166	73.69%	9.550%
19	10.146	2821	2832	2850	rBV	171159	287395	28.69%	3.718%
20	11.178	3142	3153	3190	rBV	335646	588265	58.73%	7.611%
21	11.555	3258	3270	3297	rBV	357482	619852	61.88%	8.019%




Sum of corrected areas: 7729421

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120724\
Data File : VV038437.D
Acq On : 06 Dec 2024 14:29
Operator : SY/MD
Sample : P5111-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG456

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

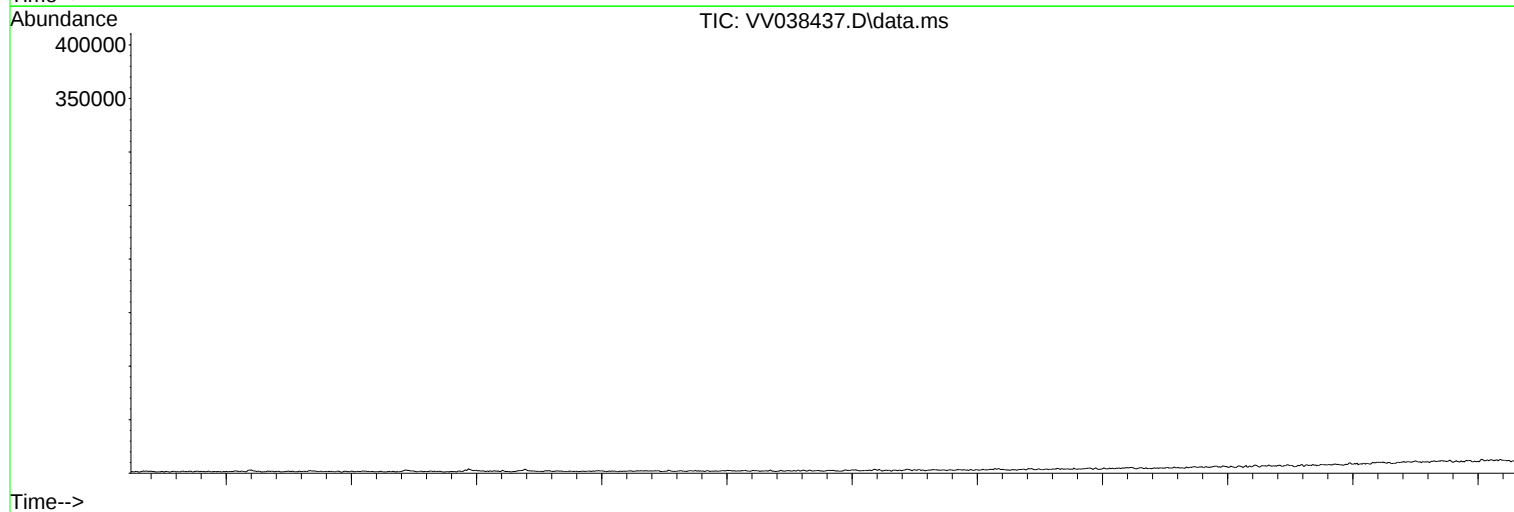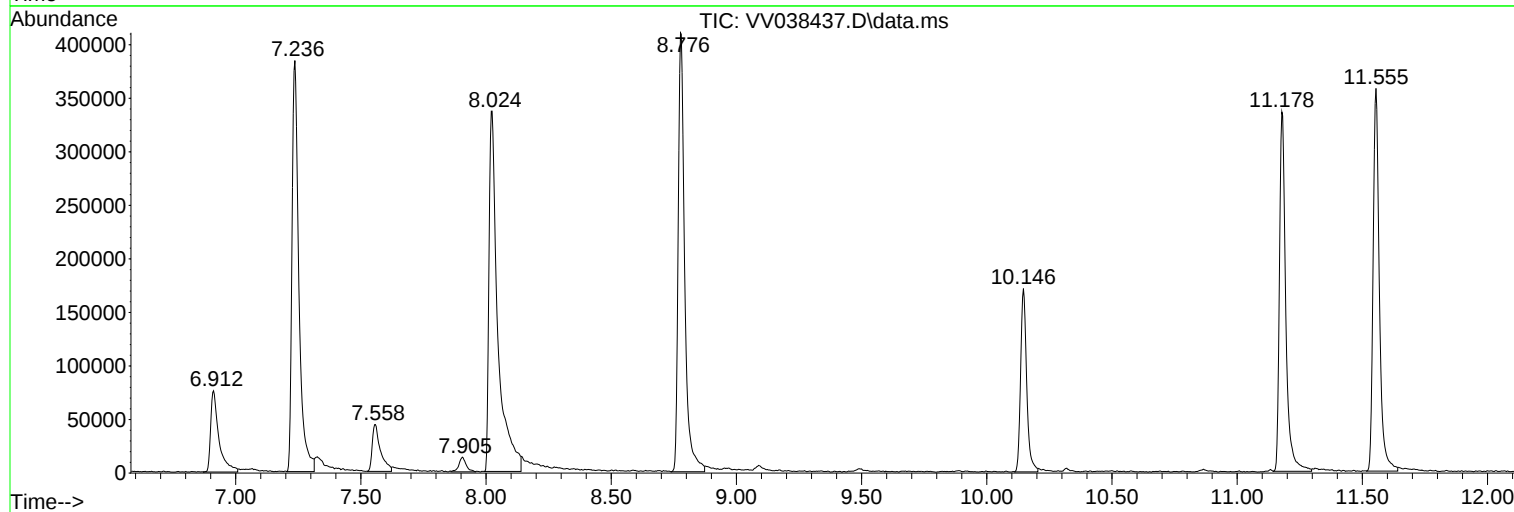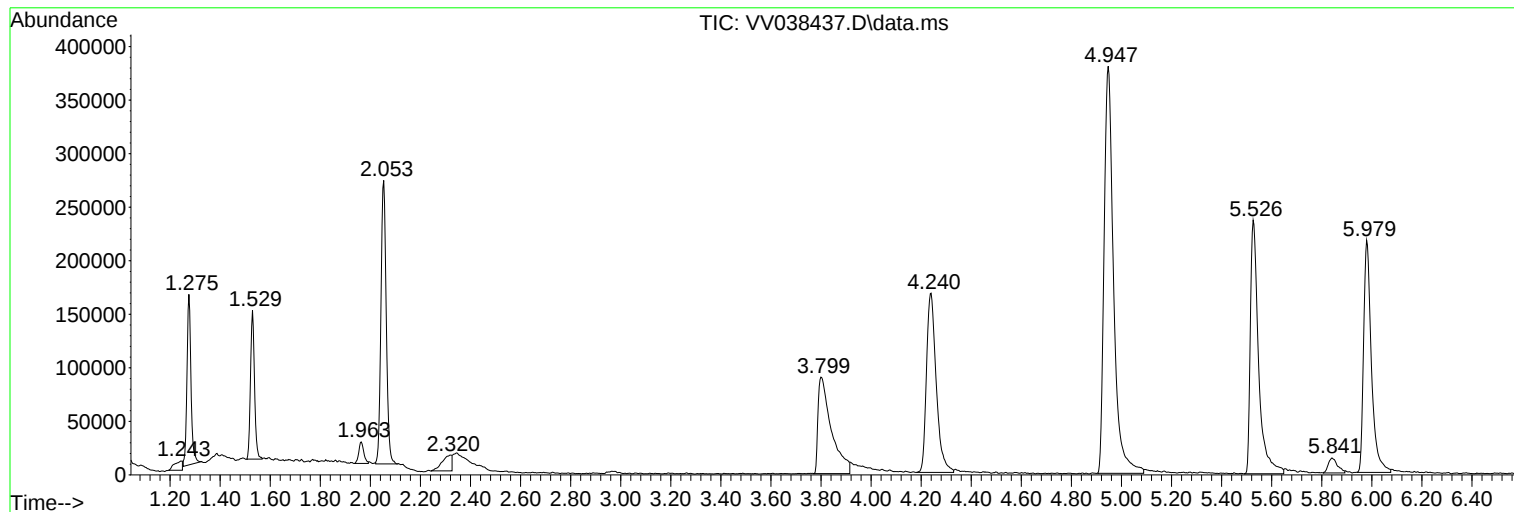

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120724\
Data File : VV038437.D
Acq On : 06 Dec 2024 14:29
Operator : SY/MD
Sample : P5111-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG456

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV120724\
Data File : VV038437.D
Acq On : 06 Dec 2024 14:29
Operator : SY/MD
Sample : P5111-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG456

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111924WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------