

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019737.D
 Acq On : 19 Dec 2020 15:02
 Operator : SY/MD
 Sample : L5101-06
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FX2

Quant Time: Dec 21 04:35:12 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Dec 21 03:36:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.62	114	721137	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.86	117	678079	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.25	152	304835	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	212689	41.13	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	82.26%
7) Chloroethane-d5	1.57	69	186299	45.68	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	91.36%
11) 1,1-Dichloroethene-d2	2.11	63	321370	33.48	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.96%
21) 2-Butanone-d5	3.89	46	369405	131.43	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	131.43%#
24) Chloroform-d	4.35	84	435822	46.76	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.52%
26) 1,2-Dichloroethane-d4	5.04	65	307302	50.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.92%
32) Benzene-d6	5.05	84	857600	47.42	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.84%
36) 1,2-Dichloropropane-d6	6.07	67	282784	49.92	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.84%
41) Toluene-d8	7.32	98	737572	45.30	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	90.60%
43) trans-1,3-Dichloropropene-	7.62	79	127270	39.50	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.00%
47) 2-Hexanone-d5	8.09	63	231255	104.01	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	104.01%
57) 1,1,2,2-Tetrachloroethane-	10.22	84	350045	45.68	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.36%
64) 1,2-Dichlorobenzene-d4	11.63	152	279387	49.03	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.06%


Target Compounds					Ovalue
13) Acetone	2.18	43	21133	8.826 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
Data File : VV019737.D
Acq On : 19 Dec 2020 15:02
Operator : SY/MD
Sample : L5101-06
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FX2

Quant Time: Dec 21 04:35:12 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Dec 21 03:36:59 2020
Response via : Initial Calibration

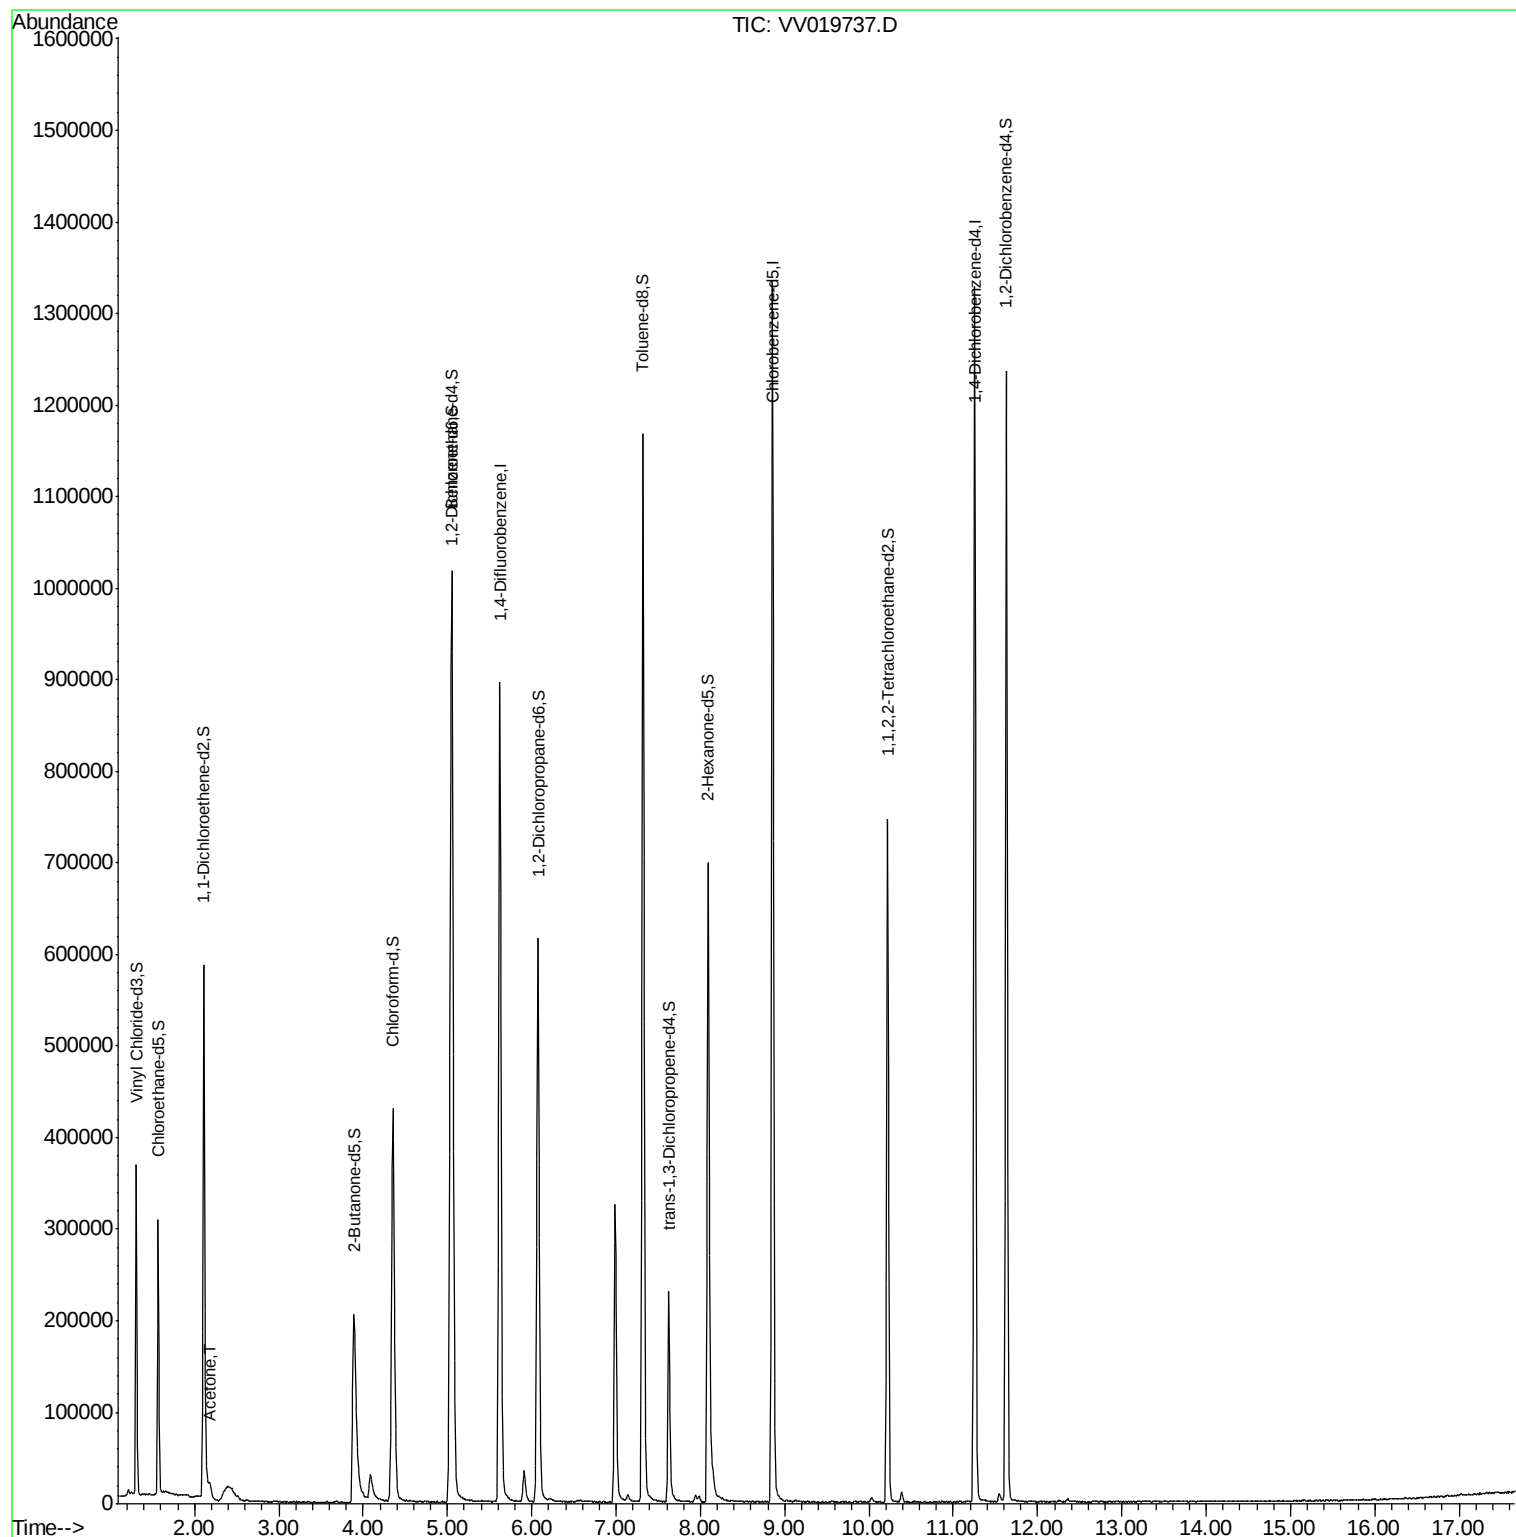

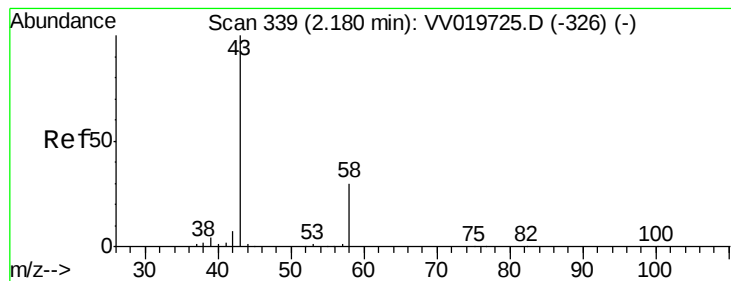

#13

Acetone

Concen: 8.826 ug/L

RT: 2.18 min Scan# 340

Delta R.T. 0.00 min

Lab File: VV019737.D

Acq: 19 Dec 2020 15:02

Instrument :
MSVOA_V
ClientSampleId :
C0FX2

Tot Ion: 43 Resp: 21133

Ion Ratio Lower Upper

43 100

58 32.8 0.0 61.6

