

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019746.D
 Acq On : 19 Dec 2020 18:36
 Operator : SY/MD
 Sample : L5131-02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4H01

Manual Integrations
 APPROVED

MMDadoda
 12/21/2020 1:47:42 PM

Quant Time: Dec 21 06:12:51 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Dec 21 03:36:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.62	114	698409	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.86	117	659212	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.25	152	297528	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	245424	49.01	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	98.02%
7) Chloroethane-d5	1.57	69	198406	50.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	100.46%
11) 1,1-Dichloroethene-d2	2.11	63	358366	38.55	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.10%
21) 2-Butanone-d5	3.89	46	348695	128.10	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	128.10%
24) Chloroform-d	4.35	84	448810	49.72	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.44%
26) 1,2-Dichloroethane-d4	5.04	65	310306	52.61	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.22%
32) Benzene-d6	5.05	84	905625	51.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.02%
36) 1,2-Dichloropropane-d6	6.07	67	291000	52.84	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	105.68%
41) Toluene-d8	7.32	98	800117	50.55	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.10%
43) trans-1,3-Dichloropropene-	7.62	79	136299	43.51	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.02%
47) 2-Hexanone-d5	8.09	63	216894	100.34	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	100.34%
57) 1,1,2,2-Tetrachloroethane-	10.22	84	357248	47.96	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.92%
64) 1,2-Dichlorobenzene-d4	11.63	152	287605	51.71	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.42%

Target Compounds					Ovalue
13) Acetone	2.18	43	41205	17.769 ug/L	97
20) cis-1,2-Dichloroethene	3.93	96	8784m	1.752 ug/L	
34) Trichloroethene	5.92	95	56111	11.025 ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
Data File : VV019746.D
Acq On : 19 Dec 2020 18:36
Operator : SY/MD
Sample : L5131-02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
F4H01

Manual Integrations
APPROVED

MMDadoda
12/21/2020 1:47:42 PM

Quant Time: Dec 21 06:12:51 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Dec 21 03:36:59 2020
Response via : Initial Calibration

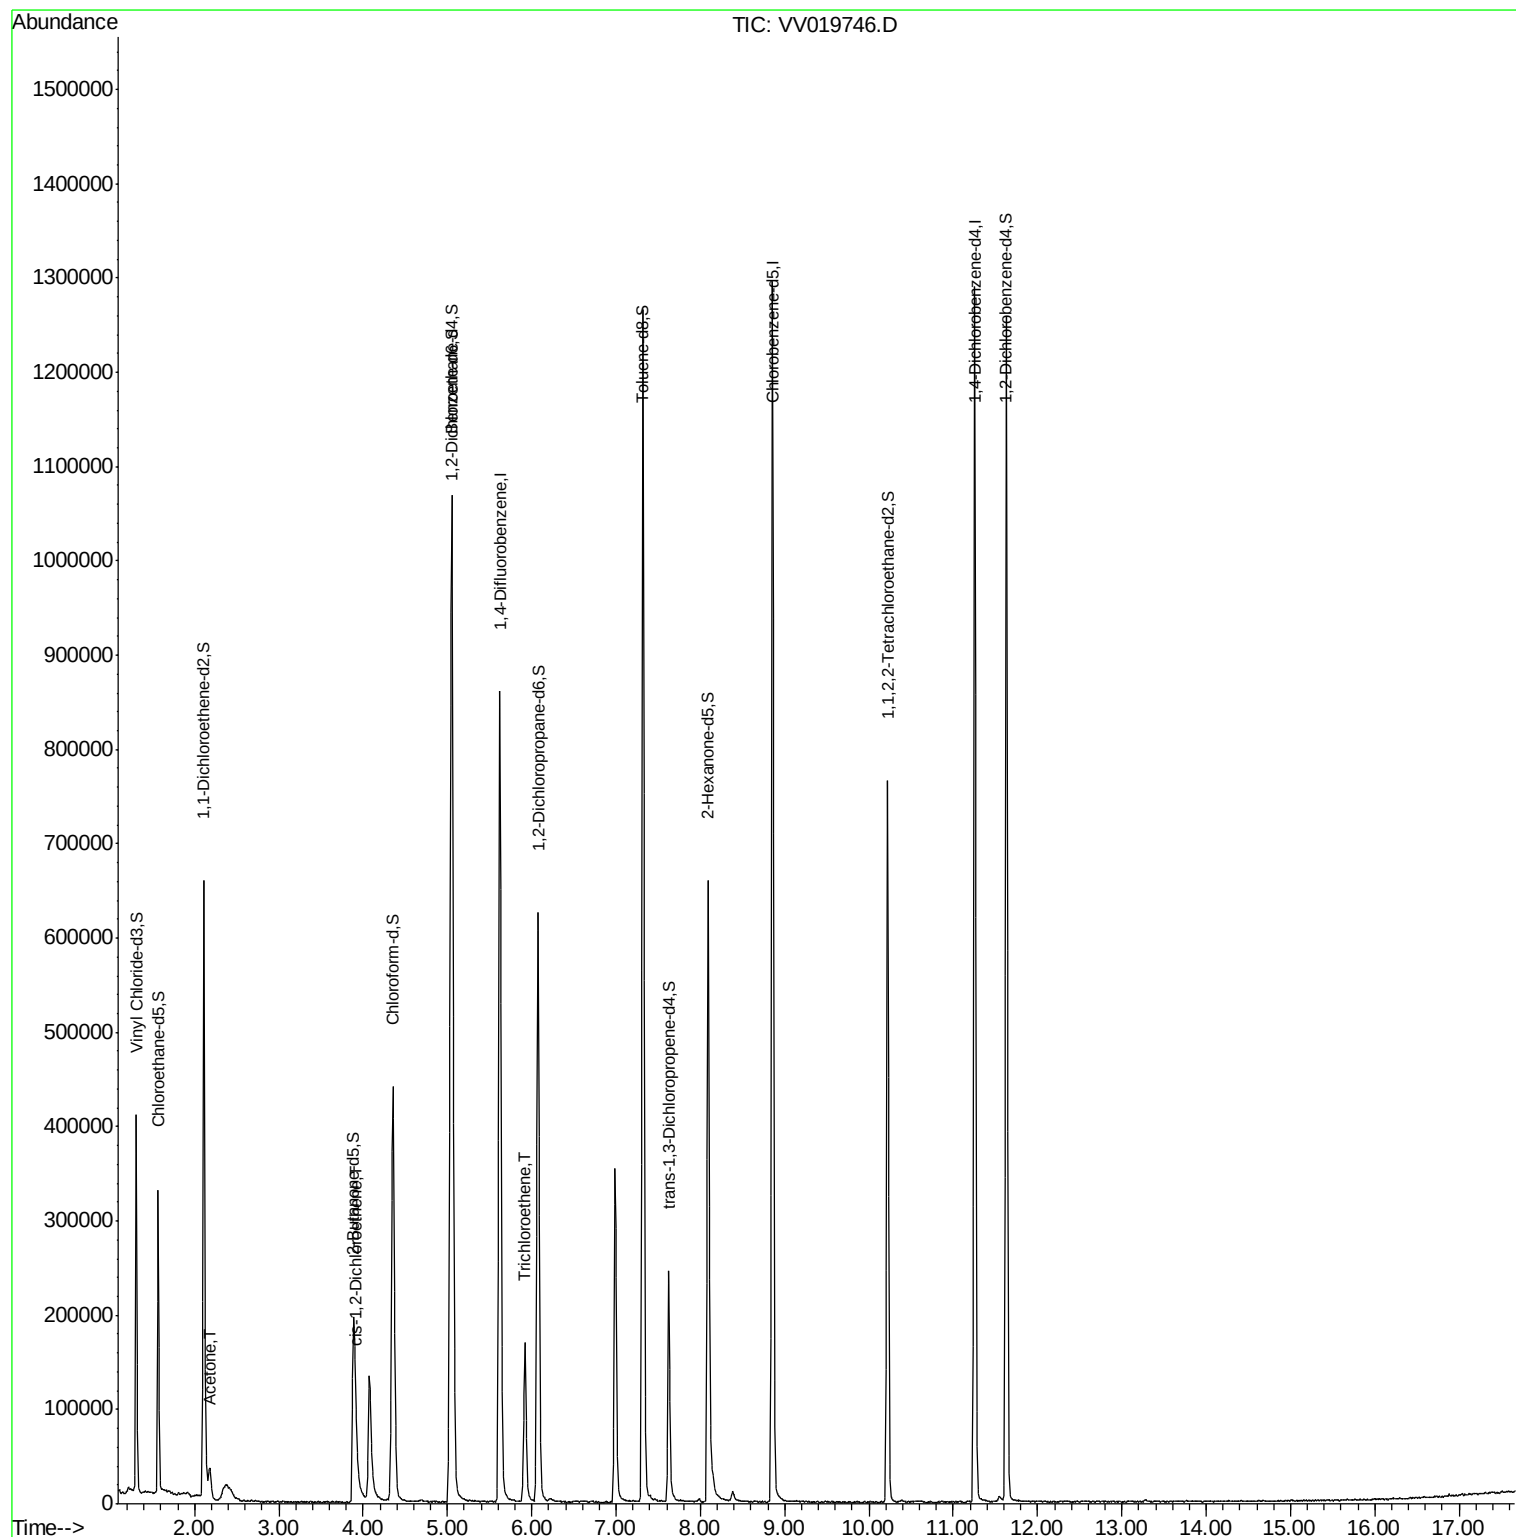

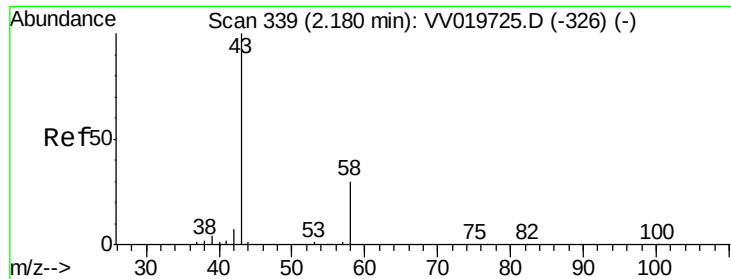

#13

Acetone

Concen: 17.769 ug/L

RT: 2.18 min Scan# 339

Delta R.T. -0.00 min

Lab File: VV019746.D

Acq: 19 Dec 2020 18:36

Instrument :

MSVOA_V

ClientSampleId :

F4H01

Tot Ion: 43 Resp: 41205

Ion Ratio Lower Upper

43 100





58 29.2 0.0 61.6

Manual Integrations

APPROVED

MMDadoda

12/21/2020 1:47:42 PM

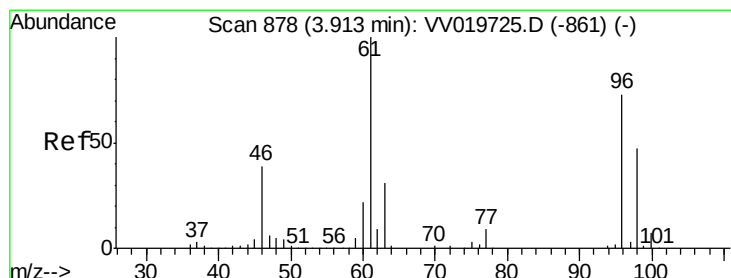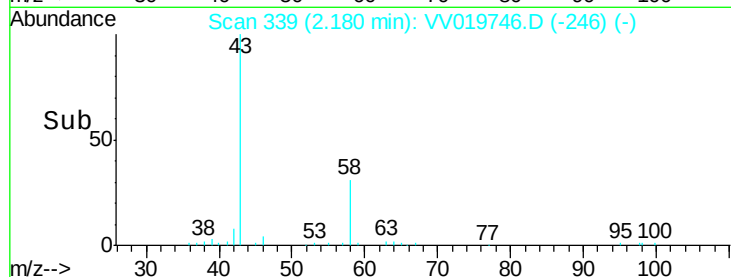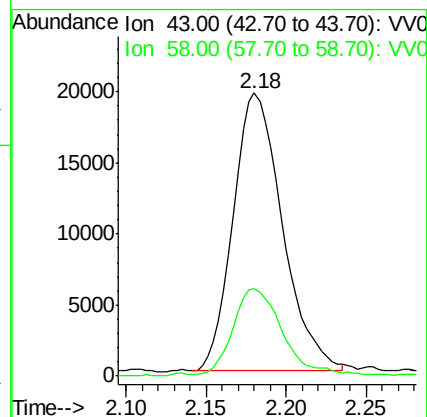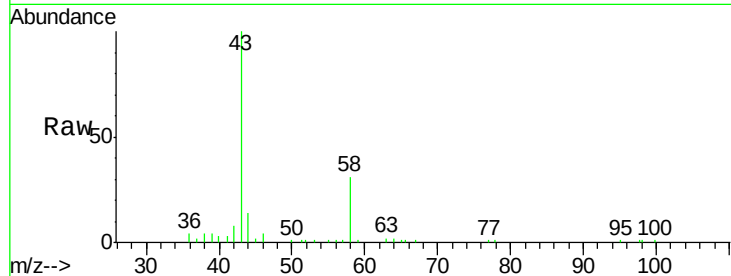

#20

cis-1,2-Dichloroethene

Concen: 1.752 ug/L m

RT: 3.93 min Scan# 882

Delta R.T. 0.01 min

Lab File: VV019746.D

Acq: 19 Dec 2020 18:36




Tgt Ion: 96 Resp: 8784


Ion Ratio Lower Upper

96 100

61 140.6 94.1 174.8

68 0.0 0.1 0.1#

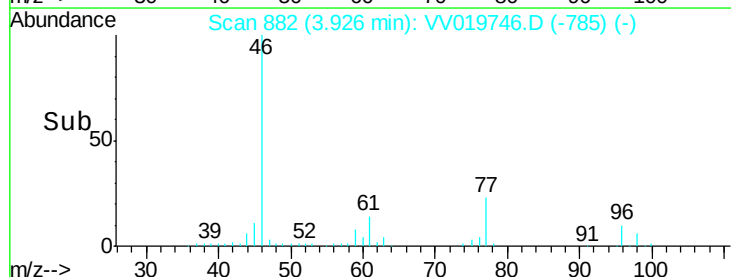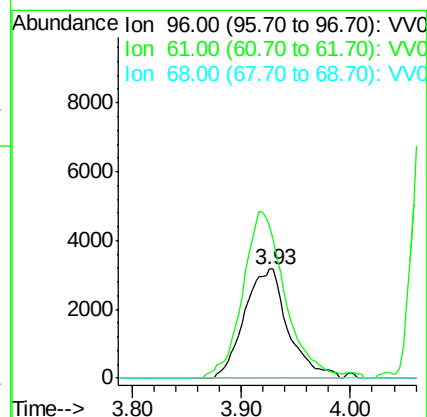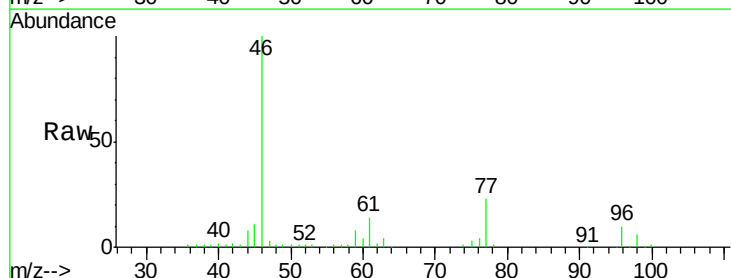

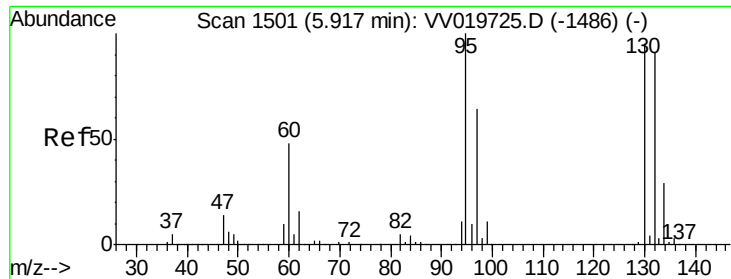

#34

Trichloroethene

Concen: 11.025 ug/L

RT: 5.92 min Scan# 1502

Delta R.T. 0.00 min

Lab File: VV019746.D


Acq: 19 Dec 2020 18:36

Instrument :

MSVOA_V

ClientSampleId :

F4H01

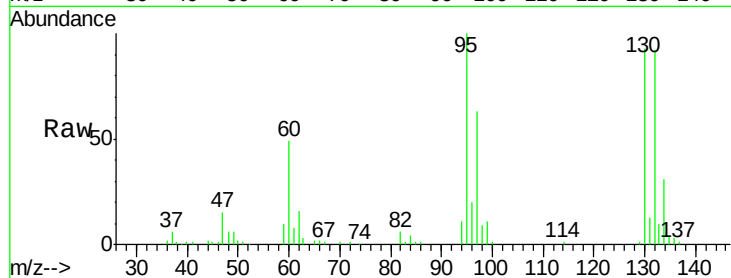

Tot Ion	Ratio	Resp Lower	Upper
95	100		
97	63.3	44.4	82.4
132	91.8	64.3	119.3
130	93.1	67.8	125.8

Manual Integrations
APPROVED

MMDadoda
12/21/2020 1:47:42 PM

