

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019726.D
 Acq On : 19 Dec 2020 09:59
 Operator : SY/MD
 Sample : VV1219WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK74

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M

Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	81	rVB	350911	355823	14.09%	1.719%
2	1.569	142	149	160	rVB	293524	330821	13.10%	1.598%
3	2.110	307	317	345	rVB	583765	911260	36.08%	4.403%
4	2.592	465	467	468	rBV	747	289	0.01%	0.001%
5	2.878	553	556	560	rBV3	735	714	0.03%	0.003%
6	2.933	571	573	576	rBV3	772	556	0.02%	0.003%
7	3.058	611	612	618	rVB4	480	371	0.01%	0.002%
8	3.167	644	646	648	rBV2	871	366	0.01%	0.002%
9	3.396	714	717	720	rBV2	484	345	0.01%	0.002%
10	3.447	731	733	736	rBV2	455	278	0.01%	0.001%
11	3.470	736	740	741	rVV2	461	271	0.01%	0.001%
12	3.495	745	748	749	rBV2	582	284	0.01%	0.001%
13	3.518	749	755	759	rVV4	662	748	0.03%	0.004%
14	3.553	763	766	768	rVB4	718	427	0.02%	0.002%
15	3.595	774	779	783	rBV3	657	645	0.03%	0.003%
16	3.624	783	788	790	rBV3	586	452	0.02%	0.002%
17	3.640	790	793	795	rVB3	772	368	0.01%	0.002%
18	3.656	795	798	799	rBV	780	484	0.02%	0.002%
19	3.685	804	807	810	rBV3	580	428	0.02%	0.002%
20	3.746	823	826	828	rBV3	388	316	0.01%	0.002%
21	3.788	837	839	844	rVB4	599	382	0.02%	0.002%
22	3.888	859	870	902	rBV	184159	574691	22.75%	2.777%
23	4.348	998	1013	1049	rVB	407001	1003038	39.71%	4.846%
24	4.765	1139	1143	1144	rBV2	762	445	0.02%	0.002%
25	4.894	1179	1183	1184	rBV2	575	334	0.01%	0.002%
26	4.962	1201	1204	1207	rBV3	984	657	0.03%	0.003%
27	5.045	1213	1230	1261	rVV2	978604	2525730	100.00%	12.203%
28	5.618	1394	1408	1441	rBV	933554	1870926	74.07%	9.040%
29	5.907	1488	1498	1516	rVB2	21396	47759	1.89%	0.231%
30	6.071	1534	1549	1578	rVV	575850	1174824	46.51%	5.676%
31	6.421	1655	1658	1659	rBV2	698	418	0.02%	0.002%
32	6.527	1688	1691	1693	rBV3	564	361	0.01%	0.002%
33	6.547	1693	1697	1700	rBV4	665	461	0.02%	0.002%
34	6.572	1700	1705	1708	rVV2	794	673	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019726.D
 Acq On : 19 Dec 2020 09:59
 Operator : SY/MD
 Sample : VV1219WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK74

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.634	1720	1724	1726	rBV4	1407	1125	0.04%	0.005%
36	6.720	1749	1751	1754	rVB2	779	474	0.02%	0.002%
37	6.781	1766	1770	1772	rBV3	1037	701	0.03%	0.003%
38	6.810	1777	1779	1781	rBV2	591	327	0.01%	0.002%
39	6.823	1781	1783	1786	rVB3	720	351	0.01%	0.002%
40	6.849	1786	1791	1793	rBV4	768	700	0.03%	0.003%
41	6.907	1807	1809	1813	rVB2	1133	732	0.03%	0.004%
42	6.936	1813	1818	1821	rBV3	1001	697	0.03%	0.003%
43	6.987	1821	1834	1864	rBV	333063	609657	24.14%	2.946%
44	7.193	1896	1898	1903	rBV5	1192	1146	0.05%	0.006%
45	7.318	1924	1937	1966	rBV	1139565	1970523	78.02%	9.521%
46	7.624	2022	2032	2054	rBV	228281	397481	15.74%	1.920%
47	7.894	2113	2116	2118	rVB3	781	563	0.02%	0.003%
48	7.978	2136	2142	2144	rBV5	2201	2136	0.08%	0.010%
49	8.090	2166	2177	2208	rBV	680344	1252590	49.59%	6.052%
50	8.736	2376	2378	2380	rBV2	655	335	0.01%	0.002%
51	8.855	2403	2415	2438	rBV	1419445	2276867	90.15%	11.001%
52	9.341	2564	2566	2568	rVB3	783	318	0.01%	0.002%
53	9.360	2569	2572	2573	rBV2	664	358	0.01%	0.002%
54	9.405	2582	2586	2589	rBV4	1069	899	0.04%	0.004%
55	9.508	2615	2618	2620	rVB3	926	580	0.02%	0.003%
56	9.524	2620	2623	2624	rBV3	673	388	0.02%	0.002%
57	9.550	2627	2631	2634	rBV4	1431	1486	0.06%	0.007%
58	9.653	2661	2663	2665	rBV2	580	338	0.01%	0.002%
59	9.781	2697	2703	2705	rBV3	590	723	0.03%	0.003%
60	9.839	2717	2721	2722	rBV	686	492	0.02%	0.002%
61	9.881	2733	2734	2738	rVB2	603	271	0.01%	0.001%
62	9.920	2743	2746	2747	rBV	1330	656	0.03%	0.003%
63	10.006	2771	2773	2775	rBV2	522	300	0.01%	0.001%
64	10.109	2802	2805	2806	rBV3	1028	351	0.01%	0.002%
65	10.222	2827	2840	2858	rBV	728380	1148371	45.47%	5.549%
66	10.350	2878	2880	2882	rVB3	950	302	0.01%	0.001%
67	10.379	2887	2889	2891	rBV2	820	449	0.02%	0.002%
68	10.437	2906	2907	2909	rBV2	717	368	0.01%	0.002%
69	10.486	2920	2922	2928	rVB4	1087	857	0.03%	0.004%
70	10.514	2928	2931	2932	rBV3	697	402	0.02%	0.002%
71	10.537	2936	2938	2942	rBV5	1109	932	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019726.D
 Acq On : 19 Dec 2020 09:59
 Operator : SY/MD
 Sample : VV1219WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK74

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.621	2962	2964	2967	rBV3	627	356	0.01%	0.002%
73	10.675	2976	2981	2983	rBV3	708	721	0.03%	0.003%
74	10.704	2987	2990	2991	rBV2	607	315	0.01%	0.002%
75	10.756	3004	3006	3010	rVV3	827	551	0.02%	0.003%
76	10.836	3028	3031	3034	rBV4	747	506	0.02%	0.002%
77	10.929	3051	3060	3064	rBV6	3031	4334	0.17%	0.021%
78	10.961	3068	3070	3073	rBV3	636	397	0.02%	0.002%
79	11.074	3101	3105	3106	rVB	636	426	0.02%	0.002%
80	11.148	3124	3128	3129	rVB4	653	340	0.01%	0.002%
81	11.190	3133	3141	3149	rBV7	4440	7664	0.30%	0.037%
82	11.254	3149	3161	3181	rBV	1512517	2289547	90.65%	11.062%
83	11.550	3251	3253	3256	rBV2	597	341	0.01%	0.002%
84	11.630	3266	3278	3299	rBV	1184559	1840961	72.89%	8.895%
85	11.852	3345	3347	3348	rBV2	803	430	0.02%	0.002%
86	12.042	3403	3406	3410	rBV3	946	781	0.03%	0.004%
87	12.257	3470	3473	3477	rBV2	693	709	0.03%	0.003%
88	12.354	3499	3503	3504	rBV2	610	403	0.02%	0.002%
89	12.379	3509	3511	3515	rVB3	1061	563	0.02%	0.003%
90	12.473	3538	3540	3542	rBV3	615	307	0.01%	0.001%
91	12.485	3542	3544	3547	rVB3	842	434	0.02%	0.002%
92	12.653	3589	3596	3609	rVB6	6647	11097	0.44%	0.054%
93	12.932	3679	3683	3689	rBV5	760	1160	0.05%	0.006%
94	12.961	3689	3692	3698	rVV5	845	1006	0.04%	0.005%
95	13.103	3733	3736	3740	rBV3	1157	973	0.04%	0.005%
96	13.273	3782	3789	3799	rVB8	9635	15969	0.63%	0.077%
97	13.392	3824	3826	3832	rBV5	830	634	0.03%	0.003%
98	13.434	3836	3839	3842	rBV3	720	590	0.02%	0.003%
99	13.518	3857	3865	3877	rBV2	10898	18937	0.75%	0.091%
100	13.755	3931	3939	3948	rVB5	9620	15282	0.61%	0.074%


Sum of corrected areas: 20696925

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121920\
Data File : VV019726.D
Acq On : 19 Dec 2020 09:59
Operator : SY/MD
Sample : VV1219WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK74

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

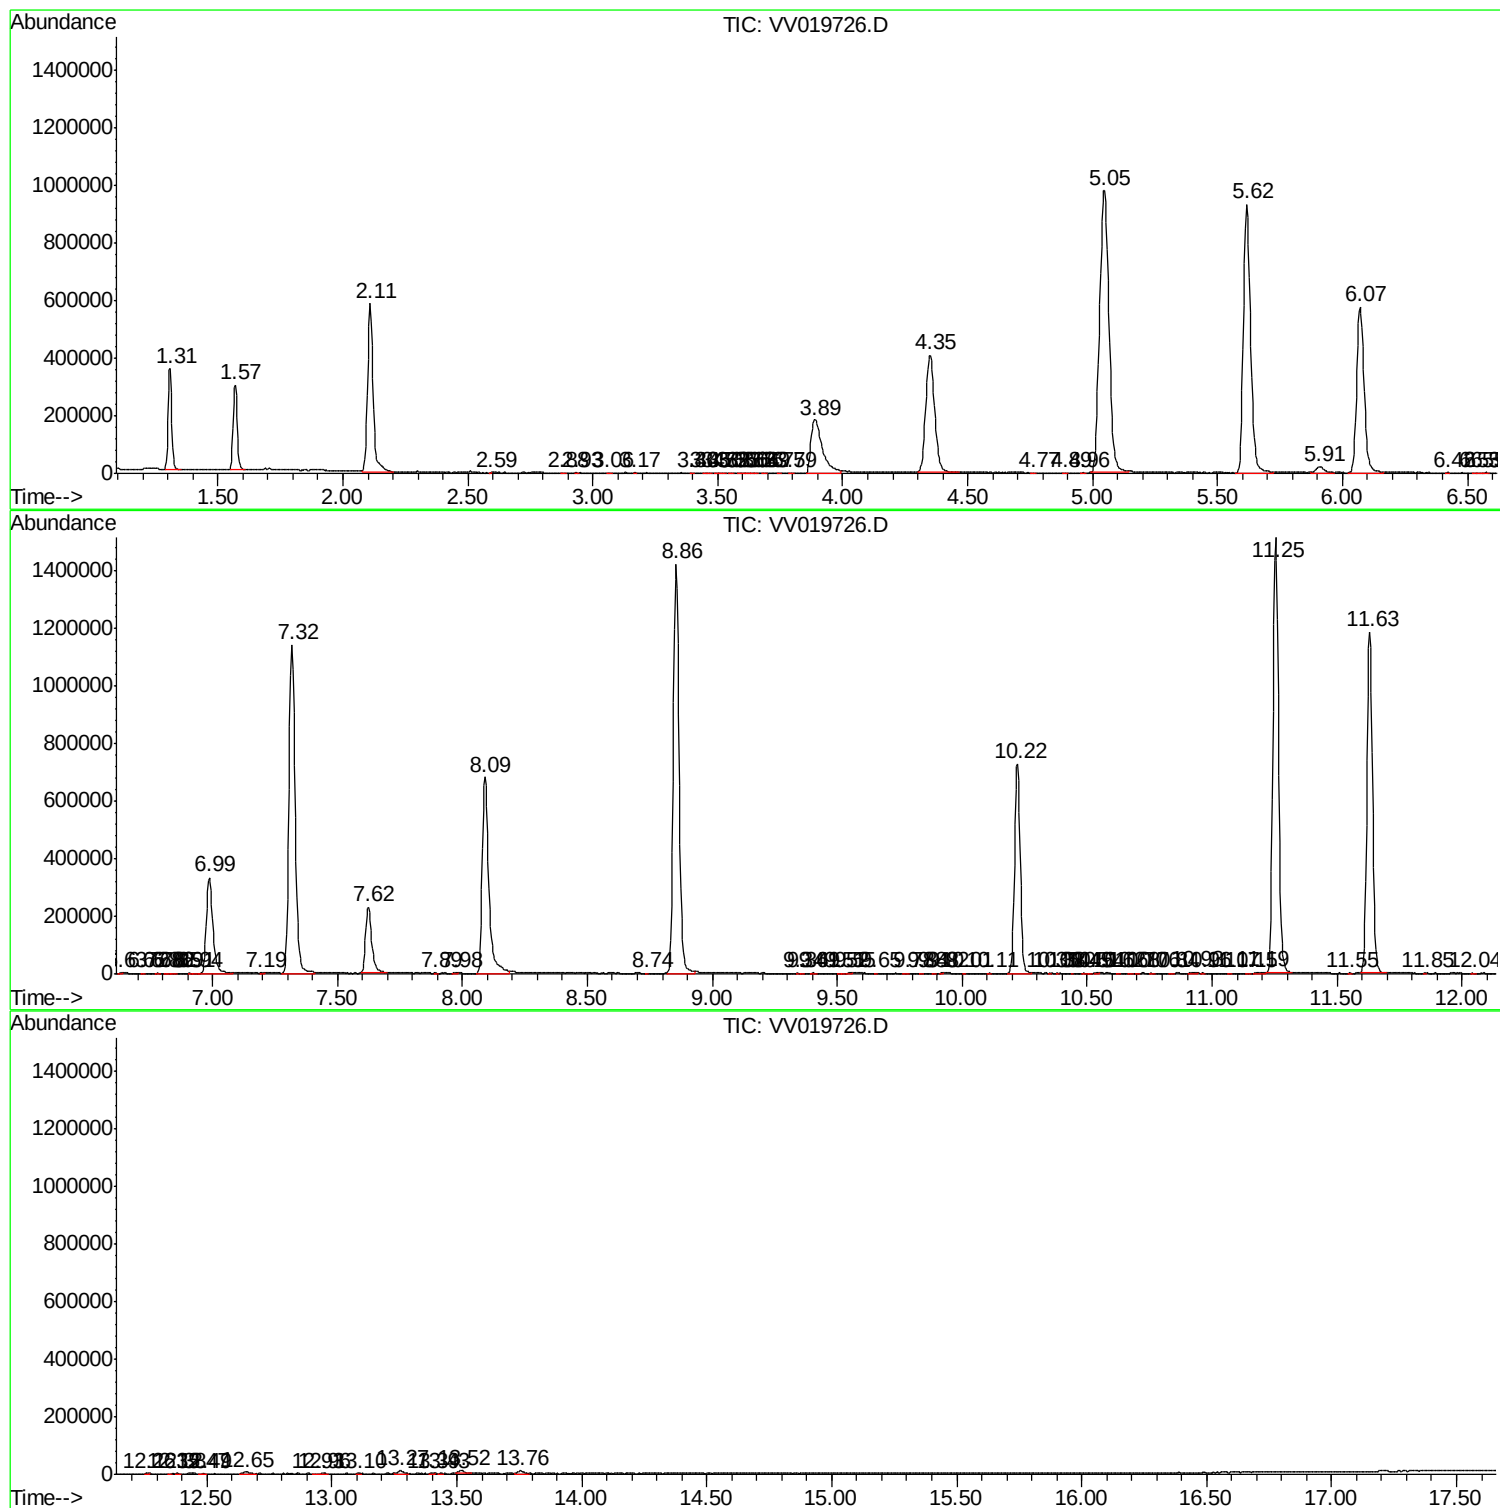

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121920\
Data File : VV019726.D
Acq On : 19 Dec 2020 09:59
Operator : SY/MD
Sample : VV1219WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK74

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121920\
Data File : VV019726.D
Acq On : 19 Dec 2020 09:59
Operator : SY/MD
Sample : VV1219WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK74

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc