

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019731.D
 Acq On : 19 Dec 2020 12:30
 Operator : SY/MD
 Sample : L5099-06 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Q3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.110	3	6	14	rVB	69877	57205	1.77%	0.233%
2	1.309	62	68	80	rVB	349509	366053	11.31%	1.491%
3	1.569	143	149	163	rVB	291740	327635	10.12%	1.335%
4	2.110	308	317	348	rVB	548793	865722	26.75%	3.527%
5	2.624	469	477	478	rBV5	1448	1869	0.06%	0.008%
6	2.772	511	523	546	rVB	145403	302843	9.36%	1.234%
7	3.122	630	632	634	rBV2	707	359	0.01%	0.001%
8	3.203	654	657	659	rBV2	803	549	0.02%	0.002%
9	3.254	671	673	676	rBV3	1008	627	0.02%	0.003%
10	3.450	732	734	736	rVB3	535	173	0.01%	0.001%
11	3.470	736	740	744	rBV4	931	756	0.02%	0.003%
12	3.505	749	751	754	rBV2	741	465	0.01%	0.002%
13	3.646	793	795	796	rBV	282	91	0.00%	0.000%
14	3.659	796	799	802	rVV3	519	318	0.01%	0.001%
15	3.749	826	827	830	rBV2	783	493	0.02%	0.002%
16	3.888	859	870	916	rBV	220901	694906	21.47%	2.831%
17	4.354	1000	1015	1040	rBV	420742	1028813	31.79%	4.191%
18	4.711	1124	1126	1127	rBV2	487	172	0.01%	0.001%
19	4.843	1164	1167	1170	rBV4	840	643	0.02%	0.003%
20	4.913	1187	1189	1192	rBV2	630	394	0.01%	0.002%
21	4.936	1193	1196	1197	rBV2	314	139	0.00%	0.001%
22	5.052	1214	1232	1245	rBV2	1005426	2636003	81.46%	10.738%
23	5.460	1357	1359	1360	rBV	982	434	0.01%	0.002%
24	5.621	1396	1409	1438	rBV	854029	1713331	52.95%	6.980%
25	5.920	1487	1502	1527	rBV2	434234	880565	27.21%	3.587%
26	6.074	1537	1550	1577	rBV	603993	1204408	37.22%	4.906%
27	6.450	1662	1667	1669	rBV4	1118	906	0.03%	0.004%
28	6.511	1682	1686	1687	rBV3	808	642	0.02%	0.003%
29	6.524	1687	1690	1695	rVB5	758	770	0.02%	0.003%
30	6.569	1700	1704	1707	rBV4	727	714	0.02%	0.003%
31	6.746	1756	1759	1762	rBV5	1011	698	0.02%	0.003%
32	6.875	1796	1799	1802	rBV3	974	701	0.02%	0.003%
33	6.932	1815	1817	1820	rBV2	641	356	0.01%	0.001%
34	6.990	1820	1835	1861	rBV	326205	596353	18.43%	2.429%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019731.D
 Acq On : 19 Dec 2020 12:30
 Operator : SY/MD
 Sample : L5099-06 10X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Q3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	7.318	1925	1937	1962	rBV	1099682	1913028	59.12%	7.793%
36	7.624	2022	2032	2062	rBV	224153	400352	12.37%	1.631%
37	7.884	2110	2113	2116	rBV4	1015	962	0.03%	0.004%
38	7.977	2128	2142	2164	rBV	1927585	3236042	100.00%	13.183%
39	8.090	2168	2177	2208	rVV	748915	1345381	41.57%	5.481%
40	8.762	2384	2386	2387	rBV2	556	251	0.01%	0.001%
41	8.855	2403	2415	2436	rBV	1263137	2035996	62.92%	8.294%
42	9.299	2551	2553	2556	rBV2	636	371	0.01%	0.002%
43	9.357	2569	2571	2573	rBV2	709	397	0.01%	0.002%
44	9.415	2586	2589	2591	rBV3	949	558	0.02%	0.002%
45	9.781	2701	2703	2704	rBV	648	273	0.01%	0.001%
46	9.881	2732	2734	2736	rVB	565	169	0.01%	0.001%
47	10.000	2769	2771	2775	rBV2	568	514	0.02%	0.002%
48	10.093	2797	2800	2805	rBV3	737	870	0.03%	0.004%
49	10.164	2819	2822	2825	rVB4	546	329	0.01%	0.001%
50	10.222	2827	2840	2860	rVV	779247	1218018	37.64%	4.962%
51	10.350	2877	2880	2881	rBV2	770	440	0.01%	0.002%
52	10.379	2887	2889	2892	rBV2	1281	569	0.02%	0.002%
53	10.440	2906	2908	2913	rVB3	917	640	0.02%	0.003%
54	10.463	2913	2915	2916	rBV	393	149	0.00%	0.001%
55	10.598	2955	2957	2959	rBV3	825	364	0.01%	0.001%
56	10.633	2966	2968	2972	rBV4	840	609	0.02%	0.002%
57	10.762	3002	3008	3011	rBV4	853	1030	0.03%	0.004%
58	10.775	3011	3012	3015	rBV2	656	313	0.01%	0.001%
59	10.842	3029	3033	3034	rBV2	603	449	0.01%	0.002%
60	11.016	3083	3087	3091	rBV5	1179	905	0.03%	0.004%
61	11.135	3122	3124	3126	rBV2	385	141	0.00%	0.001%
62	11.254	3149	3161	3184	rBV	1249210	1906200	58.91%	7.765%
63	11.630	3266	3278	3294	rBV	1155088	1783563	55.12%	7.266%
64	12.058	3409	3411	3414	rBV2	776	479	0.01%	0.002%
65	12.119	3427	3430	3431	rBV2	662	434	0.01%	0.002%
66	12.138	3434	3436	3437	rBV3	778	335	0.01%	0.001%
67	12.241	3466	3468	3470	rBV2	1044	688	0.02%	0.003%
68	12.421	3521	3524	3529	rBV3	682	585	0.02%	0.002%
69	12.450	3529	3533	3538	rBV7	1310	1126	0.03%	0.005%
70	12.511	3547	3552	3555	rBV5	1120	941	0.03%	0.004%
71	12.553	3563	3565	3568	rBV2	805	542	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
Data File : VV019731.D
Acq On : 19 Dec 2020 12:30
Operator : SY/MD
Sample : L5099-06 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Q3

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Title : VOC Analysis

72	12.826	3649	3650	3657	rVB5	813	639	0.02%	0.003%
73	12.868	3659	3663	3668	rBV4	1023	861	0.03%	0.004%
74	13.132	3743	3745	3746	rBV	663	352	0.01%	0.001%
75	13.270	3786	3788	3790	rBV3	1250	818	0.03%	0.003%
76	14.045	4022	4029	4034	rBV6	2162	3197	0.10%	0.013%
77	15.218	4392	4394	4399	rBV4	1639	1441	0.04%	0.006%


Sum of corrected areas: 24547427

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121920\
Data File : VV019731.D
Acq On : 19 Dec 2020 12:30
Operator : SY/MD
Sample : L5099-06 10X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Q3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

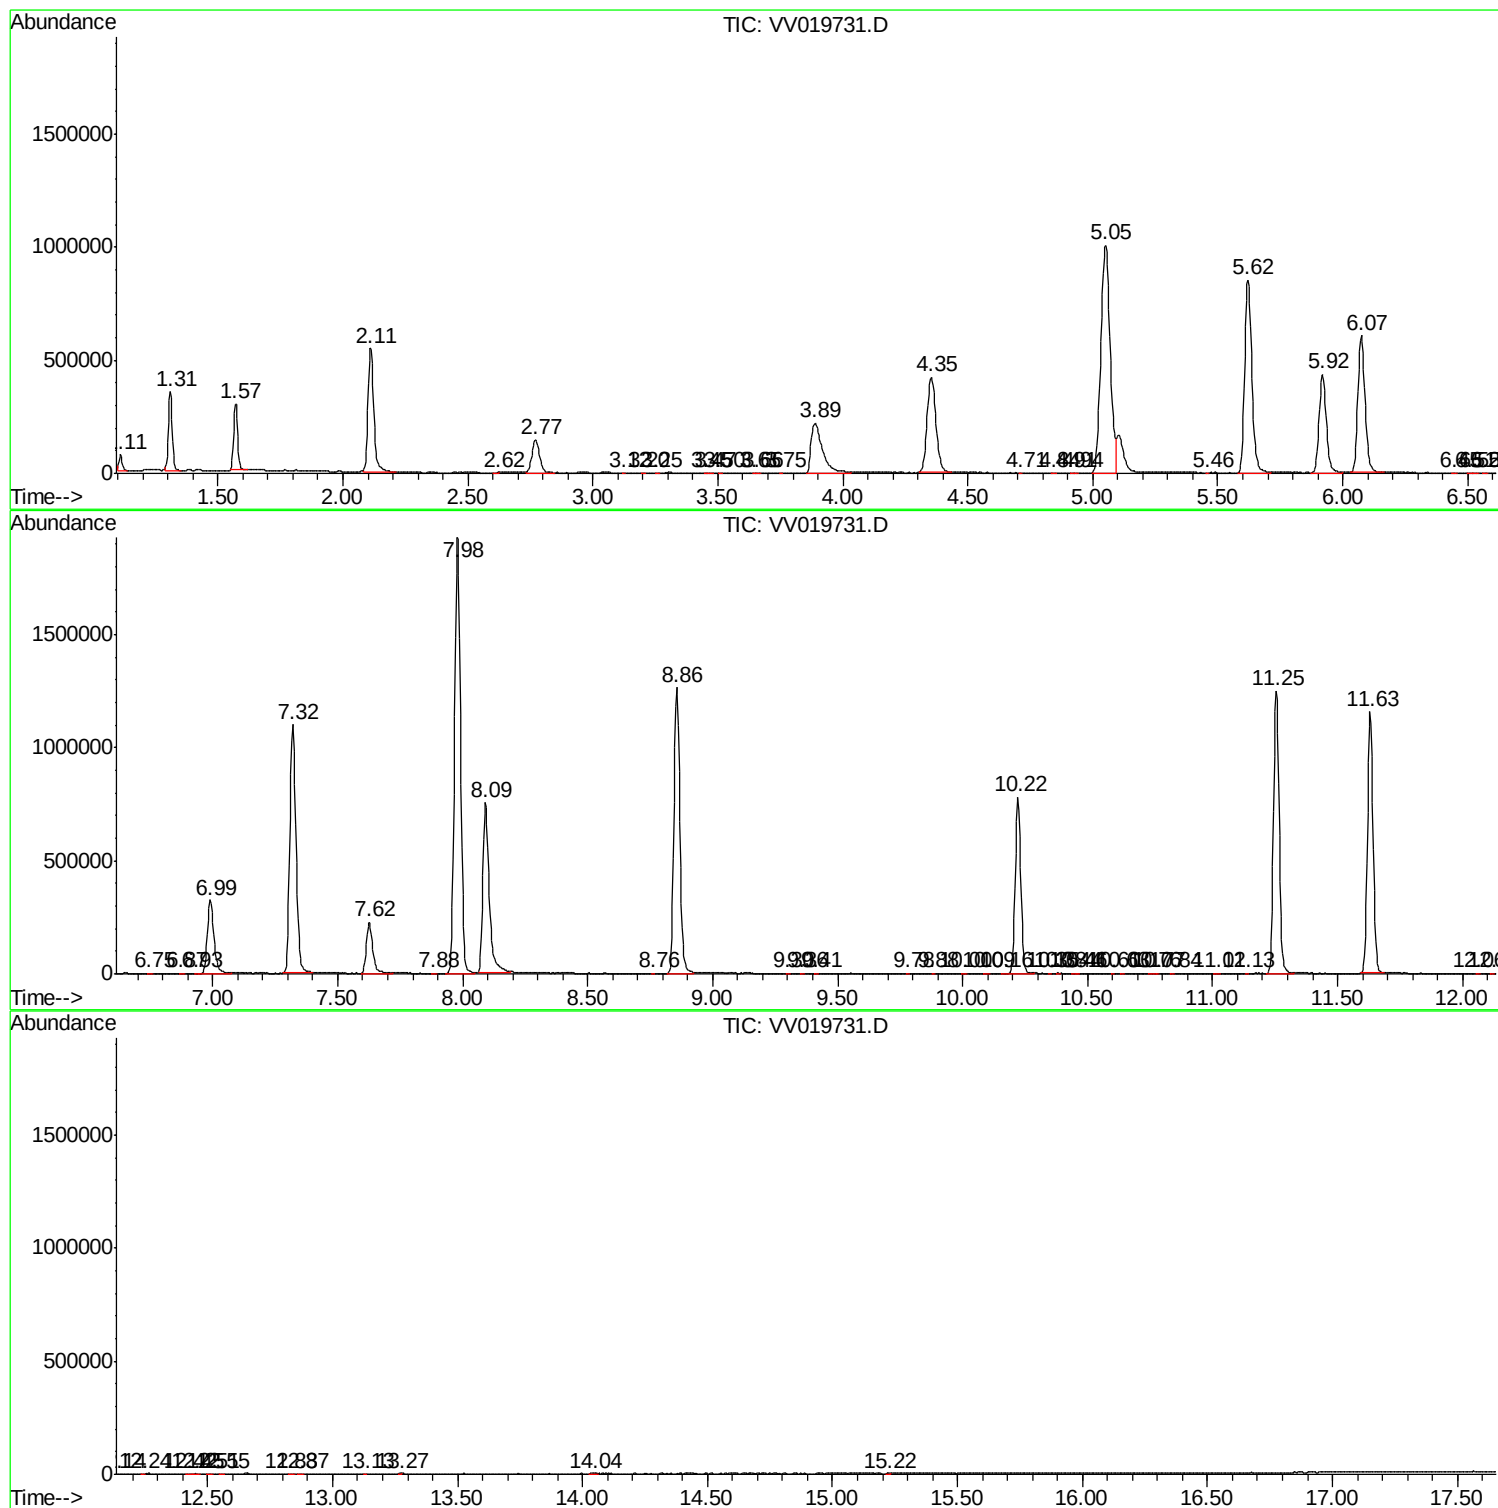

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121920\
Data File : VV019731.D
Acq On : 19 Dec 2020 12:30
Operator : SY/MD
Sample : L5099-06 10X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4Q3

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121920\
Data File : VV019731.D
Acq On : 19 Dec 2020 12:30
Operator : SY/MD
Sample : L5099-06 10X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4Q3

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc