

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019733.D
 Acq On : 19 Dec 2020 13:24
 Operator : SY/MD
 Sample : L5099-04 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4P9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.110	3	6	17	rVB	83428	69221	1.06%	0.227%
2	1.309	60	68	81	rVB	428102	452000	6.94%	1.485%
3	1.386	87	92	98	rBV	18790	19870	0.31%	0.065%
4	1.570	142	149	160	rBV	331995	368512	5.66%	1.210%
5	2.110	305	317	359	rVB	685254	1105057	16.97%	3.630%
6	2.354	386	393	401	rVB5	3820	6060	0.09%	0.020%
7	2.650	479	485	486	rBV5	2004	1599	0.02%	0.005%
8	2.769	511	522	538	rVB	79190	164397	2.53%	0.540%
9	2.933	569	573	574	rBV3	2087	1341	0.02%	0.004%
10	2.962	575	582	591	rVB9	3929	8086	0.12%	0.027%
11	3.045	596	608	623	rVV2	33765	66707	1.02%	0.219%
12	3.261	671	675	677	rBV	646	574	0.01%	0.002%
13	3.438	726	730	732	rBV2	737	649	0.01%	0.002%
14	3.512	749	753	756	rBV2	1225	1022	0.02%	0.003%
15	3.621	784	787	790	rBV4	978	665	0.01%	0.002%
16	3.766	815	832	845	rVV3	17692	48471	0.74%	0.159%
17	3.888	858	870	905	rBV	189404	602551	9.26%	1.979%
18	4.113	938	940	948	rVB7	2121	1790	0.03%	0.006%
19	4.148	948	951	954	rBV5	1116	820	0.01%	0.003%
20	4.351	995	1014	1041	rBV	448303	1107231	17.01%	3.637%
21	4.772	1142	1145	1149	rVB2	789	605	0.01%	0.002%
22	5.049	1211	1231	1272	rBV2	1104992	2905950	44.64%	9.545%
23	5.618	1394	1408	1435	rBV	880163	1776113	27.28%	5.834%
24	5.917	1484	1501	1535	rBV	869520	1725088	26.50%	5.666%
25	6.071	1536	1549	1572	rBV	635498	1275369	19.59%	4.189%
26	6.569	1701	1704	1710	rVB4	1016	804	0.01%	0.003%
27	6.643	1724	1727	1733	rVB6	1186	1008	0.02%	0.003%
28	6.814	1778	1780	1787	rVB7	1042	703	0.01%	0.002%
29	6.923	1812	1814	1817	rVB	1524	708	0.01%	0.002%
30	6.987	1822	1834	1860	rBV	373136	676523	10.39%	2.222%
31	7.238	1909	1912	1917	rBV5	1320	1285	0.02%	0.004%
32	7.319	1924	1937	1956	rBV	1317796	2271331	34.89%	7.461%
33	7.624	2021	2032	2055	rBV	258442	447297	6.87%	1.469%
34	7.978	2127	2142	2166	rBV	3918320	6510239	100.00%	21.384%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019733.D
 Acq On : 19 Dec 2020 13:24
 Operator : SY/MD
 Sample : L5099-04 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4P9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	8.090	2167	2177	2217	rVB	659297	1201410	18.45%	3.946%
36	8.515	2306	2309	2312	rBV3	872	632	0.01%	0.002%
37	8.563	2319	2324	2326	rBV6	935	859	0.01%	0.003%
38	8.691	2360	2364	2367	rBV4	771	692	0.01%	0.002%
39	8.855	2400	2415	2445	rBV	1345462	2185466	33.57%	7.179%
40	9.026	2461	2468	2475	rVB6	4481	6865	0.11%	0.023%
41	9.148	2500	2506	2513	rBV8	1923	2781	0.04%	0.009%
42	9.219	2525	2528	2531	rVB4	1279	880	0.01%	0.003%
43	9.331	2561	2563	2568	rVB5	961	780	0.01%	0.003%
44	9.457	2599	2602	2604	rVB	919	619	0.01%	0.002%
45	9.482	2604	2610	2612	rBV7	1052	968	0.01%	0.003%
46	9.521	2616	2622	2623	rBV5	991	957	0.01%	0.003%
47	9.566	2633	2636	2642	rVB6	1573	1563	0.02%	0.005%
48	9.656	2661	2664	2670	rVB4	711	769	0.01%	0.003%
49	9.714	2679	2682	2687	rBV6	895	846	0.01%	0.003%
50	9.817	2710	2714	2725	rVB8	2660	4360	0.07%	0.014%
51	9.942	2749	2753	2755	rBV3	845	662	0.01%	0.002%
52	10.003	2769	2772	2777	rVB5	835	792	0.01%	0.003%
53	10.142	2810	2815	2818	rBV3	1206	801	0.01%	0.003%
54	10.219	2826	2839	2865	rBV	766107	1202052	18.46%	3.948%
55	10.486	2916	2922	2924	rBV3	769	606	0.01%	0.002%
56	10.579	2945	2951	2952	rBV4	1618	1132	0.02%	0.004%
57	10.598	2952	2957	2964	rVB6	1670	2242	0.03%	0.007%
58	10.781	3012	3014	3019	rVB5	951	829	0.01%	0.003%
59	10.852	3031	3036	3038	rBV3	975	982	0.02%	0.003%
60	11.052	3095	3098	3099	rBV2	1056	629	0.01%	0.002%
61	11.161	3124	3132	3138	rBV9	3978	7008	0.11%	0.023%
62	11.254	3149	3161	3181	rBV	1370124	2106390	32.36%	6.919%
63	11.460	3222	3225	3228	rVV4	1273	807	0.01%	0.003%
64	11.476	3228	3230	3233	rVB5	1120	638	0.01%	0.002%
65	11.502	3233	3238	3241	rVB5	1197	823	0.01%	0.003%
66	11.630	3265	3278	3297	rBV	1307013	2049274	31.48%	6.731%
67	12.003	3391	3394	3400	rBV4	921	1022	0.02%	0.003%
68	12.096	3420	3423	3427	rVB3	862	715	0.01%	0.002%
69	12.125	3427	3432	3435	rVB7	861	839	0.01%	0.003%
70	12.148	3435	3439	3441	rBV2	1020	676	0.01%	0.002%
71	12.360	3497	3505	3511	rBV8	3396	4669	0.07%	0.015%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019733.D
 Acq On : 19 Dec 2020 13:24
 Operator : SY/MD
 Sample : L5099-04 5X
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4P9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	12.431	3524	3527	3531	rVB4	1187	835	0.01%	0.003%
73	12.514	3551	3553	3557	rVB2	1137	620	0.01%	0.002%
74	12.556	3557	3566	3569	rBV5	1237	1611	0.02%	0.005%
75	12.698	3608	3610	3615	rVB4	1024	582	0.01%	0.002%
76	12.794	3637	3640	3642	rBV3	932	605	0.01%	0.002%
77	12.846	3651	3656	3658	rBV2	1026	881	0.01%	0.003%
78	12.891	3665	3670	3671	rBV5	994	797	0.01%	0.003%
79	13.006	3700	3706	3710	rBV6	873	1197	0.02%	0.004%
80	13.051	3716	3720	3729	rBV8	1671	2408	0.04%	0.008%
81	13.273	3782	3789	3793	rBV6	2016	2550	0.04%	0.008%
82	13.418	3830	3834	3837	rVB3	1493	983	0.02%	0.003%
83	13.518	3862	3865	3866	rBV3	1403	748	0.01%	0.002%
84	13.608	3889	3893	3895	rBV2	968	679	0.01%	0.002%
85	13.630	3897	3900	3906	rVB5	1371	998	0.02%	0.003%
86	13.711	3922	3925	3929	rVB5	1451	1115	0.02%	0.004%
87	13.785	3944	3948	3951	rVB3	1459	1162	0.02%	0.004%
88	13.920	3986	3990	3997	rVB6	1181	1296	0.02%	0.004%
89	13.971	4001	4006	4008	rBV5	950	839	0.01%	0.003%
90	14.032	4022	4025	4029	rBV5	926	717	0.01%	0.002%
91	14.106	4042	4048	4052	rBV5	1441	1940	0.03%	0.006%
92	14.289	4101	4105	4107	rBV4	1281	958	0.01%	0.003%
93	14.524	4173	4178	4180	rBV3	681	657	0.01%	0.002%
94	14.617	4205	4207	4210	rVB4	1217	638	0.01%	0.002%
95	15.087	4348	4353	4355	rBV3	1145	1004	0.02%	0.003%
96	15.109	4355	4360	4362	rBV6	1196	1009	0.02%	0.003%
97	15.231	4395	4398	4401	rBV3	813	720	0.01%	0.002%
98	15.357	4433	4437	4440	rBV4	1134	1147	0.02%	0.004%
99	15.688	4537	4540	4543	rBV5	1409	941	0.01%	0.003%
100	15.846	4586	4589	4590	rBV3	1265	722	0.01%	0.002%


Sum of corrected areas: 30444040

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121920\
Data File : VV019733.D
Acq On : 19 Dec 2020 13:24
Operator : SY/MD
Sample : L5099-04 5X
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4P9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

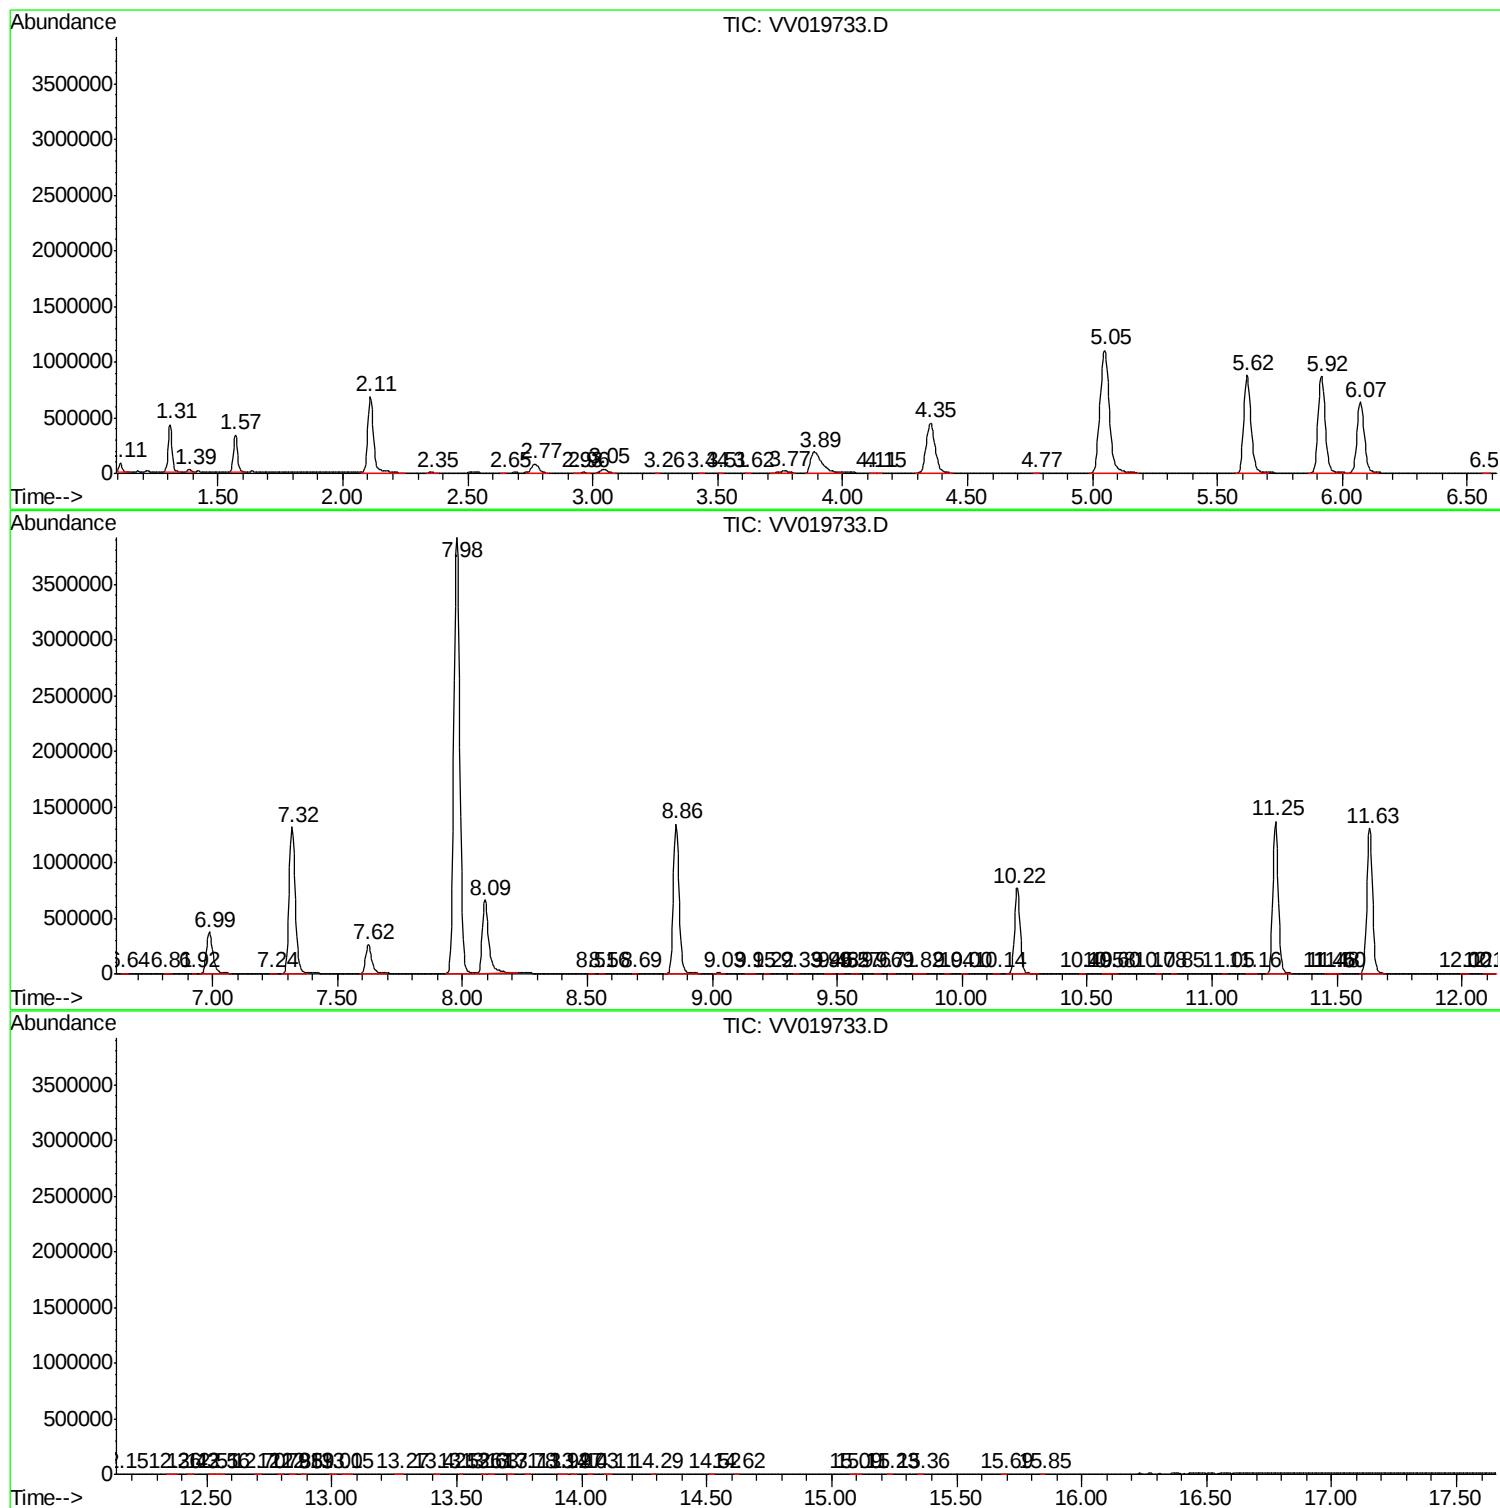

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121920\
Data File : VV019733.D
Acq On : 19 Dec 2020 13:24
Operator : SY/MD
Sample : L5099-04 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4P9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121920\
Data File : VV019733.D
Acq On : 19 Dec 2020 13:24
Operator : SY/MD
Sample : L5099-04 5X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BG4P9

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc