

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019734.D
 Acq On : 19 Dec 2020 13:50
 Operator : SY/MD
 Sample : VIBLK65
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	80	rVB	347130	335753	13.37%	1.675%
2	1.569	142	149	163	rBV	287744	325379	12.95%	1.623%
3	2.110	308	317	355	rVB	565959	885369	35.25%	4.416%
4	2.756	516	518	519	rBV	961	381	0.02%	0.002%
5	2.923	567	570	578	rVB6	1076	1131	0.05%	0.006%
6	2.955	578	580	583	rBV2	548	287	0.01%	0.001%
7	3.019	595	600	603	rBV5	934	857	0.03%	0.004%
8	3.064	612	614	619	rBV3	753	583	0.02%	0.003%
9	3.148	638	640	643	rBV2	685	289	0.01%	0.001%
10	3.360	703	706	709	rVB3	807	587	0.02%	0.003%
11	3.380	709	712	713	rBV2	329	206	0.01%	0.001%
12	3.392	714	716	719	rVV4	434	200	0.01%	0.001%
13	3.428	724	727	728	rBV2	862	489	0.02%	0.002%
14	3.447	731	733	735	rBV3	589	265	0.01%	0.001%
15	3.505	749	751	752	rBV2	543	156	0.01%	0.001%
16	3.531	757	759	762	rBV2	562	261	0.01%	0.001%
17	3.566	768	770	772	rBV2	493	138	0.01%	0.001%
18	3.653	795	797	798	rVB2	564	187	0.01%	0.001%
19	3.675	800	804	805	rVV2	843	595	0.02%	0.003%
20	3.701	809	812	815	rBV3	426	329	0.01%	0.002%
21	3.717	815	817	819	rBV2	518	256	0.01%	0.001%
22	3.740	822	824	825	rBV	557	224	0.01%	0.001%
23	3.769	831	833	837	rBV3	658	314	0.01%	0.002%
24	3.794	837	841	843	rBV3	823	456	0.02%	0.002%
25	3.833	850	853	855	rBV3	551	353	0.01%	0.002%
26	3.894	860	872	911	rBV	189119	619042	24.64%	3.088%
27	4.351	1000	1014	1042	rVB	402013	984741	39.20%	4.912%
28	4.653	1106	1108	1109	rBV2	908	413	0.02%	0.002%
29	4.756	1136	1140	1143	rBV3	801	773	0.03%	0.004%
30	4.814	1154	1158	1161	rVB4	1052	708	0.03%	0.004%
31	4.830	1161	1163	1166	rBV3	500	361	0.01%	0.002%
32	4.968	1203	1206	1207	rBV3	480	251	0.01%	0.001%
33	5.048	1214	1231	1258	rBV2	974190	2511943	100.00%	12.529%
34	5.392	1336	1338	1341	rBV3	803	591	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019734.D
 Acq On : 19 Dec 2020 13:50
 Operator : SY/MD
 Sample : VIBLK65
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	5.572	1390	1394	1396	rBV3	1299	981	0.04%	0.005%
36	5.617	1396	1408	1438	rVV	872622	1752959	69.78%	8.743%
37	5.907	1488	1498	1513	rBV3	23897	52044	2.07%	0.260%
38	6.071	1536	1549	1580	rBV	567309	1156065	46.02%	5.766%
39	6.344	1632	1634	1636	rBV2	870	473	0.02%	0.002%
40	6.357	1636	1638	1642	rVV4	785	540	0.02%	0.003%
41	6.428	1657	1660	1663	rBV3	560	421	0.02%	0.002%
42	6.447	1663	1666	1668	rVV3	936	555	0.02%	0.003%
43	6.511	1685	1686	1690	rVB3	490	185	0.01%	0.001%
44	6.736	1754	1756	1758	rBV2	511	298	0.01%	0.001%
45	6.772	1764	1767	1768	rBV2	676	373	0.01%	0.002%
46	6.804	1774	1777	1778	rBV2	585	383	0.02%	0.002%
47	6.826	1782	1784	1788	rVB4	709	497	0.02%	0.002%
48	6.894	1803	1805	1807	rBV3	765	358	0.01%	0.002%
49	6.987	1823	1834	1856	rBV	305129	563698	22.44%	2.812%
50	7.318	1924	1937	1964	rBV	1105656	1926886	76.71%	9.611%
51	7.624	2022	2032	2057	rBV	217569	377774	15.04%	1.884%
52	8.090	2167	2177	2215	rBV	692778	1300800	51.78%	6.488%
53	8.662	2353	2355	2356	rBV2	689	246	0.01%	0.001%
54	8.855	2401	2415	2438	rBV	1346510	2151484	85.65%	10.731%
55	9.109	2492	2494	2495	rBV	772	292	0.01%	0.001%
56	9.248	2535	2537	2538	rBV	629	221	0.01%	0.001%
57	9.379	2576	2578	2581	rBV3	939	506	0.02%	0.003%
58	9.521	2620	2622	2626	rBV3	465	272	0.01%	0.001%
59	9.540	2626	2628	2629	rBV2	778	333	0.01%	0.002%
60	9.701	2677	2678	2679	rBV	500	113	0.00%	0.001%
61	9.846	2721	2723	2730	rVB5	956	782	0.03%	0.004%
62	9.871	2730	2731	2732	rBV	453	128	0.01%	0.001%
63	10.064	2787	2791	2793	rBV3	783	693	0.03%	0.003%
64	10.129	2806	2811	2813	rBV3	977	749	0.03%	0.004%
65	10.164	2820	2822	2827	rBV5	563	587	0.02%	0.003%
66	10.222	2827	2840	2865	rVV	731592	1154352	45.95%	5.758%
67	10.585	2947	2953	2959	rBV8	1084	1386	0.06%	0.007%
68	10.611	2959	2961	2964	rBV2	775	660	0.03%	0.003%
69	10.701	2986	2989	2992	rBV3	580	612	0.02%	0.003%
70	10.919	3052	3057	3060	rBV5	945	1056	0.04%	0.005%
71	10.964	3069	3071	3072	rBV	466	179	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019734.D
 Acq On : 19 Dec 2020 13:50
 Operator : SY/MD
 Sample : VIBLK65
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK65

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.993	3076	3080	3084	rBV3	792	660	0.03%	0.003%
73	11.254	3150	3161	3184	rBV	1396835	2115563	84.22%	10.552%
74	11.630	3266	3278	3296	rBV	1147113	1804472	71.84%	9.000%
75	11.939	3371	3374	3378	rBV2	633	516	0.02%	0.003%
76	12.064	3411	3413	3414	rBV2	656	243	0.01%	0.001%
77	12.218	3458	3461	3464	rBV2	561	543	0.02%	0.003%
78	12.392	3513	3515	3518	rBV3	840	490	0.02%	0.002%
79	12.415	3518	3522	3524	rBV5	786	652	0.03%	0.003%
80	12.624	3583	3587	3589	rBV3	675	582	0.02%	0.003%
81	12.878	3664	3666	3668	rBV4	644	338	0.01%	0.002%
82	12.977	3695	3697	3702	rBV2	708	561	0.02%	0.003%
83	13.067	3724	3725	3730	rVB2	888	486	0.02%	0.002%
84	13.164	3753	3755	3756	rBV	479	229	0.01%	0.001%


Sum of corrected areas: 20049144

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121920\
Data File : VV019734.D
Acq On : 19 Dec 2020 13:50
Operator : SY/MD
Sample : VIBLK65
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK65

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

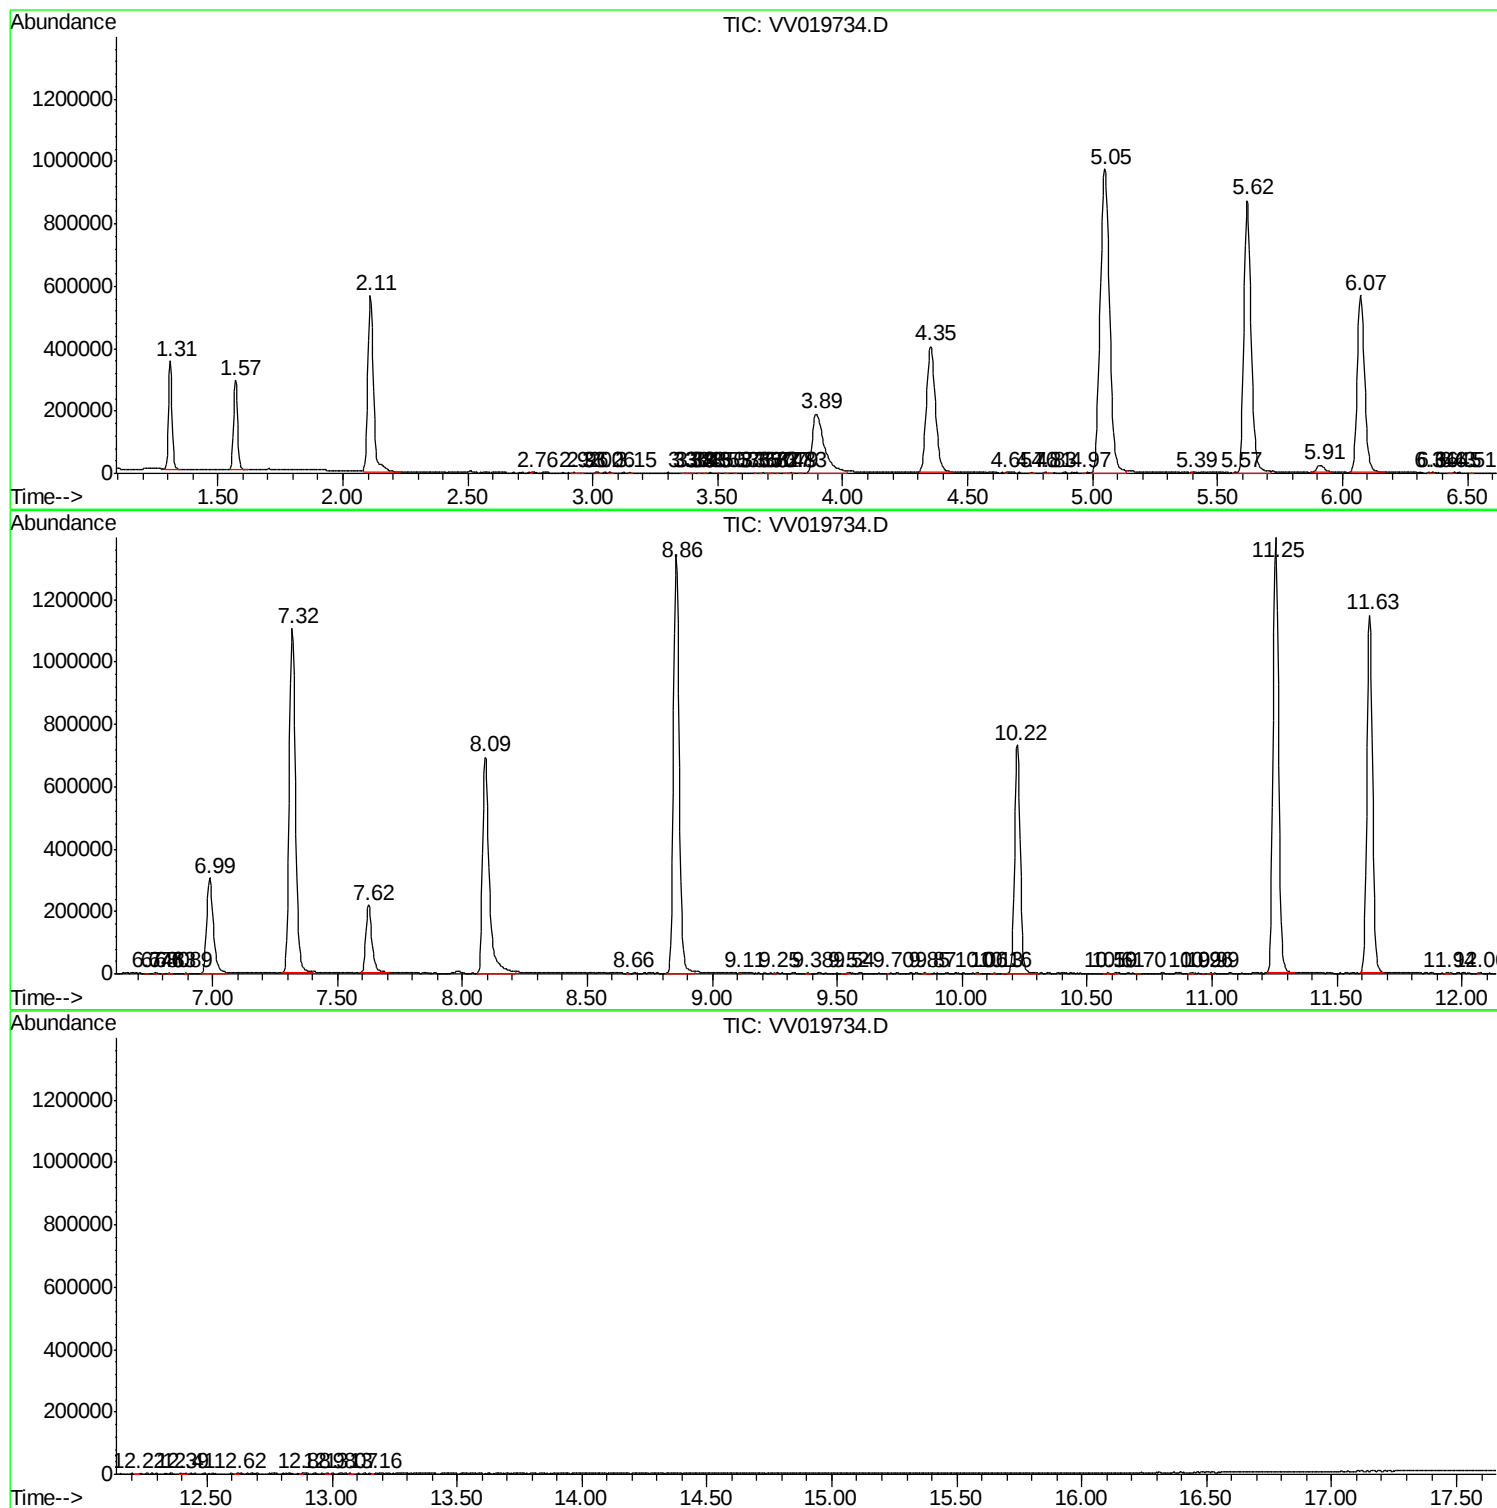

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121920\
Data File : VV019734.D
Acq On : 19 Dec 2020 13:50
Operator : SY/MD
Sample : VIBLK65
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK65

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121920\
Data File : VV019734.D
Acq On : 19 Dec 2020 13:50
Operator : SY/MD
Sample : VIBLK65
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VIBLK65

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc