

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019743.D
 Acq On : 19 Dec 2020 17:25
 Operator : SY/MD
 Sample : L5151-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	82	rVB	398449	395607	14.52%	1.867%
2	1.386	87	92	104	rVB	12964	15537	0.57%	0.073%
3	1.569	141	149	164	rBV	311761	352811	12.95%	1.665%
4	2.109	307	317	333	rBV	644990	960051	35.23%	4.530%
5	2.386	401	403	410	rBV6	838	839	0.03%	0.004%
6	2.611	465	473	474	rBV4	2738	2387	0.09%	0.011%
7	2.862	549	551	554	rBV4	979	559	0.02%	0.003%
8	2.958	579	581	585	rBV2	861	713	0.03%	0.003%
9	3.093	619	623	626	rVB3	795	715	0.03%	0.003%
10	3.113	626	629	632	rBV3	1202	885	0.03%	0.004%
11	3.315	690	692	698	rVB3	980	763	0.03%	0.004%
12	3.347	698	702	706	rBV5	760	670	0.02%	0.003%
13	3.408	717	721	723	rBV3	991	815	0.03%	0.004%
14	3.540	755	762	763	rBV4	636	652	0.02%	0.003%
15	3.669	795	802	803	rBV4	2962	2561	0.09%	0.012%
16	3.688	804	808	821	rVB6	4163	7995	0.29%	0.038%
17	3.891	857	871	912	rBV2	216063	716414	26.29%	3.381%
18	4.354	998	1015	1042	rBV	428158	1055629	38.74%	4.981%
19	4.862	1170	1173	1176	rBV3	946	563	0.02%	0.003%
20	4.965	1201	1205	1207	rBV3	856	661	0.02%	0.003%
21	5.048	1213	1231	1266	rBV2	1053488	2725210	100.00%	12.860%
22	5.621	1391	1409	1439	rBV	890959	1774561	65.12%	8.374%
23	5.797	1457	1464	1469	rVB8	1933	2152	0.08%	0.010%
24	5.907	1489	1498	1517	rVB3	32174	65672	2.41%	0.310%
25	6.074	1534	1550	1571	rBV	599175	1235110	45.32%	5.828%
26	6.357	1632	1638	1641	rBV8	887	1045	0.04%	0.005%
27	6.431	1657	1661	1662	rBV4	1045	786	0.03%	0.004%
28	6.540	1688	1695	1700	rBV9	2038	3194	0.12%	0.015%
29	6.656	1729	1731	1736	rVB4	1160	848	0.03%	0.004%
30	6.749	1757	1760	1762	rVV4	1178	595	0.02%	0.003%
31	6.785	1767	1771	1774	rVB4	955	658	0.02%	0.003%
32	6.804	1774	1777	1781	rBV3	986	657	0.02%	0.003%
33	6.900	1802	1807	1810	rBV6	1000	1037	0.04%	0.005%
34	6.987	1821	1834	1860	rBV	345802	628810	23.07%	2.967%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019743.D
 Acq On : 19 Dec 2020 17:25
 Operator : SY/MD
 Sample : L5151-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	7.264	1918	1920	1924	rVB4	1033	659	0.02%	0.003%
36	7.318	1924	1937	1964	rBV	1242146	2150027	78.89%	10.146%
37	7.624	2021	2032	2060	rVV	238484	418569	15.36%	1.975%
38	7.916	2118	2123	2126	rBV6	1335	1498	0.05%	0.007%
39	7.984	2136	2144	2154	rVB7	3495	6800	0.25%	0.032%
40	8.090	2167	2177	2213	rBV	644825	1210218	44.41%	5.711%
41	8.585	2328	2331	2337	rBV4	906	605	0.02%	0.003%
42	8.617	2337	2341	2346	rBV6	1024	944	0.03%	0.004%
43	8.707	2367	2369	2375	rVB5	1250	840	0.03%	0.004%
44	8.736	2375	2378	2382	rBV4	1020	872	0.03%	0.004%
45	8.765	2382	2387	2390	rBV4	939	980	0.04%	0.005%
46	8.855	2403	2415	2439	rBV	1332824	2159540	79.24%	10.191%
47	8.987	2454	2456	2461	rVB3	1260	826	0.03%	0.004%
48	9.067	2479	2481	2483	rBV2	1005	587	0.02%	0.003%
49	9.151	2504	2507	2510	rBV5	1054	835	0.03%	0.004%
50	9.183	2515	2517	2522	rBV4	920	923	0.03%	0.004%
51	9.405	2581	2586	2587	rBV3	753	549	0.02%	0.003%
52	9.447	2598	2599	2607	rVB6	948	795	0.03%	0.004%
53	9.604	2642	2648	2649	rBV4	1495	1142	0.04%	0.005%
54	9.611	2649	2650	2653	rVB3	952	566	0.02%	0.003%
55	9.717	2677	2683	2691	rBV5	3982	6764	0.25%	0.032%
56	9.823	2706	2716	2717	rBV3	1342	1790	0.07%	0.008%
57	10.029	2776	2780	2783	rBV5	779	646	0.02%	0.003%
58	10.222	2827	2840	2863	rBV	718783	1146093	42.06%	5.408%
59	10.392	2886	2893	2896	rBV7	1694	2365	0.09%	0.011%
60	10.418	2898	2901	2906	rVB6	846	636	0.02%	0.003%
61	10.444	2906	2909	2912	rVB3	912	598	0.02%	0.003%
62	10.469	2912	2917	2924	rVB6	1468	1969	0.07%	0.009%
63	10.521	2924	2933	2936	rBV6	1290	1613	0.06%	0.008%
64	10.582	2946	2952	2953	rBV4	1492	1423	0.05%	0.007%
65	10.675	2978	2981	2986	rVB3	623	558	0.02%	0.003%
66	10.726	2992	2997	2998	rBV3	898	627	0.02%	0.003%
67	10.752	3002	3005	3010	rVB3	1175	913	0.03%	0.004%
68	10.791	3013	3017	3021	rBV4	1038	739	0.03%	0.003%
69	10.807	3021	3022	3025	rVB2	1351	606	0.02%	0.003%
70	10.829	3025	3029	3031	rBV3	1146	978	0.04%	0.005%
71	11.013	3078	3086	3090	rBV9	2095	3189	0.12%	0.015%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019743.D
 Acq On : 19 Dec 2020 17:25
 Operator : SY/MD
 Sample : L5151-07
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	11.161	3125	3132	3133	rBV5	3139	3277	0.12%	0.015%
73	11.254	3149	3161	3185	rBV	1352274	2071608	76.02%	9.776%
74	11.466	3223	3227	3229	rBV4	1127	836	0.03%	0.004%
75	11.540	3240	3250	3265	rBV2	27165	57142	2.10%	0.270%
76	11.630	3267	3278	3296	rVB	1248987	1928209	70.75%	9.099%
77	11.788	3324	3327	3330	rBV3	1219	753	0.03%	0.004%
78	12.000	3389	3393	3401	rBV9	1799	2134	0.08%	0.010%
79	12.070	3413	3415	3420	rBV4	954	597	0.02%	0.003%
80	12.244	3463	3469	3470	rBV4	1641	1442	0.05%	0.007%
81	12.353	3496	3503	3512	rBV8	5627	8462	0.31%	0.040%
82	12.582	3570	3574	3576	rVB3	1165	642	0.02%	0.003%
83	12.813	3642	3646	3648	rBV2	1165	808	0.03%	0.004%
84	12.897	3668	3672	3676	rVB4	675	565	0.02%	0.003%
85	12.929	3679	3682	3687	rVB5	902	860	0.03%	0.004%
86	12.958	3687	3691	3695	rBV5	846	845	0.03%	0.004%
87	12.987	3695	3700	3703	rBV3	888	717	0.03%	0.003%
88	13.009	3703	3707	3710	rVB4	1335	939	0.03%	0.004%
89	13.167	3754	3756	3759	rVB3	989	550	0.02%	0.003%
90	13.273	3782	3789	3805	rBV3	6431	12261	0.45%	0.058%
91	13.643	3900	3904	3906	rBV3	652	578	0.02%	0.003%
92	13.752	3929	3938	3948	rBV3	3725	6155	0.23%	0.029%
93	13.958	3999	4002	4004	rBV3	791	546	0.02%	0.003%
94	14.797	4259	4263	4266	rBV4	770	710	0.03%	0.003%
95	14.820	4266	4270	4272	rVV5	691	558	0.02%	0.003%
96	14.836	4272	4275	4277	rVB3	955	600	0.02%	0.003%
97	15.196	4384	4387	4389	rBV3	964	614	0.02%	0.003%
98	15.594	4509	4511	4514	rBV3	905	681	0.02%	0.003%
99	15.659	4526	4531	4533	rBV6	1329	1227	0.05%	0.006%
100	15.967	4625	4627	4630	rVB4	1897	933	0.03%	0.004%


Sum of corrected areas: 21191693

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121920\
Data File : VV019743.D
Acq On : 19 Dec 2020 17:25
Operator : SY/MD
Sample : L5151-07
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0AE9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

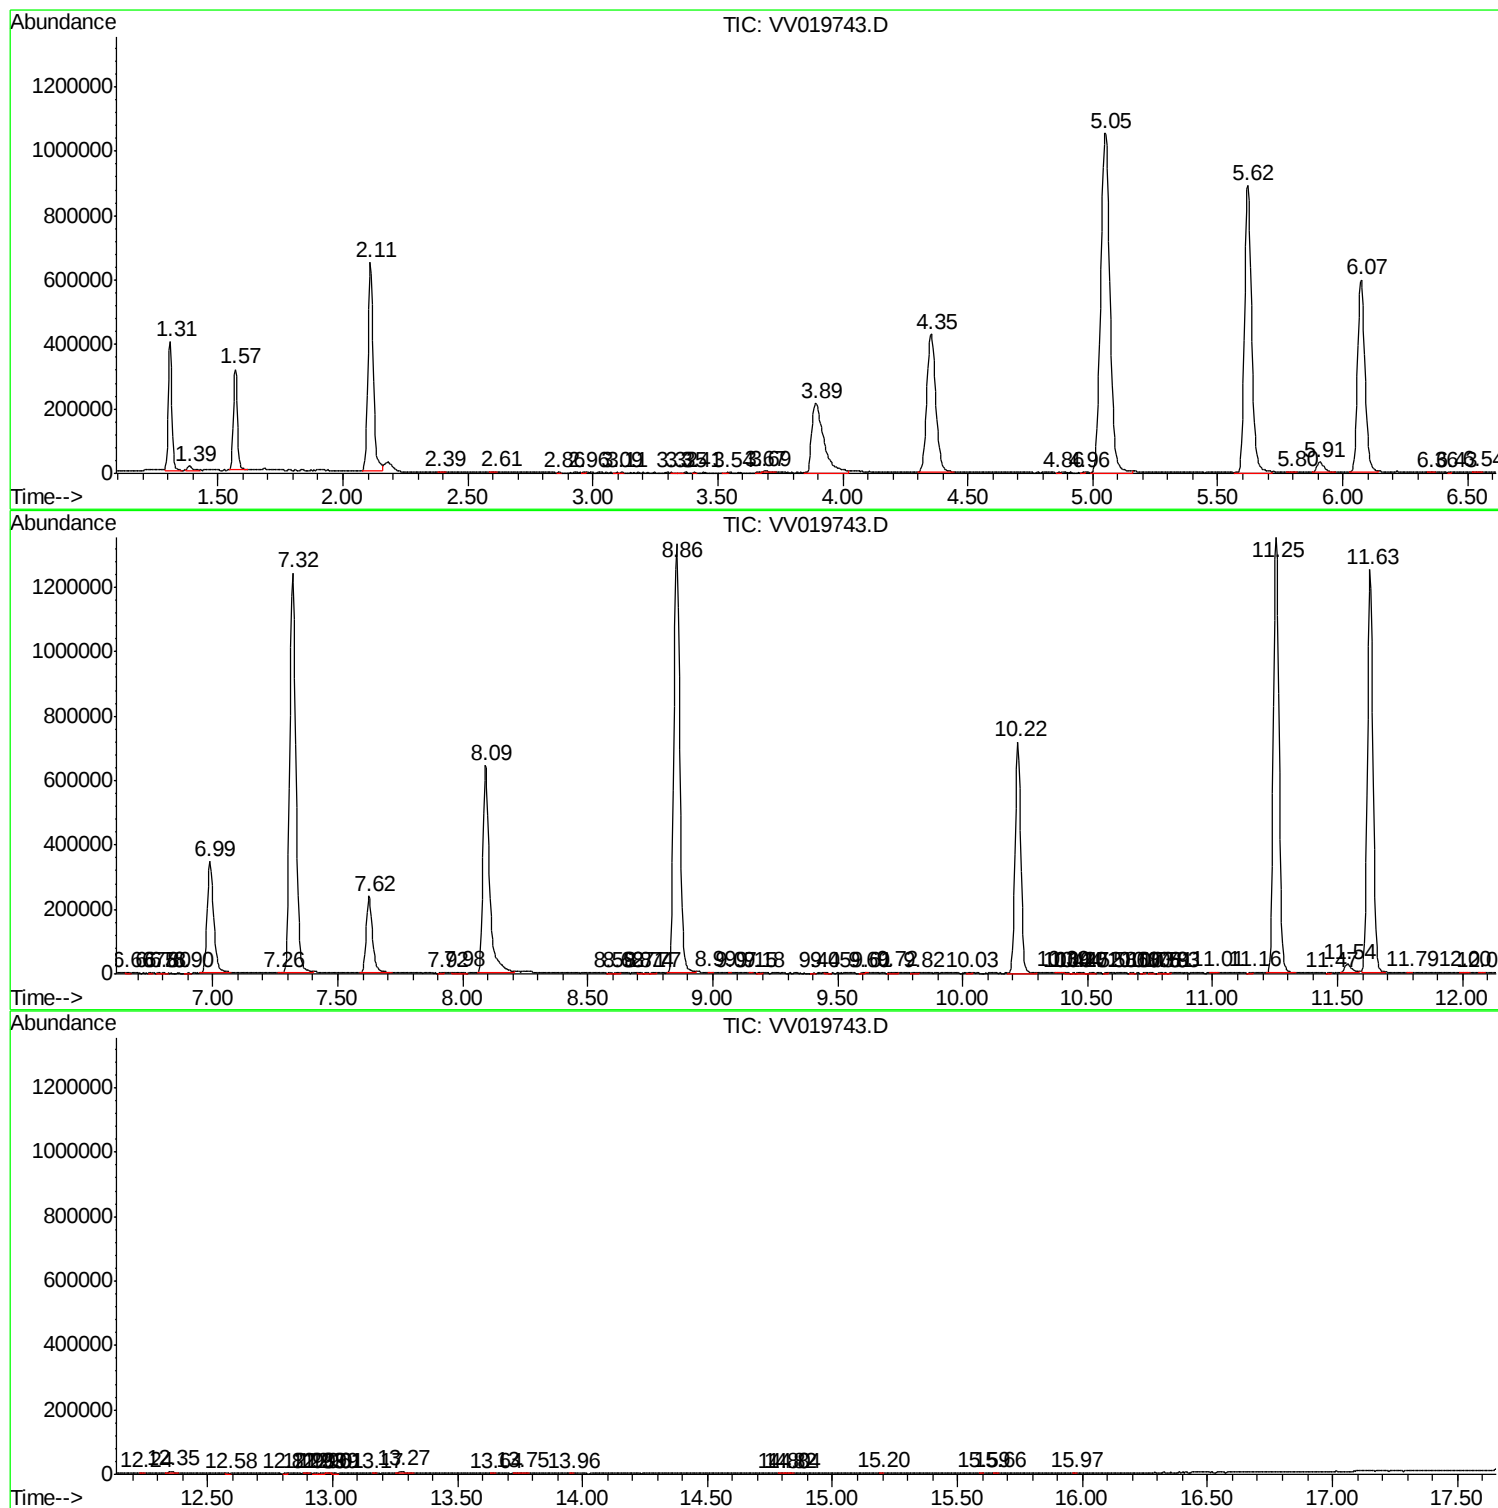

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121920\
Data File : VV019743.D
Acq On : 19 Dec 2020 17:25
Operator : SY/MD
Sample : L5151-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121920\
Data File : VV019743.D
Acq On : 19 Dec 2020 17:25
Operator : SY/MD
Sample : L5151-07
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0AE9

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
