

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019750.D
 Acq On : 19 Dec 2020 21:12
 Operator : SY/MD
 Sample : VV1219WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	80	rVB	393857	379678	13.71%	1.790%
2	1.573	142	150	161	rBV	309017	352183	12.71%	1.660%
3	2.110	308	317	352	rVB	632431	977923	35.30%	4.610%
4	2.753	514	517	520	rBV3	1125	987	0.04%	0.005%
5	2.849	544	547	552	rBV4	728	821	0.03%	0.004%
6	2.958	578	581	582	rBV3	788	345	0.01%	0.002%
7	3.016	596	599	606	rVB6	678	733	0.03%	0.003%
8	3.081	617	619	622	rVB4	796	410	0.01%	0.002%
9	3.103	622	626	627	rBV3	884	542	0.02%	0.003%
10	3.196	652	655	656	rBV	648	313	0.01%	0.001%
11	3.219	660	662	665	rVV3	746	417	0.02%	0.002%
12	3.328	692	696	700	rBV5	1303	1369	0.05%	0.006%
13	3.399	715	718	722	rBV3	702	456	0.02%	0.002%
14	3.544	758	763	765	rBV3	910	969	0.03%	0.005%
15	3.579	772	774	776	rVV	621	408	0.01%	0.002%
16	3.605	779	782	784	rBV3	676	424	0.02%	0.002%
17	3.656	794	798	801	rBV2	498	365	0.01%	0.002%
18	3.695	807	810	814	rVB4	1068	620	0.02%	0.003%
19	3.746	823	826	827	rBV3	694	334	0.01%	0.002%
20	3.791	836	840	842	rBV5	782	696	0.03%	0.003%
21	3.836	850	854	855	rBV4	714	462	0.02%	0.002%
22	3.897	861	873	913	rBV2	181145	583368	21.06%	2.750%
23	4.354	1000	1015	1042	rBV	437094	1056969	38.15%	4.983%
24	4.878	1175	1178	1180	rBV3	761	534	0.02%	0.003%
25	4.933	1192	1195	1199	rVB3	1242	997	0.04%	0.005%
26	4.955	1199	1202	1205	rBV3	974	540	0.02%	0.003%
27	5.052	1214	1232	1274	rBV2	1074906	2770266	100.00%	13.060%
28	5.457	1352	1358	1361	rBV5	1087	924	0.03%	0.004%
29	5.473	1361	1363	1365	rVV	786	346	0.01%	0.002%
30	5.544	1382	1385	1387	rBV3	715	379	0.01%	0.002%
31	5.621	1396	1409	1436	rBV	905537	1808416	65.28%	8.525%
32	5.871	1483	1487	1488	rBV4	992	600	0.02%	0.003%
33	5.910	1489	1499	1517	rVV4	23501	51552	1.86%	0.243%
34	6.074	1536	1550	1575	rBV	617071	1248715	45.08%	5.887%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019750.D
 Acq On : 19 Dec 2020 21:12
 Operator : SY/MD
 Sample : VV1219WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.344	1632	1634	1640	rVB4	698	489	0.02%	0.002%
36	6.370	1640	1642	1645	rBV3	655	426	0.02%	0.002%
37	6.486	1674	1678	1679	rBV4	919	584	0.02%	0.003%
38	6.611	1715	1717	1722	rVB2	747	456	0.02%	0.002%
39	6.640	1722	1726	1727	rBV2	840	500	0.02%	0.002%
40	6.749	1757	1760	1762	rBV3	753	415	0.01%	0.002%
41	6.759	1762	1763	1773	rVB6	1103	1546	0.06%	0.007%
42	6.798	1773	1775	1777	rBV2	567	320	0.01%	0.002%
43	6.817	1777	1781	1783	rBV3	741	625	0.02%	0.003%
44	6.868	1795	1797	1801	rVB3	872	683	0.02%	0.003%
45	6.894	1801	1805	1807	rBV3	517	335	0.01%	0.002%
46	6.933	1815	1817	1820	rVB3	828	416	0.02%	0.002%
47	6.990	1823	1835	1859	rBV	348639	635762	22.95%	2.997%
48	7.318	1925	1937	1964	rBV	1237932	2161526	78.03%	10.190%
49	7.624	2022	2032	2060	rBV	247324	431522	15.58%	2.034%
50	7.978	2136	2142	2149	rBV9	2343	3950	0.14%	0.019%
51	8.093	2167	2178	2216	rBV	668676	1255100	45.31%	5.917%
52	8.649	2349	2351	2354	rVB2	847	447	0.02%	0.002%
53	8.675	2356	2359	2362	rVB4	892	413	0.01%	0.002%
54	8.695	2362	2365	2366	rBV4	646	446	0.02%	0.002%
55	8.762	2384	2386	2390	rBV3	1069	692	0.02%	0.003%
56	8.855	2402	2415	2446	rBV	1381922	2212915	79.88%	10.432%
57	9.251	2535	2538	2541	rBV3	897	581	0.02%	0.003%
58	9.305	2552	2555	2559	rVB2	731	473	0.02%	0.002%
59	9.328	2560	2562	2566	rBV2	906	593	0.02%	0.003%
60	9.543	2625	2629	2630	rBV3	1131	896	0.03%	0.004%
61	9.666	2665	2667	2672	rVB5	735	384	0.01%	0.002%
62	9.736	2685	2689	2694	rVB6	719	635	0.02%	0.003%
63	9.855	2723	2726	2727	rBV2	769	372	0.01%	0.002%
64	9.894	2736	2738	2742	rBV4	596	352	0.01%	0.002%
65	9.932	2747	2750	2751	rBV3	972	586	0.02%	0.003%
66	10.006	2770	2773	2775	rBV3	881	477	0.02%	0.002%
67	10.032	2779	2781	2784	rVB2	638	301	0.01%	0.001%
68	10.071	2791	2793	2796	rVB3	735	378	0.01%	0.002%
69	10.090	2796	2799	2802	rBV2	770	604	0.02%	0.003%
70	10.135	2807	2813	2816	rBV3	891	686	0.02%	0.003%
71	10.222	2826	2840	2858	rBV	758154	1194456	43.12%	5.631%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019750.D
 Acq On : 19 Dec 2020 21:12
 Operator : SY/MD
 Sample : VV1219WBL02
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.376	2886	2888	2890	rBV3	919	448	0.02%	0.002%
73	10.495	2920	2925	2929	rBV5	1159	1029	0.04%	0.005%
74	10.550	2938	2942	2946	rVB4	1472	1335	0.05%	0.006%
75	10.720	2992	2995	2996	rBV2	535	331	0.01%	0.002%
76	10.743	3000	3002	3004	rBV2	645	409	0.01%	0.002%
77	10.794	3013	3018	3021	rBV3	1085	968	0.03%	0.005%
78	10.826	3025	3028	3031	rVV3	950	644	0.02%	0.003%
79	10.887	3043	3047	3049	rVB4	531	348	0.01%	0.002%
80	11.087	3105	3109	3114	rBV5	685	628	0.02%	0.003%
81	11.125	3116	3121	3123	rVV2	647	538	0.02%	0.003%
82	11.167	3131	3134	3135	rBV2	947	473	0.02%	0.002%
83	11.254	3149	3161	3183	rBV	1370133	2087931	75.37%	9.843%
84	11.501	3235	3238	3240	rBV3	916	523	0.02%	0.002%
85	11.550	3250	3253	3255	rVB3	701	377	0.01%	0.002%
86	11.630	3265	3278	3297	rBV	1219227	1928714	69.62%	9.092%
87	11.926	3367	3370	3376	rVB5	751	575	0.02%	0.003%
88	12.093	3418	3422	3425	rBV3	546	400	0.01%	0.002%
89	12.238	3465	3467	3468	rBV	1007	440	0.02%	0.002%
90	12.357	3501	3504	3505	rBV2	627	322	0.01%	0.002%
91	12.617	3583	3585	3590	rBV4	703	498	0.02%	0.002%
92	12.659	3590	3598	3606	rVB10	3453	4752	0.17%	0.022%
93	12.823	3646	3649	3653	rBV3	944	561	0.02%	0.003%
94	13.090	3727	3732	3734	rBV2	793	658	0.02%	0.003%
95	13.273	3781	3789	3799	rVB10	4934	6896	0.25%	0.033%
96	13.354	3812	3814	3816	rBV3	911	604	0.02%	0.003%
97	13.392	3824	3826	3829	rBV3	877	640	0.02%	0.003%
98	13.466	3844	3849	3852	rBV3	1107	1128	0.04%	0.005%
99	13.514	3857	3864	3875	rBV4	4230	7850	0.28%	0.037%
100	13.755	3932	3939	3946	rVB9	4520	6954	0.25%	0.033%


Sum of corrected areas: 21212377

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121920\
Data File : VV019750.D
Acq On : 19 Dec 2020 21:12
Operator : SY/MD
Sample : VV1219WBL02
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK76

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

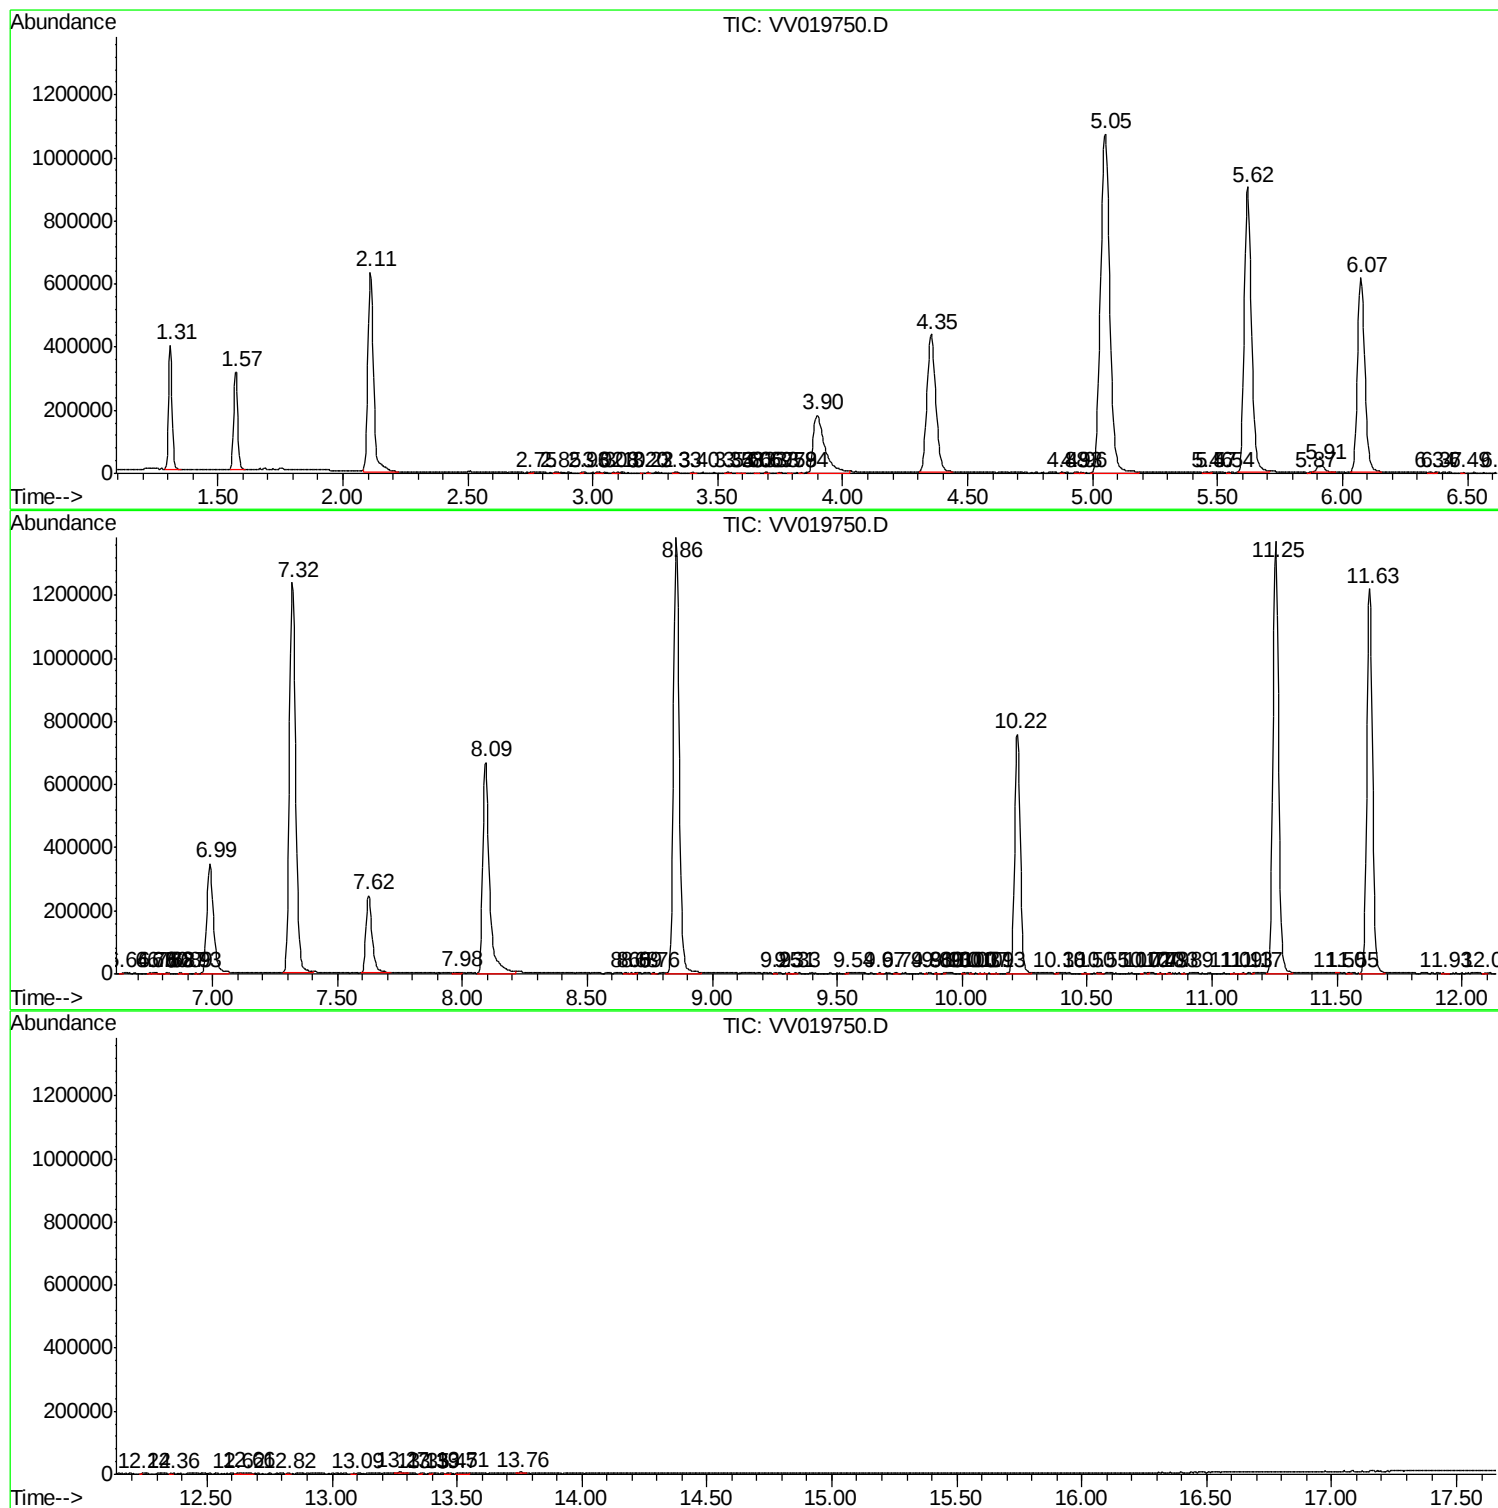

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121920\
Data File : VV019750.D
Acq On : 19 Dec 2020 21:12
Operator : SY/MD
Sample : VV1219WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK76

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV121920\
Data File : VV019750.D
Acq On : 19 Dec 2020 21:12
Operator : SY/MD
Sample : VV1219WBL02
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK76

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc