

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019758.D
 Acq On : 20 Dec 2020 00:48
 Operator : SY/MD
 Sample : L5131-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4H09

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	61	68	81	rVB	377432	379590	8.88%	1.363%
2	1.569	142	149	163	rBV	312381	350947	8.21%	1.261%
3	2.113	308	318	331	rBV	623491	939082	21.98%	3.373%
4	3.116	627	630	631	rBV	725	309	0.01%	0.001%
5	3.190	646	653	654	rBV5	2541	2880	0.07%	0.010%
6	3.309	686	690	694	rBV5	693	676	0.02%	0.002%
7	3.383	710	713	717	rVB3	656	486	0.01%	0.002%
8	3.402	717	719	721	rBV3	546	273	0.01%	0.001%
9	3.418	721	724	726	rVV3	659	350	0.01%	0.001%
10	3.431	726	728	731	rBV3	474	270	0.01%	0.001%
11	3.473	739	741	743	rVB2	1113	434	0.01%	0.002%
12	3.482	743	744	746	rBV	431	189	0.00%	0.001%
13	3.566	768	770	772	rVB2	433	147	0.00%	0.001%
14	3.589	774	777	778	rBV2	465	266	0.01%	0.001%
15	3.621	785	787	791	rBV4	734	410	0.01%	0.001%
16	3.653	795	797	800	rBV3	761	518	0.01%	0.002%
17	3.679	803	805	808	rVB3	475	220	0.01%	0.001%
18	3.753	826	828	832	rVB4	938	452	0.01%	0.002%
19	3.836	851	854	856	rBV4	590	273	0.01%	0.001%
20	3.913	859	878	919	rBV2	1591908	4273240	100.00%	15.349%
21	4.354	999	1015	1042	rBV	425878	1051774	24.61%	3.778%
22	4.852	1168	1170	1171	rBV	478	192	0.00%	0.001%
23	4.862	1171	1173	1175	rVV2	639	324	0.01%	0.001%
24	4.958	1200	1203	1206	rBV4	831	747	0.02%	0.003%
25	4.990	1210	1213	1214	rBV2	622	335	0.01%	0.001%
26	5.052	1214	1232	1276	rBV2	1048130	2730483	63.90%	9.807%
27	5.428	1347	1349	1352	rBV4	826	398	0.01%	0.001%
28	5.621	1395	1409	1441	rBV	858491	1719917	40.25%	6.178%
29	5.916	1486	1501	1534	rBV	1911545	3727975	87.24%	13.390%
30	6.074	1538	1550	1576	rVB	612596	1224649	28.66%	4.399%
31	6.460	1666	1670	1671	rBV3	832	482	0.01%	0.002%
32	6.508	1682	1685	1688	rBV4	1128	788	0.02%	0.003%
33	6.547	1695	1697	1700	rBV4	956	664	0.02%	0.002%
34	6.637	1723	1725	1728	rBV3	828	589	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019758.D
 Acq On : 20 Dec 2020 00:48
 Operator : SY/MD
 Sample : L5131-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4H09

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.698	1743	1744	1747	rBV	405	275	0.01%	0.001%
36	6.730	1751	1754	1758	rBV4	1311	1059	0.02%	0.004%
37	6.756	1760	1762	1765	rBV5	1011	513	0.01%	0.002%
38	6.791	1769	1773	1774	rBV3	418	227	0.01%	0.001%
39	6.804	1774	1777	1778	rBV3	936	433	0.01%	0.002%
40	6.884	1801	1802	1803	rBV2	552	207	0.00%	0.001%
41	6.916	1808	1812	1815	rVB4	659	429	0.01%	0.002%
42	6.936	1815	1818	1819	rBV4	844	462	0.01%	0.002%
43	6.990	1822	1835	1860	rBV	340965	622468	14.57%	2.236%
44	7.318	1925	1937	1957	rBV	1241966	2130420	49.85%	7.652%
45	7.579	2015	2018	2021	rBV3	595	429	0.01%	0.002%
46	7.624	2022	2032	2050	rBV2	235078	409393	9.58%	1.470%
47	7.887	2112	2114	2117	rBV4	598	243	0.01%	0.001%
48	8.090	2167	2177	2211	rBV	610776	1168026	27.33%	4.195%
49	8.723	2371	2374	2375	rBV	904	427	0.01%	0.002%
50	8.855	2403	2415	2444	rBV	1303814	2100421	49.15%	7.544%
51	9.190	2517	2519	2523	rBV2	835	653	0.02%	0.002%
52	9.376	2571	2577	2580	rBV4	1080	923	0.02%	0.003%
53	9.392	2580	2582	2584	rBV	696	395	0.01%	0.001%
54	9.428	2591	2593	2595	rBV3	758	355	0.01%	0.001%
55	9.768	2695	2699	2703	rVB3	815	712	0.02%	0.003%
56	9.936	2746	2751	2755	rBV4	1318	1503	0.04%	0.005%
57	10.003	2770	2772	2773	rVB	488	122	0.00%	0.000%
58	10.026	2775	2779	2782	rBV3	763	736	0.02%	0.003%
59	10.064	2789	2791	2792	rBV3	464	141	0.00%	0.001%
60	10.116	2803	2807	2808	rBV3	733	456	0.01%	0.002%
61	10.135	2810	2813	2815	rVV3	507	271	0.01%	0.001%
62	10.222	2828	2840	2860	rBV	720193	1124296	26.31%	4.038%
63	10.492	2921	2924	2925	rBV3	1040	483	0.01%	0.002%
64	10.659	2974	2976	2977	rBV2	635	244	0.01%	0.001%
65	10.710	2988	2992	2993	rBV4	384	280	0.01%	0.001%
66	10.797	3018	3019	3021	rBV2	449	166	0.00%	0.001%
67	10.836	3028	3031	3032	rBV2	822	459	0.01%	0.002%
68	10.919	3053	3057	3060	rBV2	1029	775	0.02%	0.003%
69	10.958	3065	3069	3070	rBV2	679	391	0.01%	0.001%
70	11.045	3094	3096	3098	rBV3	849	384	0.01%	0.001%
71	11.106	3111	3115	3118	rVB4	886	757	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV121920\
 Data File : VV019758.D
 Acq On : 20 Dec 2020 00:48
 Operator : SY/MD
 Sample : L5131-10
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F4H09

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	11.202	3141	3145	3149	rBV3	716	832	0.02%	0.003%
73	11.254	3149	3161	3193	rVV	1264813	1967901	46.05%	7.068%
74	11.518	3241	3243	3246	rBV2	930	484	0.01%	0.002%
75	11.630	3266	3278	3297	rBV	1214073	1886461	44.15%	6.776%
76	11.852	3346	3347	3349	rBV2	711	297	0.01%	0.001%
77	12.132	3432	3434	3435	rBV	392	97	0.00%	0.000%
78	12.328	3493	3495	3496	rBV2	644	170	0.00%	0.001%
79	12.559	3565	3567	3569	rBV	920	368	0.01%	0.001%
80	12.572	3569	3571	3573	rVV3	683	318	0.01%	0.001%
81	12.608	3580	3582	3584	rBV2	720	405	0.01%	0.001%
82	12.659	3595	3598	3601	rBV3	858	740	0.02%	0.003%
83	12.800	3640	3642	3645	rVB	735	413	0.01%	0.001%
84	12.817	3645	3647	3649	rBV2	775	300	0.01%	0.001%
85	13.231	3771	3776	3780	rBV3	923	1210	0.03%	0.004%
86	13.280	3789	3791	3794	rBV3	1211	838	0.02%	0.003%


Sum of corrected areas: 27841097

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV121920\
Data File : VV019758.D
Acq On : 20 Dec 2020 00:48
Operator : SY/MD
Sample : L5131-10
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4H09

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

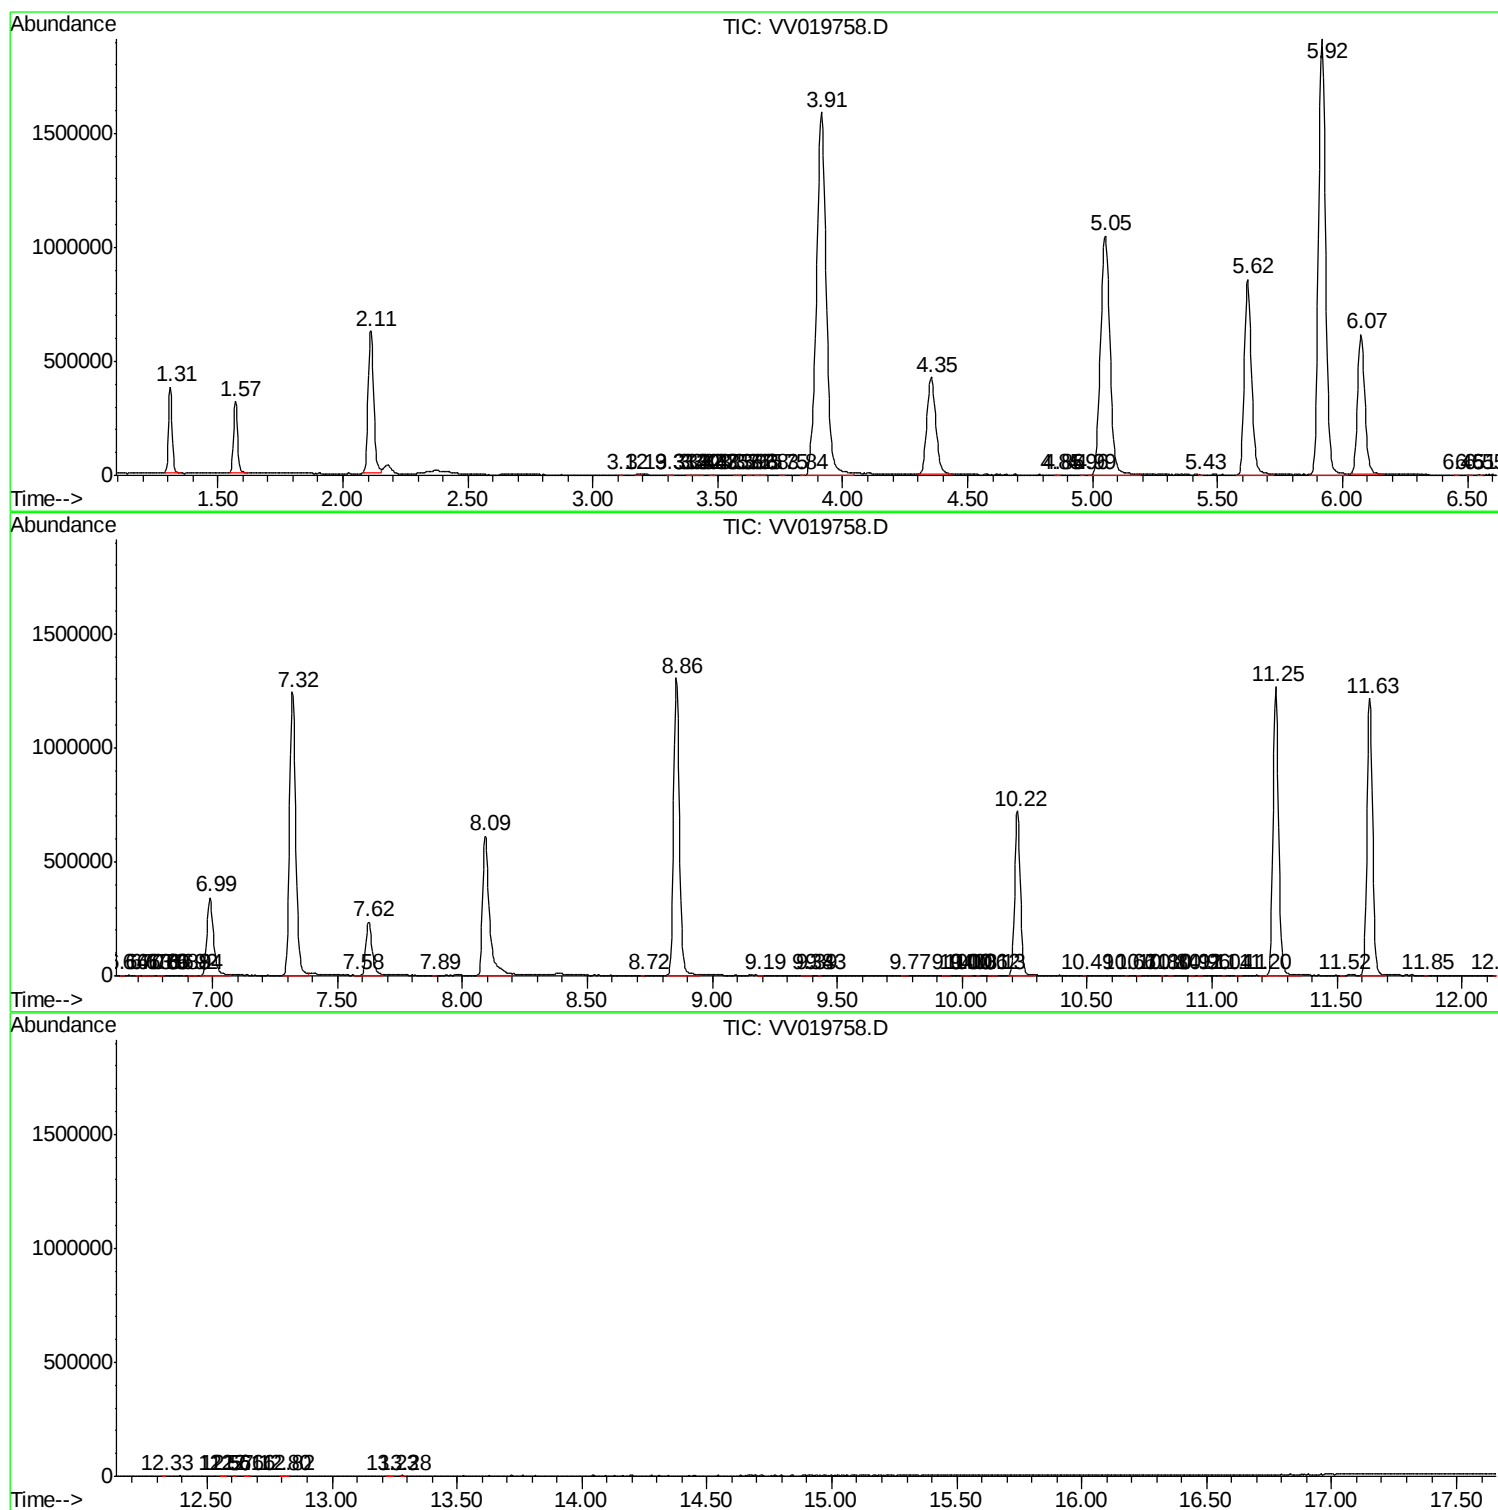

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV121920\
Data File : VV019758.D
Acq On : 20 Dec 2020 00:48
Operator : SY/MD
Sample : L5131-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4H09

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV121920\
Data File : VV019758.D
Acq On : 20 Dec 2020 00:48
Operator : SY/MD
Sample : L5131-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F4H09

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
