


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV121920\
 Data File : VV019724.D
 Acq On : 19 Dec 2020 08:56
 Operator : SY/MD
 Sample : BFB69
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB69

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis
 Last Update : Mon Dec 21 06:23:42 2020

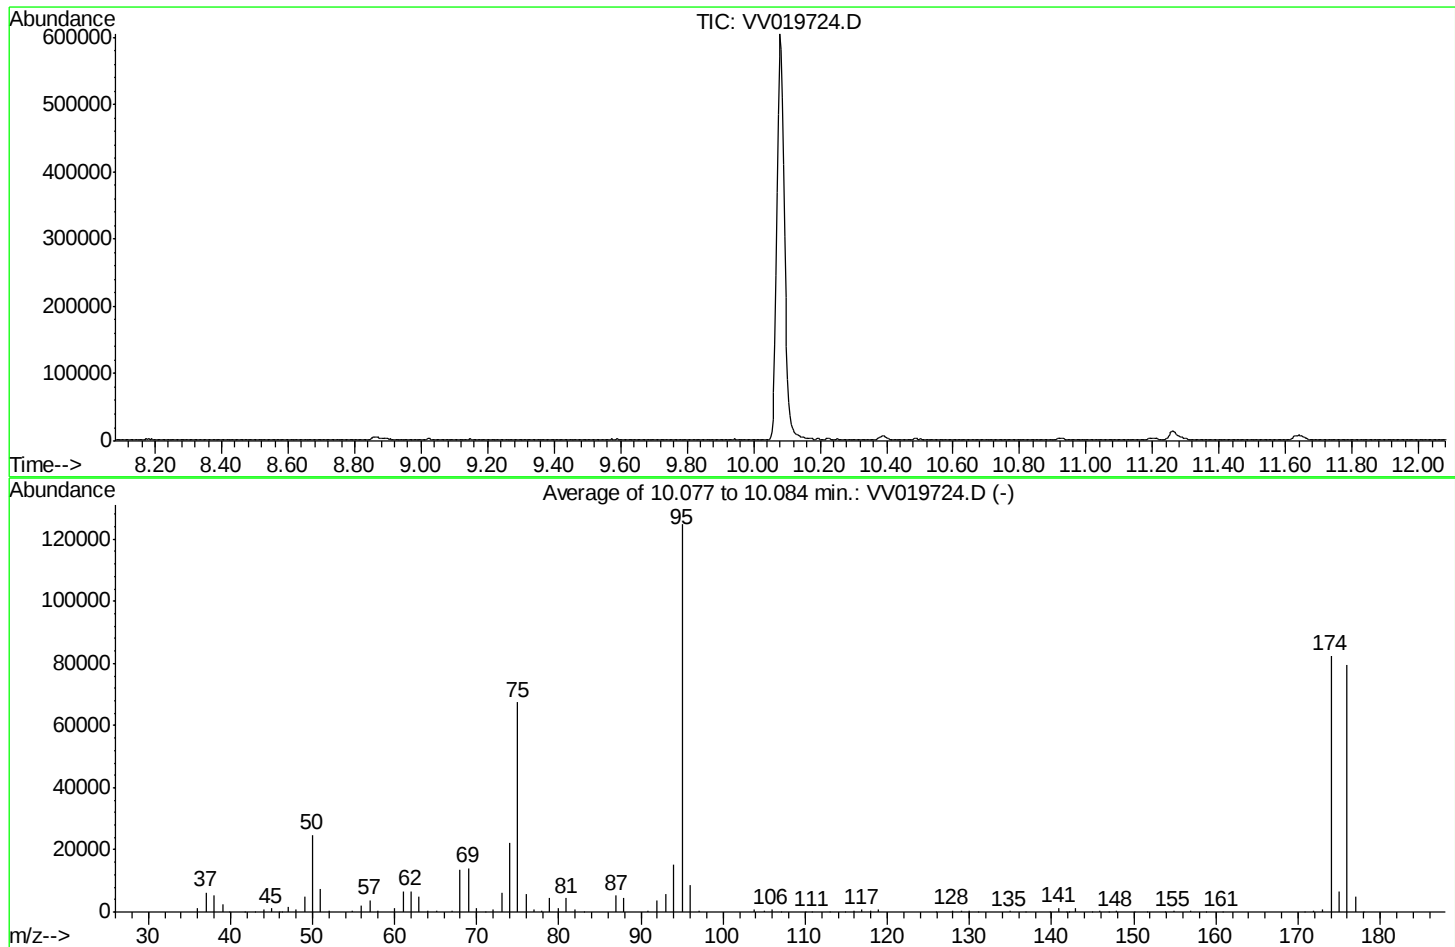

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2784

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	24925	PASS
75	95	30	80	54.0	67402	PASS
95	95	100	100	100.0	124768	PASS
96	95	5	9	6.9	8668	PASS
173	174	0.00	2	1.2	1015	PASS
174	95	50	120	66.0	82397	PASS
175	174	5	9	8.0	6570	PASS
176	174	95	101	96.5	79522	PASS
177	176	5	9	6.4	5063	PASS

m/z	Abundance
36.00	1378.0
37.00	6278.0
38.00	5660.0
39.10	2119.0
39.90	374.0
41.70	141.0
43.10	150.0
44.00	1651.0
45.00	1258.0
46.00	148.0
47.00	1694.0
47.90	773.0
49.00	4976.0
50.00	24824.0
51.00	7612.0
52.00	326.0
54.90	324.0
56.00	1828.0
57.00	3737.0
57.90	259.0
60.00	1167.0
61.00	6472.0
62.00	6473.0
63.00	4645.0
64.00	541.0
65.00	239.0
66.90	335.0
68.00	13358.0
69.00	13679.0
70.00	1104.0
71.90	748.0
73.00	5882.0
74.00	22112.0
75.00	66656.0
76.00	5777.0
76.90	668.0
77.80	469.0
78.90	4481.0
79.90	1157.0
80.90	4296.0
81.90	970.0
83.00	167.0
87.00	5268.0
87.90	4637.0
90.90	567.0
92.00	3784.0
93.00	5144.0
94.00	15157.0
95.00	121368.0
96.00	8912.0
97.10	324.0
103.90	587.0
105.00	278.0
105.90	652.0
107.00	123.0
110.00	127.0
110.80	160.0
112.90	189.0
114.80	152.0
115.90	544.0
116.90	716.0
117.90	403.0
118.90	695.0
125.90	109.0
127.90	469.0
128.90	203.0
129.90	373.0
131.10	185.0
135.00	324.0
136.80	191.0
139.70	132.0
140.90	1205.0
142.10	152.0
142.90	1182.0
144.90	150.0
145.70	268.0
146.90	161.0
147.80	292.0
150.10	161.0
154.90	370.0
157.00	265.0
158.80	144.0
160.70	148.0
170.80	119.0
171.90	281.0
173.10	980.0
174.00	78904.0
175.00	6214.0
176.00	75768.0
177.00	5054.0
178.00	198.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
36.00	1407.0
37.00	6570.0
38.00	5729.0
39.10	2347.0
39.90	356.0
41.70	105.0
42.90	180.0
44.00	1631.0
45.00	1227.0
46.00	128.0
47.00	1773.0
48.00	730.0
49.00	5146.0
50.00	25624.0
51.00	7678.0
52.00	348.0
55.00	446.0
55.90	2045.0
57.00	3992.0
57.90	259.0
60.00	1290.0
61.00	6849.0
62.00	6992.0
63.00	4897.0
64.00	589.0
65.10	251.0
67.00	368.0
68.00	13985.0
69.00	14742.0
70.00	1160.0
71.00	109.0
72.00	740.0
73.00	6388.0
74.00	23032.0
75.00	69512.0
76.00	6004.0
77.00	699.0
77.90	547.0
78.90	4766.0
79.90	1248.0
80.90	4582.0
81.90	1038.0
83.10	178.0
87.00	5430.0
87.90	4924.0
90.80	577.0
92.00	3883.0
93.00	5899.0
94.00	15619.0
95.00	128976.0
96.00	8848.0
97.10	400.0
103.90	651.0
104.90	219.0
105.90	714.0
110.00	129.0
110.80	246.0
112.90	189.0
114.80	133.0
115.90	588.0
116.90	811.0
117.90	442.0
118.90	722.0
127.90	513.0
129.00	245.0
129.90	488.0
131.00	179.0
134.90	260.0
136.80	176.0
139.80	162.0
140.90	1351.0
142.10	164.0
143.00	1232.0
144.90	120.0
145.80	219.0
146.90	190.0
147.80	247.0
150.10	187.0
151.60	108.0
154.90	347.0
157.00	296.0
158.80	136.0
160.80	165.0
170.80	124.0
171.90	274.0
173.10	1036.0
174.00	84928.0
175.00	6826.0
176.00	82248.0
177.00	5225.0
177.90	192.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
36.00	1261.0
37.00	6243.0
38.00	5187.0
39.10	2383.0
39.90	353.0
43.00	215.0
44.00	1559.0
45.00	1092.0
46.20	127.0
47.00	1619.0
48.00	765.0
49.00	4969.0
50.00	24328.0
51.00	7235.0
52.00	356.0
55.00	532.0
55.90	2050.0
57.00	3712.0
57.90	247.0
60.00	1261.0
61.00	6423.0
62.00	6574.0
63.00	4749.0
64.00	560.0
65.10	280.0
67.00	358.0
68.00	13459.0
69.00	13936.0
70.00	1136.0
72.00	699.0
73.00	6152.0
74.00	21664.0
75.00	66040.0
76.00	5680.0
77.00	732.0
77.90	553.0
78.90	4448.0
79.90	1237.0
80.90	4531.0
81.90	1038.0
83.10	164.0
87.00	5189.0
87.90	4638.0
90.90	577.0
91.90	3525.0
93.00	5875.0
94.00	14678.0
95.00	123960.0
96.00	8246.0
97.10	373.0
103.80	693.0
104.90	164.0
105.90	696.0
110.80	250.0
112.90	193.0
114.90	107.0
116.00	585.0
116.90	835.0
117.90	466.0
118.90	688.0
127.90	526.0
128.90	246.0
129.90	545.0
130.90	189.0
134.80	229.0
136.80	165.0
139.80	156.0
140.90	1362.0
141.80	170.0
143.00	1127.0
144.80	120.0
145.90	215.0
146.90	161.0
147.90	252.0
150.00	173.0
151.70	126.0
153.80	110.0
154.90	255.0
157.00	240.0
158.90	129.0
160.80	158.0
172.00	279.0
173.00	1030.0
174.00	83360.0
175.00	6672.0
176.00	80552.0
177.00	4910.0
177.90	149.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

Scan 2784 (10.042 min): VV019724.D
BFB69

m/z	Abundance
38.20	116.0
39.90	270.0
44.00	785.0
54.90	110.0
79.80	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69