

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122120\
 Data File : VV019784.D
 Acq On : 21 Dec 2020 18:41
 Operator : SY/MD
 Sample : VIBLK72
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Dec 22 00:27:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 22 00:24:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.62	114	697134	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.86	117	651223	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.26	152	296714	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	179809	35.97	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	71.94%
7) Chloroethane-d5	1.57	69	160603	40.73	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	81.46%
11) 1,1-Dichloroethene-d2	2.11	63	281063	30.29	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.58%
21) 2-Butanone-d5	3.89	46	337120	124.07	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	124.07%
24) Chloroform-d	4.35	84	390086	43.30	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.60%
26) 1,2-Dichloroethane-d4	5.04	65	274986	46.70	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.40%
32) Benzene-d6	5.05	84	759648	43.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.48%
36) 1,2-Dichloropropane-d6	6.07	67	256331	47.11	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.22%
41) Toluene-d8	7.32	98	664276	42.48	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	84.96%
43) trans-1,3-Dichloropropene-	7.63	79	117633	38.01	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.02%
47) 2-Hexanone-d5	8.09	63	205652	96.31	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	96.31%
57) 1,1,2,2-Tetrachloroethane-	10.22	84	324012	44.03	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.06%
64) 1,2-Dichlorobenzene-d4	11.63	152	248052	44.72	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.44%


Target Compounds					Ovalue
59) 1,2,3-Trichloropropane	11.25	75	42157	6.819 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV122120\
Data File : VV019784.D
Acq On : 21 Dec 2020 18:41
Operator : SY/MD
Sample : VIBLK72
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Dec 22 00:27:03 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 22 00:24:34 2020
Response via : Initial Calibration

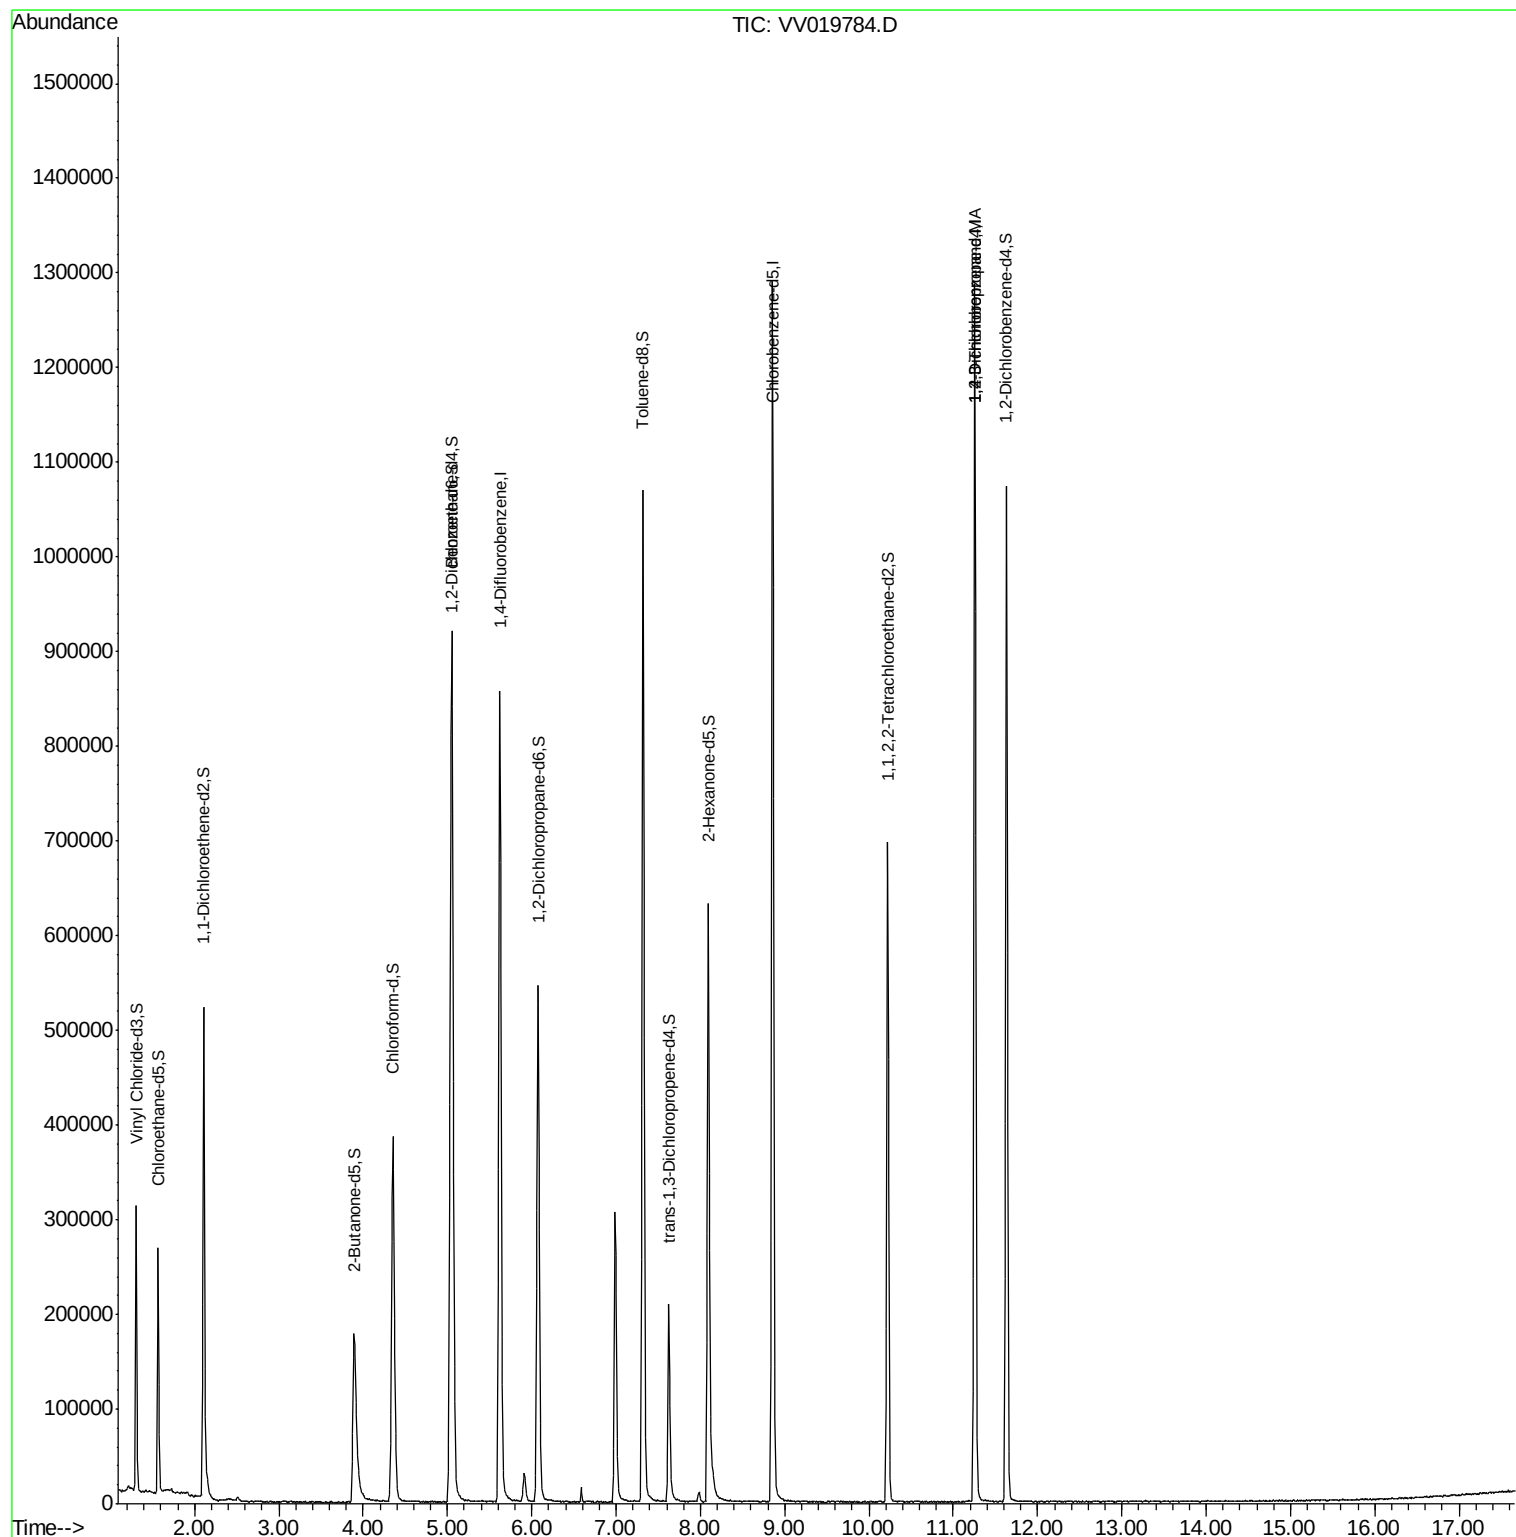

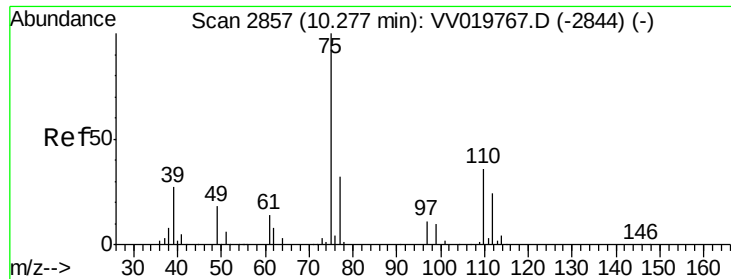

#59

1,2,3-Trichloropropane

Concen: 6.819 ug/L

RT: 11.25 min Scan# 3161

Delta R.T. 0.98 min

Lab File: VV019784.D

Acq: 21 Dec 2020 18:41

Instrument :

MSVOA_V

ClientSampleId :

Tot Ion: 75 Resp: 42157

Ion Ratio Lower Upper

75 100

77 37.6 25.8 38.8

