

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
 Data File : VV019773.D
 Acq On : 21 Dec 2020 13:07
 Operator : SY/MD
 Sample : L5098-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.306	61	67	79	rVB	325294	333286	13.26%	1.691%
2	1.569	142	149	164	rVB	274693	306236	12.18%	1.554%
3	2.110	308	317	346	rVB	567794	872303	34.70%	4.426%
4	2.775	522	524	529	rVB4	1010	606	0.02%	0.003%
5	2.894	560	561	562	rBV	463	167	0.01%	0.001%
6	2.971	584	585	588	rVB2	844	364	0.01%	0.002%
7	2.991	588	591	592	rBV	781	416	0.02%	0.002%
8	3.023	600	601	606	rVB4	745	441	0.02%	0.002%
9	3.251	671	672	673	rBV	614	219	0.01%	0.001%
10	3.335	696	698	706	rVB4	1183	1347	0.05%	0.007%
11	3.367	706	708	710	rBV2	646	349	0.01%	0.002%
12	3.386	713	714	716	rVV	381	162	0.01%	0.001%
13	3.405	719	720	723	rBV3	550	311	0.01%	0.002%
14	3.460	735	737	738	rBV2	356	107	0.00%	0.001%
15	3.483	741	744	748	rBV4	597	477	0.02%	0.002%
16	3.592	776	778	780	rBV	571	240	0.01%	0.001%
17	3.621	785	787	789	rVB2	761	270	0.01%	0.001%
18	3.640	789	793	795	rBV3	826	742	0.03%	0.004%
19	3.753	826	828	833	rVB4	1103	827	0.03%	0.004%
20	3.782	833	837	842	rVV2	629	705	0.03%	0.004%
21	3.807	842	845	847	rVB2	1013	605	0.02%	0.003%
22	3.823	847	850	853	rVB2	802	450	0.02%	0.002%
23	3.888	859	870	910	rBV	189749	551458	21.93%	2.798%
24	4.354	999	1015	1041	rBV	400713	985407	39.19%	5.000%
25	4.904	1183	1186	1187	rBV3	934	489	0.02%	0.002%
26	4.984	1209	1211	1213	rVB3	871	298	0.01%	0.002%
27	5.052	1213	1232	1267	rBV2	965274	2514125	100.00%	12.757%
28	5.466	1360	1361	1365	rBV3	935	653	0.03%	0.003%
29	5.540	1381	1384	1388	rBV4	1361	1052	0.04%	0.005%
30	5.621	1396	1409	1432	rBV	876394	1735271	69.02%	8.805%
31	5.910	1489	1499	1516	rBV4	25628	53825	2.14%	0.273%
32	6.074	1536	1550	1573	rBV	564067	1151076	45.78%	5.841%
33	6.309	1620	1623	1627	rBV5	1176	804	0.03%	0.004%
34	6.502	1679	1683	1685	rBV3	1111	813	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
 Data File : VV019773.D
 Acq On : 21 Dec 2020 13:07
 Operator : SY/MD
 Sample : L5098-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.579	1704	1707	1710	rBV3	919	572	0.02%	0.003%
36	6.704	1743	1746	1748	rBV4	674	462	0.02%	0.002%
37	6.794	1772	1774	1780	rVB4	655	590	0.02%	0.003%
38	6.926	1810	1815	1819	rVB5	992	750	0.03%	0.004%
39	6.990	1822	1835	1864	rBV	327709	599020	23.83%	3.040%
40	7.318	1925	1937	1961	rBV	1139193	1965839	78.19%	9.975%
41	7.624	2022	2032	2057	rBV	226932	399419	15.89%	2.027%
42	7.929	2124	2127	2129	rBV4	972	701	0.03%	0.004%
43	8.093	2167	2178	2213	rBV	641904	1193603	47.48%	6.057%
44	8.791	2393	2395	2396	rBV2	499	193	0.01%	0.001%
45	8.855	2404	2415	2438	rBV	1293766	2105159	83.73%	10.682%
46	9.244	2534	2536	2540	rBV3	822	432	0.02%	0.002%
47	9.344	2564	2567	2569	rBV2	750	390	0.02%	0.002%
48	9.492	2611	2613	2616	rBV3	715	443	0.02%	0.002%
49	9.630	2653	2656	2660	rVB4	1175	834	0.03%	0.004%
50	9.656	2660	2664	2666	rBV2	562	552	0.02%	0.003%
51	9.669	2666	2668	2672	rVV3	561	378	0.02%	0.002%
52	9.743	2686	2691	2696	rBV5	889	1091	0.04%	0.006%
53	9.762	2696	2697	2698	rBV	443	95	0.00%	0.000%
54	9.830	2716	2718	2719	rBV	757	319	0.01%	0.002%
55	9.913	2742	2744	2745	rBV	519	196	0.01%	0.001%
56	10.071	2791	2793	2797	rBV3	672	484	0.02%	0.002%
57	10.141	2811	2815	2821	rVB7	874	1030	0.04%	0.005%
58	10.222	2828	2840	2861	rBV	718454	1119511	44.53%	5.681%
59	10.460	2910	2914	2916	rBV5	951	777	0.03%	0.004%
60	10.495	2924	2925	2931	rVB3	974	719	0.03%	0.004%
61	10.527	2931	2935	2938	rBV4	855	548	0.02%	0.003%
62	10.704	2986	2990	2992	rBV3	1068	817	0.03%	0.004%
63	10.743	2999	3002	3004	rBV4	868	463	0.02%	0.002%
64	10.781	3012	3014	3019	rBV4	663	675	0.03%	0.003%
65	10.887	3045	3047	3049	rBV3	563	305	0.01%	0.002%
66	10.900	3049	3051	3053	rVV	884	356	0.01%	0.002%
67	10.965	3068	3071	3074	rBV2	575	430	0.02%	0.002%
68	11.010	3083	3085	3088	rBV2	969	533	0.02%	0.003%
69	11.093	3109	3111	3114	rVB2	1080	506	0.02%	0.003%
70	11.116	3115	3118	3121	rBV4	629	494	0.02%	0.003%
71	11.254	3149	3161	3182	rBV	1308279	2011744	80.02%	10.208%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
Data File : VV019773.D
Acq On : 21 Dec 2020 13:07
Operator : SY/MD
Sample : L5098-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Title : VOC Analysis

72	11.630	3266	3278	3294	rBV	1142551	1777503	70.70%	9.019%
73	11.968	3382	3383	3384	rBV	755	266	0.01%	0.001%
74	12.042	3403	3406	3408	rBV3	671	491	0.02%	0.002%
75	12.302	3485	3487	3489	rBV	883	549	0.02%	0.003%
76	12.350	3497	3502	3505	rBV6	1169	1315	0.05%	0.007%
77	12.527	3554	3557	3558	rBV3	733	379	0.02%	0.002%
78	12.592	3574	3577	3578	rBV2	620	409	0.02%	0.002%
79	13.450	3841	3844	3845	rBV2	883	504	0.02%	0.003%


Sum of corrected areas: 19707747

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
Data File : VV019773.D
Acq On : 21 Dec 2020 13:07
Operator : SY/MD
Sample : L5098-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

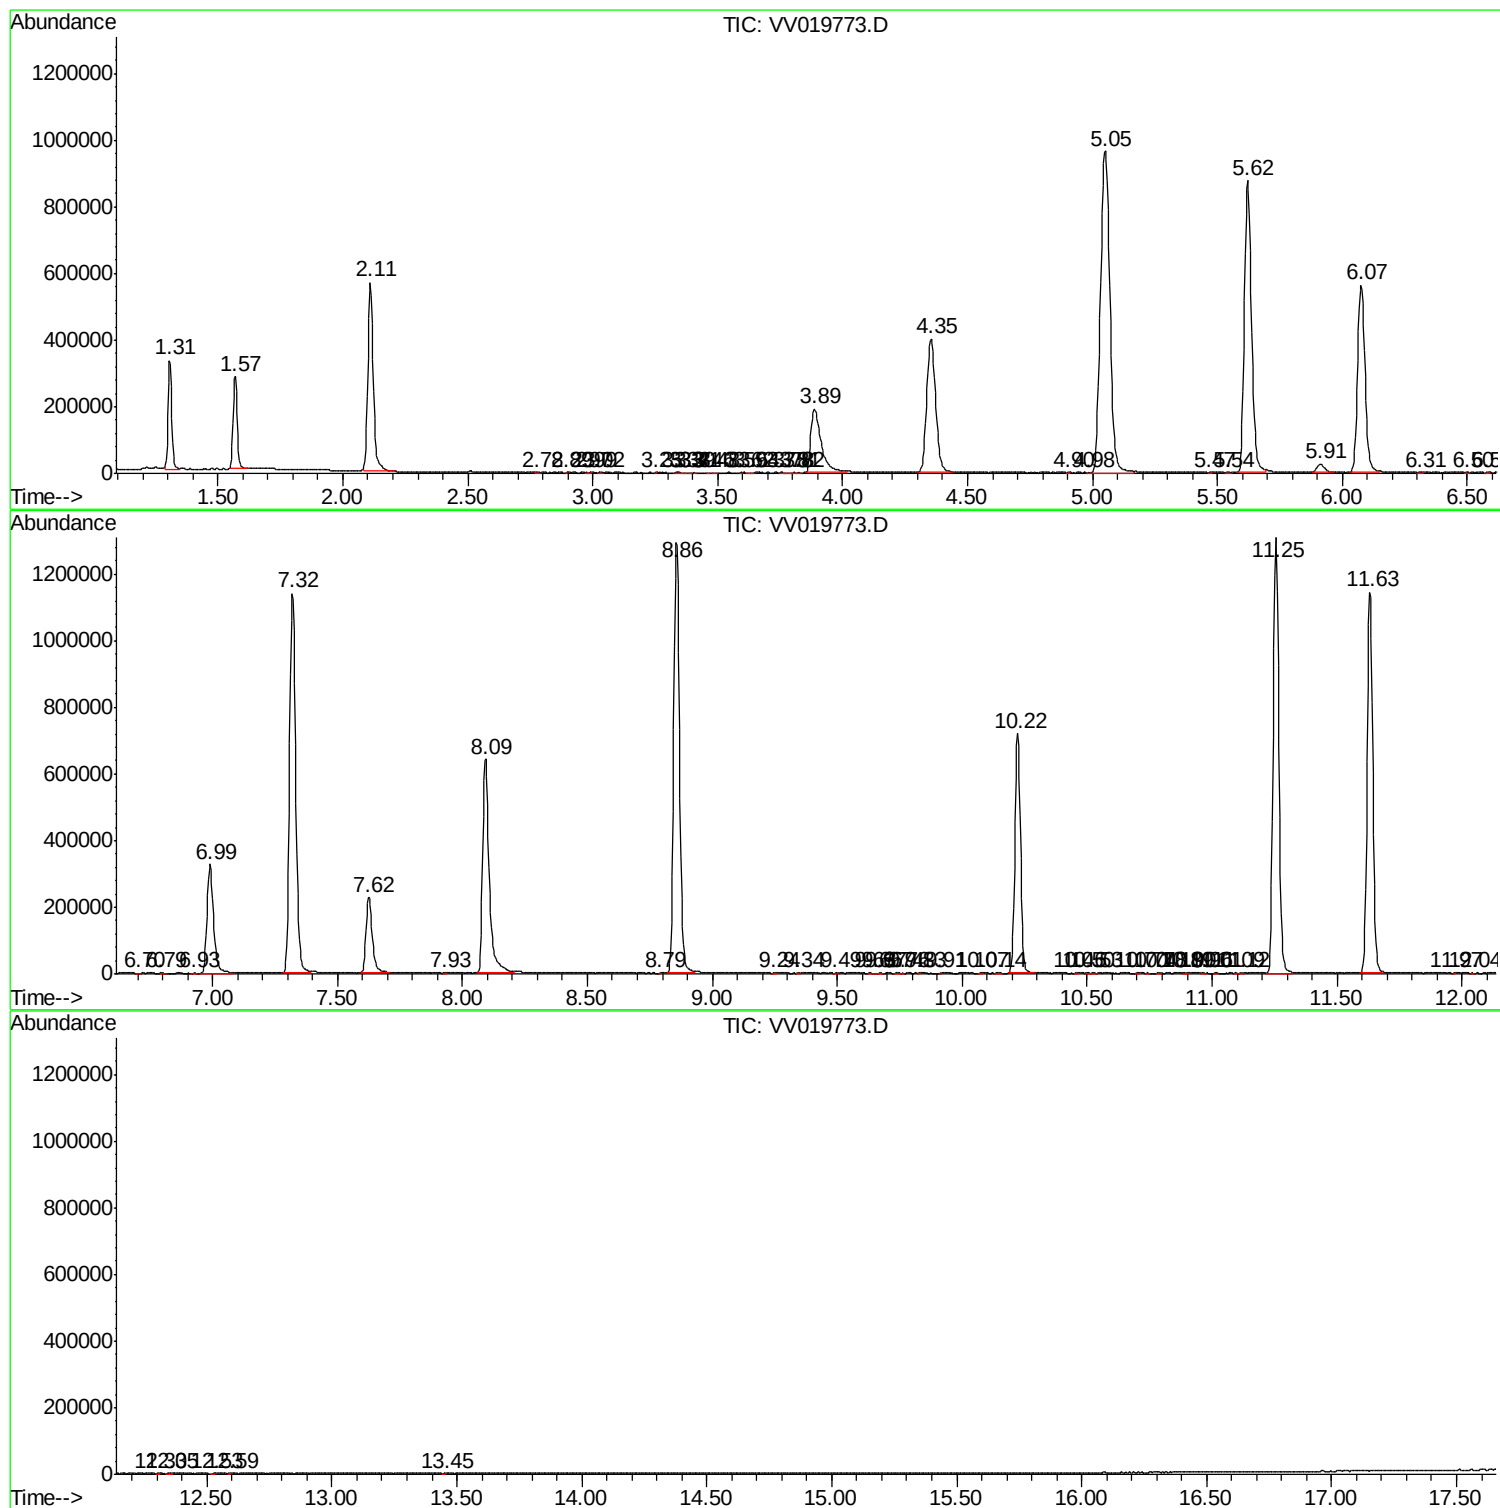

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
Data File : VV019773.D
Acq On : 21 Dec 2020 13:07
Operator : SY/MD
Sample : L5098-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV122120\
Data File : VV019773.D
Acq On : 21 Dec 2020 13:07
Operator : SY/MD
Sample : L5098-03
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc