

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
 Data File : VV019774.D
 Acq On : 21 Dec 2020 14:40
 Operator : SY/MD
 Sample : L5101-01DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FW6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	79	rVB	351800	343186	8.82%	1.379%
2	1.570	142	149	162	rVB	289255	324135	8.33%	1.302%
3	2.110	307	317	355	rVB	590547	930773	23.92%	3.740%
4	2.881	554	557	560	rBV3	901	537	0.01%	0.002%
5	2.946	575	577	579	rBV3	527	218	0.01%	0.001%
6	3.039	604	606	608	rBV2	325	121	0.00%	0.000%
7	3.081	617	619	620	rBV	535	279	0.01%	0.001%
8	3.164	643	645	646	rBV2	739	323	0.01%	0.001%
9	3.193	652	654	658	rVB3	694	332	0.01%	0.001%
10	3.219	658	662	668	rVB6	922	1103	0.03%	0.004%
11	3.248	668	671	673	rBV3	820	468	0.01%	0.002%
12	3.309	685	690	694	rBV6	1041	1126	0.03%	0.005%
13	3.405	715	720	722	rBV4	839	895	0.02%	0.004%
14	3.518	753	755	758	rBV2	315	147	0.00%	0.001%
15	3.589	774	777	779	rBV2	807	494	0.01%	0.002%
16	3.611	782	784	786	rBV2	456	235	0.01%	0.001%
17	3.647	792	795	798	rBV3	831	528	0.01%	0.002%
18	3.666	798	801	804	rBV3	652	518	0.01%	0.002%
19	3.724	816	819	823	rVB2	831	615	0.02%	0.002%
20	3.743	823	825	826	rBV2	673	223	0.01%	0.001%
21	3.778	834	836	838	rBV3	1041	464	0.01%	0.002%
22	3.830	850	852	854	rBV2	306	112	0.00%	0.000%
23	3.891	860	871	907	rBV	187143	624222	16.04%	2.508%
24	4.351	997	1014	1043	rBV	417287	1031452	26.50%	4.144%
25	4.746	1134	1137	1140	rBV5	847	493	0.01%	0.002%
26	4.817	1157	1159	1161	rBV3	663	299	0.01%	0.001%
27	4.862	1170	1173	1174	rBV2	524	283	0.01%	0.001%
28	4.888	1180	1181	1183	rBV	488	231	0.01%	0.001%
29	4.975	1206	1208	1211	rVB3	705	344	0.01%	0.001%
30	5.048	1211	1231	1268	rBV2	1014660	2639657	67.83%	10.606%
31	5.335	1317	1320	1322	rBV3	1272	703	0.02%	0.003%
32	5.466	1358	1361	1363	rBV3	930	678	0.02%	0.003%
33	5.618	1395	1408	1441	rBV	960692	1914348	49.19%	7.691%
34	6.071	1534	1549	1581	rBV	592494	1205223	30.97%	4.842%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
 Data File : VV019774.D
 Acq On : 21 Dec 2020 14:40
 Operator : SY/MD
 Sample : L5101-01DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleID :
 C0FW6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.470	1669	1673	1677	rBV4	828	899	0.02%	0.004%
36	6.534	1691	1693	1698	rBV5	959	816	0.02%	0.003%
37	6.560	1698	1701	1704	rBV5	892	550	0.01%	0.002%
38	6.576	1704	1706	1707	rBV2	522	184	0.00%	0.001%
39	6.634	1720	1724	1728	rBV6	1217	1416	0.04%	0.006%
40	6.727	1752	1753	1755	rBV6	499	186	0.00%	0.001%
41	6.814	1778	1780	1782	rVB2	779	317	0.01%	0.001%
42	6.833	1782	1786	1787	rBV3	371	258	0.01%	0.001%
43	6.913	1807	1811	1813	rBV3	545	395	0.01%	0.002%
44	6.987	1821	1834	1864	rBV	342559	624186	16.04%	2.508%
45	7.319	1924	1937	1963	rBV	1197014	2065905	53.09%	8.300%
46	7.624	2022	2032	2051	rBV	239502	412698	10.60%	1.658%
47	7.981	2140	2143	2150	rVB9	2035	2032	0.05%	0.008%
48	8.026	2155	2157	2158	rBV	453	137	0.00%	0.001%
49	8.090	2167	2177	2212	rBV	641052	1189033	30.55%	4.777%
50	8.547	2317	2319	2320	rBV	747	277	0.01%	0.001%
51	8.675	2357	2359	2363	rBV3	913	698	0.02%	0.003%
52	8.698	2364	2366	2368	rVB2	706	260	0.01%	0.001%
53	8.743	2377	2380	2382	rBV3	1285	641	0.02%	0.003%
54	8.855	2403	2415	2441	rBV	1469467	2650520	68.11%	10.649%
55	9.225	2524	2530	2531	rBV3	1243	971	0.02%	0.004%
56	9.293	2549	2551	2553	rBV3	985	349	0.01%	0.001%
57	9.331	2561	2563	2566	rBV2	728	458	0.01%	0.002%
58	9.396	2581	2583	2584	rBV	481	219	0.01%	0.001%
59	9.457	2601	2602	2607	rVB4	773	381	0.01%	0.002%
60	9.479	2607	2609	2611	rBV2	624	346	0.01%	0.001%
61	9.543	2626	2629	2630	rBV2	614	296	0.01%	0.001%
62	9.598	2644	2646	2648	rBV4	874	367	0.01%	0.001%
63	9.634	2654	2657	2659	rBV3	930	626	0.02%	0.003%
64	9.849	2720	2724	2726	rBV3	610	475	0.01%	0.002%
65	9.900	2737	2740	2743	rBV3	939	670	0.02%	0.003%
66	9.933	2747	2750	2754	rBV3	1061	669	0.02%	0.003%
67	9.952	2754	2756	2761	rVB4	793	621	0.02%	0.002%
68	9.981	2761	2765	2767	rBV3	484	357	0.01%	0.001%
69	10.010	2769	2774	2775	rBV2	917	557	0.01%	0.002%
70	10.048	2781	2786	2787	rBV3	873	707	0.02%	0.003%
71	10.119	2806	2808	2809	rBV	310	160	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
 Data File : VV019774.D
 Acq On : 21 Dec 2020 14:40
 Operator : SY/MD
 Sample : L5101-01DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FW6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.125	2809	2810	2812	rVB2	702	222	0.01%	0.001%
73	10.138	2812	2814	2816	rBV	530	320	0.01%	0.001%
74	10.167	2821	2823	2825	rVB3	373	120	0.00%	0.000%
75	10.222	2825	2840	2865	rBV	730105	1153913	29.65%	4.636%
76	10.511	2926	2930	2933	rBV3	611	557	0.01%	0.002%
77	10.543	2938	2940	2942	rVB2	1123	395	0.01%	0.002%
78	10.788	3013	3016	3018	rBV3	434	254	0.01%	0.001%
79	10.804	3018	3021	3025	rVV4	828	614	0.02%	0.002%
80	10.849	3032	3035	3037	rBV3	867	530	0.01%	0.002%
81	10.920	3055	3057	3059	rBV2	814	418	0.01%	0.002%
82	10.978	3073	3075	3076	rBV	594	223	0.01%	0.001%
83	11.071	3102	3104	3107	rVB2	606	229	0.01%	0.001%
84	11.190	3131	3141	3150	rBV2	44422	72577	1.86%	0.292%
85	11.254	3150	3161	3187	rVB2	1544481	2721067	69.92%	10.933%
86	11.643	3266	3282	3310	rBV2	1657982	3891602	100.00%	15.636%
87	11.852	3341	3347	3353	rBV6	1442	1988	0.05%	0.008%
88	12.087	3417	3420	3421	rBV2	727	391	0.01%	0.002%
89	12.164	3442	3444	3447	rBV2	570	368	0.01%	0.001%
90	12.177	3447	3448	3449	rBV2	648	174	0.00%	0.001%
91	12.231	3463	3465	3468	rBV4	969	417	0.01%	0.002%
92	12.463	3535	3537	3539	rBV2	723	332	0.01%	0.001%
93	12.585	3570	3575	3578	rBV5	986	1039	0.03%	0.004%
94	12.649	3588	3595	3604	rBV2	16182	25629	0.66%	0.103%
95	12.823	3647	3649	3650	rBV2	678	289	0.01%	0.001%
96	12.913	3674	3677	3681	rBV3	906	752	0.02%	0.003%
97	13.270	3777	3788	3807	rBV	389816	594504	15.28%	2.389%
98	13.752	3927	3938	3956	rBV	242351	383429	9.85%	1.541%
99	14.588	4193	4198	4200	rBV4	1291	1250	0.03%	0.005%
100	15.408	4446	4453	4465	rVB5	33070	51148	1.31%	0.206%


Sum of corrected areas: 24889153

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
Data File : VV019774.D
Acq On : 21 Dec 2020 14:40
Operator : SY/MD
Sample : L5101-01DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
C0FW6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

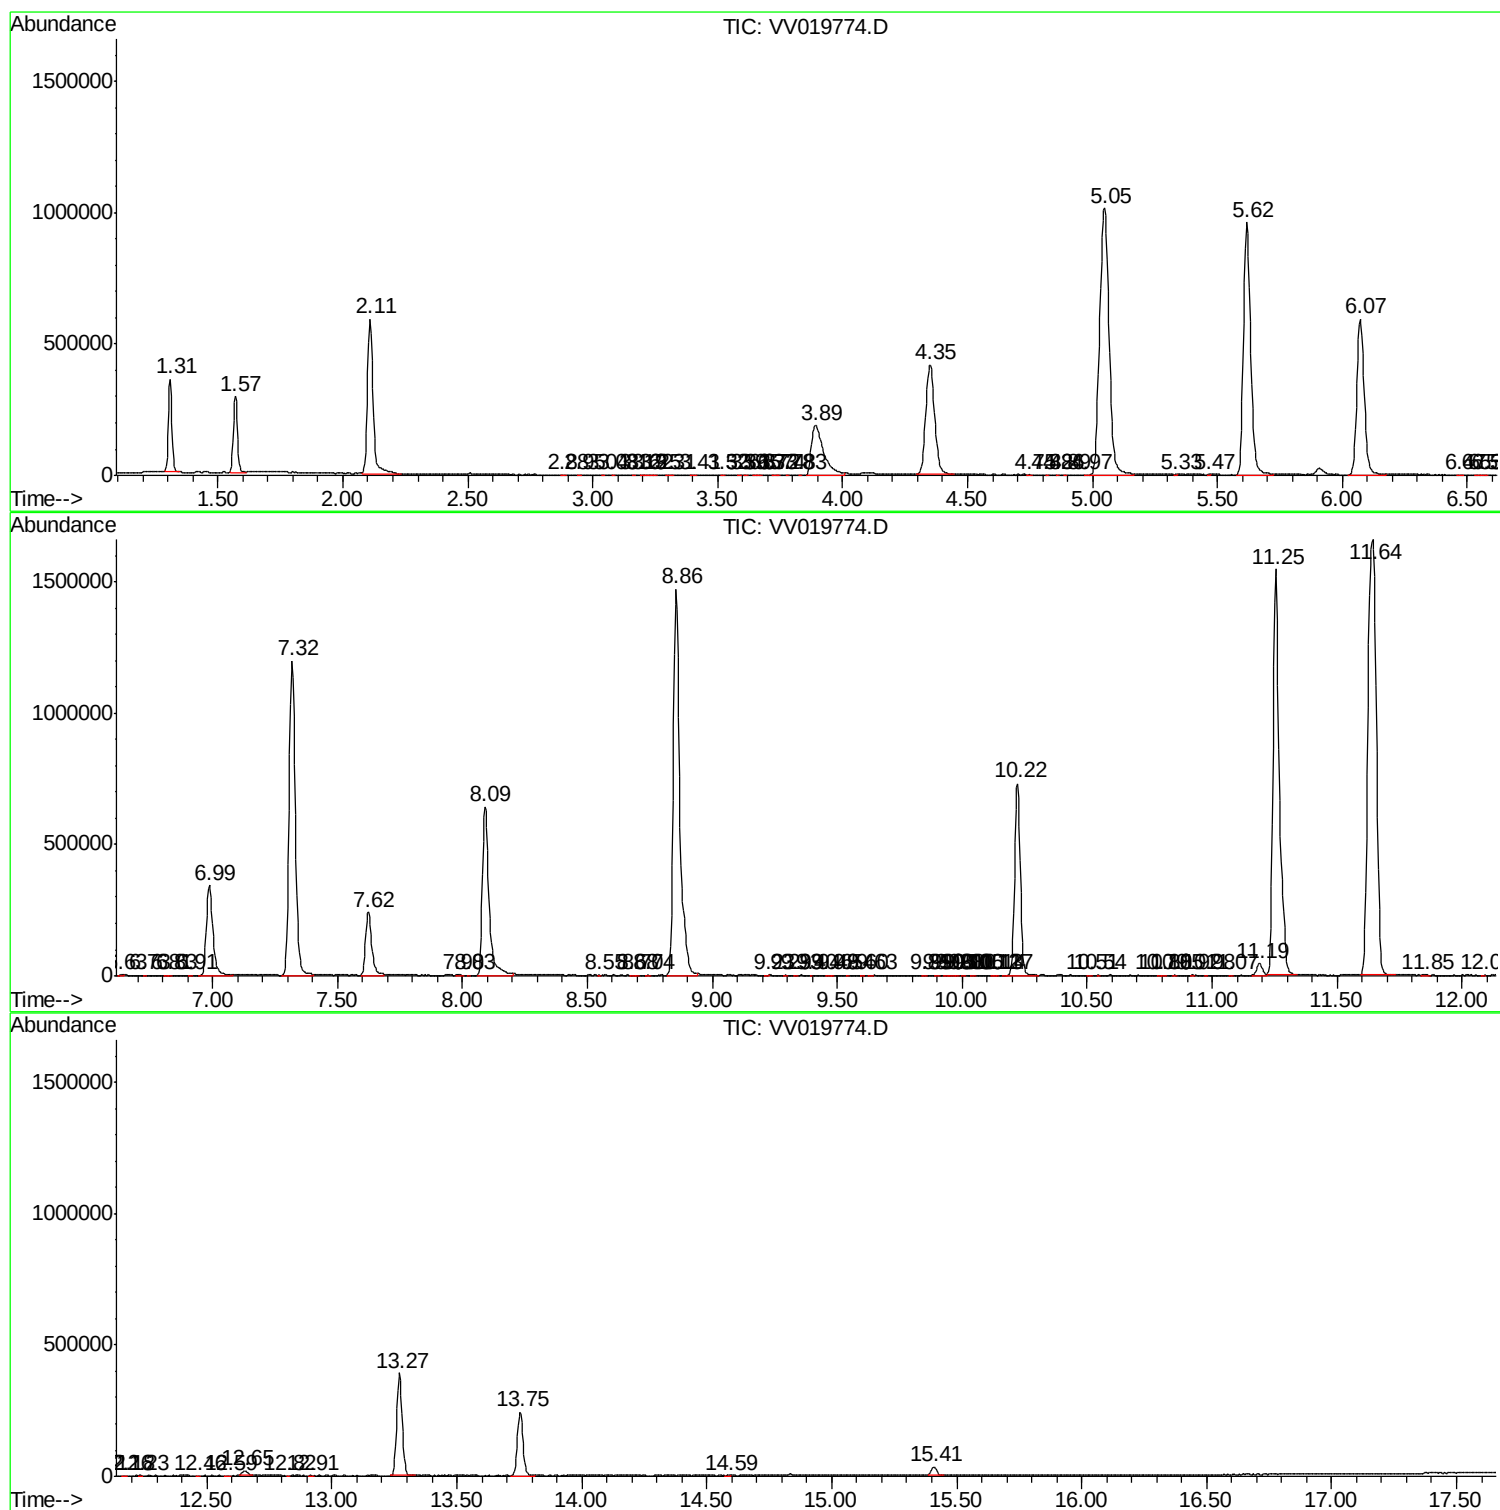

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
Data File : VV019774.D
Acq On : 21 Dec 2020 14:40
Operator : SY/MD
Sample : L5101-01DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FW6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV122120\
Data File : VV019774.D
Acq On : 21 Dec 2020 14:40
Operator : SY/MD
Sample : L5101-01DL 4X
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
C0FW6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
