

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
 Data File : VV019776.D
 Acq On : 21 Dec 2020 15:28
 Operator : SY/MD
 Sample : L5087-06 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Q1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	86	rVB	458025	454353	15.80%	2.134%
2	1.569	142	149	162	rVB	341923	385033	13.39%	1.809%
3	2.110	307	317	358	rVB	703336	1097954	38.19%	5.158%
4	3.110	625	628	629	rBV3	659	314	0.01%	0.001%
5	3.155	639	642	644	rBV2	811	394	0.01%	0.002%
6	3.174	645	648	650	rVV2	800	384	0.01%	0.002%
7	3.235	664	667	669	rBV3	619	445	0.02%	0.002%
8	3.341	698	700	702	rVB2	652	214	0.01%	0.001%
9	3.383	711	713	715	rBV3	485	240	0.01%	0.001%
10	3.412	718	722	723	rBV3	691	427	0.01%	0.002%
11	3.450	731	734	735	rBV3	843	529	0.02%	0.002%
12	3.489	742	746	750	rBV3	859	698	0.02%	0.003%
13	3.527	756	758	760	rBV2	243	102	0.00%	0.000%
14	3.553	764	766	768	rBV2	434	263	0.01%	0.001%
15	3.611	782	784	789	rVB2	607	450	0.02%	0.002%
16	3.646	789	795	797	rBV5	642	507	0.02%	0.002%
17	3.663	797	800	801	rVV	612	289	0.01%	0.001%
18	3.685	805	807	811	rBV3	433	322	0.01%	0.002%
19	3.701	811	812	813	rBV	434	122	0.00%	0.001%
20	3.756	826	829	832	rBV4	608	489	0.02%	0.002%
21	3.769	832	833	836	rVV2	528	207	0.01%	0.001%
22	3.785	836	838	841	rVV2	626	347	0.01%	0.002%
23	3.817	846	848	852	rBV3	553	387	0.01%	0.002%
24	3.897	859	873	915	rBV	201045	664408	23.11%	3.121%
25	4.354	998	1015	1045	rBV	452441	1111367	38.66%	5.221%
26	4.865	1172	1174	1179	rBV3	950	973	0.03%	0.005%
27	4.913	1187	1189	1193	rBV3	830	498	0.02%	0.002%
28	4.936	1193	1196	1199	rVV3	469	355	0.01%	0.002%
29	5.052	1214	1232	1275	rBV2	1118204	2874850	100.00%	13.505%
30	5.556	1387	1389	1395	rBV7	699	529	0.02%	0.002%
31	5.621	1396	1409	1440	rBV	795996	1587942	55.24%	7.459%
32	5.910	1489	1499	1519	rBV6	30452	69500	2.42%	0.326%
33	6.074	1537	1550	1580	rBV	636127	1271867	44.24%	5.975%
34	6.412	1650	1655	1656	rBV3	896	753	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
 Data File : VV019776.D
 Acq On : 21 Dec 2020 15:28
 Operator : SY/MD
 Sample : L5087-06 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Q1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	6.476	1673	1675	1676	rBV2	584	213	0.01%	0.001%
36	6.508	1683	1685	1690	rBV4	610	522	0.02%	0.002%
37	6.527	1690	1691	1695	rVV3	686	393	0.01%	0.002%
38	6.553	1697	1699	1700	rBV2	566	223	0.01%	0.001%
39	6.579	1704	1707	1710	rBV4	936	647	0.02%	0.003%
40	6.727	1750	1753	1762	rVB6	1327	1362	0.05%	0.006%
41	6.765	1762	1765	1767	rBV2	458	289	0.01%	0.001%
42	6.791	1771	1773	1774	rBV	921	459	0.02%	0.002%
43	6.823	1780	1783	1788	rVB3	1007	820	0.03%	0.004%
44	6.846	1788	1790	1793	rBV2	661	346	0.01%	0.002%
45	6.862	1793	1795	1798	rVB2	944	400	0.01%	0.002%
46	6.878	1798	1800	1802	rBV3	448	207	0.01%	0.001%
47	6.929	1809	1816	1820	rVB6	994	1208	0.04%	0.006%
48	6.945	1820	1821	1823	rBV2	621	277	0.01%	0.001%
49	6.990	1823	1835	1863	rBV	368335	669430	23.29%	3.145%
50	7.322	1925	1938	1967	rBV	1294391	2254632	78.43%	10.591%
51	7.624	2022	2032	2054	rBV	249796	441169	15.35%	2.072%
52	7.862	2103	2106	2108	rBV3	1344	950	0.03%	0.004%
53	7.945	2130	2132	2134	rVB2	1042	391	0.01%	0.002%
54	7.981	2134	2143	2155	rVB6	15213	27246	0.95%	0.128%
55	8.093	2166	2178	2209	rBV	708969	1316315	45.79%	6.183%
56	8.508	2305	2307	2308	rBV2	934	334	0.01%	0.002%
57	8.855	2403	2415	2443	rBV	1181317	1932123	67.21%	9.076%
58	9.145	2503	2505	2509	rVB4	1084	573	0.02%	0.003%
59	9.305	2554	2555	2557	rBV	577	223	0.01%	0.001%
60	9.350	2565	2569	2572	rBV4	709	658	0.02%	0.003%
61	9.450	2596	2600	2603	rBV3	849	806	0.03%	0.004%
62	9.611	2646	2650	2653	rBV4	955	727	0.03%	0.003%
63	9.752	2691	2694	2697	rBV2	1005	694	0.02%	0.003%
64	9.820	2712	2715	2717	rBV3	687	450	0.02%	0.002%
65	9.858	2725	2727	2729	rBV3	731	361	0.01%	0.002%
66	9.923	2742	2747	2748	rBV2	840	675	0.02%	0.003%
67	9.958	2756	2758	2762	rVB3	712	293	0.01%	0.001%
68	10.093	2799	2800	2802	rVB3	413	126	0.00%	0.001%
69	10.109	2802	2805	2809	rBV6	1042	975	0.03%	0.005%
70	10.151	2816	2818	2819	rVB	620	226	0.01%	0.001%
71	10.222	2828	2840	2865	rBV	777711	1221787	42.50%	5.739%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
 Data File : VV019776.D
 Acq On : 21 Dec 2020 15:28
 Operator : SY/MD
 Sample : L5087-06 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG4Q1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.550	2939	2942	2943	rBV4	761	368	0.01%	0.002%
73	10.685	2980	2984	2987	rBV4	730	532	0.02%	0.002%
74	10.701	2987	2989	2990	rBV2	464	150	0.01%	0.001%
75	10.772	3009	3011	3013	rVB3	697	274	0.01%	0.001%
76	10.923	3056	3058	3060	rBV2	744	490	0.02%	0.002%
77	11.006	3082	3084	3086	rVB3	921	444	0.02%	0.002%
78	11.019	3086	3088	3091	rBV2	585	408	0.01%	0.002%
79	11.035	3091	3093	3095	rBV2	397	195	0.01%	0.001%
80	11.170	3132	3135	3137	rBV3	1036	666	0.02%	0.003%
81	11.254	3149	3161	3187	rBV	1223718	1906199	66.31%	8.954%
82	11.630	3266	3278	3300	rBV	1277454	1969844	68.52%	9.253%
83	11.984	3384	3388	3390	rBV4	913	697	0.02%	0.003%
84	12.218	3459	3461	3464	rBV2	666	482	0.02%	0.002%
85	12.444	3527	3531	3533	rBV2	790	611	0.02%	0.003%
86	12.897	3669	3672	3674	rBV2	470	328	0.01%	0.002%
87	12.929	3680	3682	3684	rBV2	771	300	0.01%	0.001%


Sum of corrected areas: 21288030

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
Data File : VV019776.D
Acq On : 21 Dec 2020 15:28
Operator : SY/MD
Sample : L5087-06 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Q1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

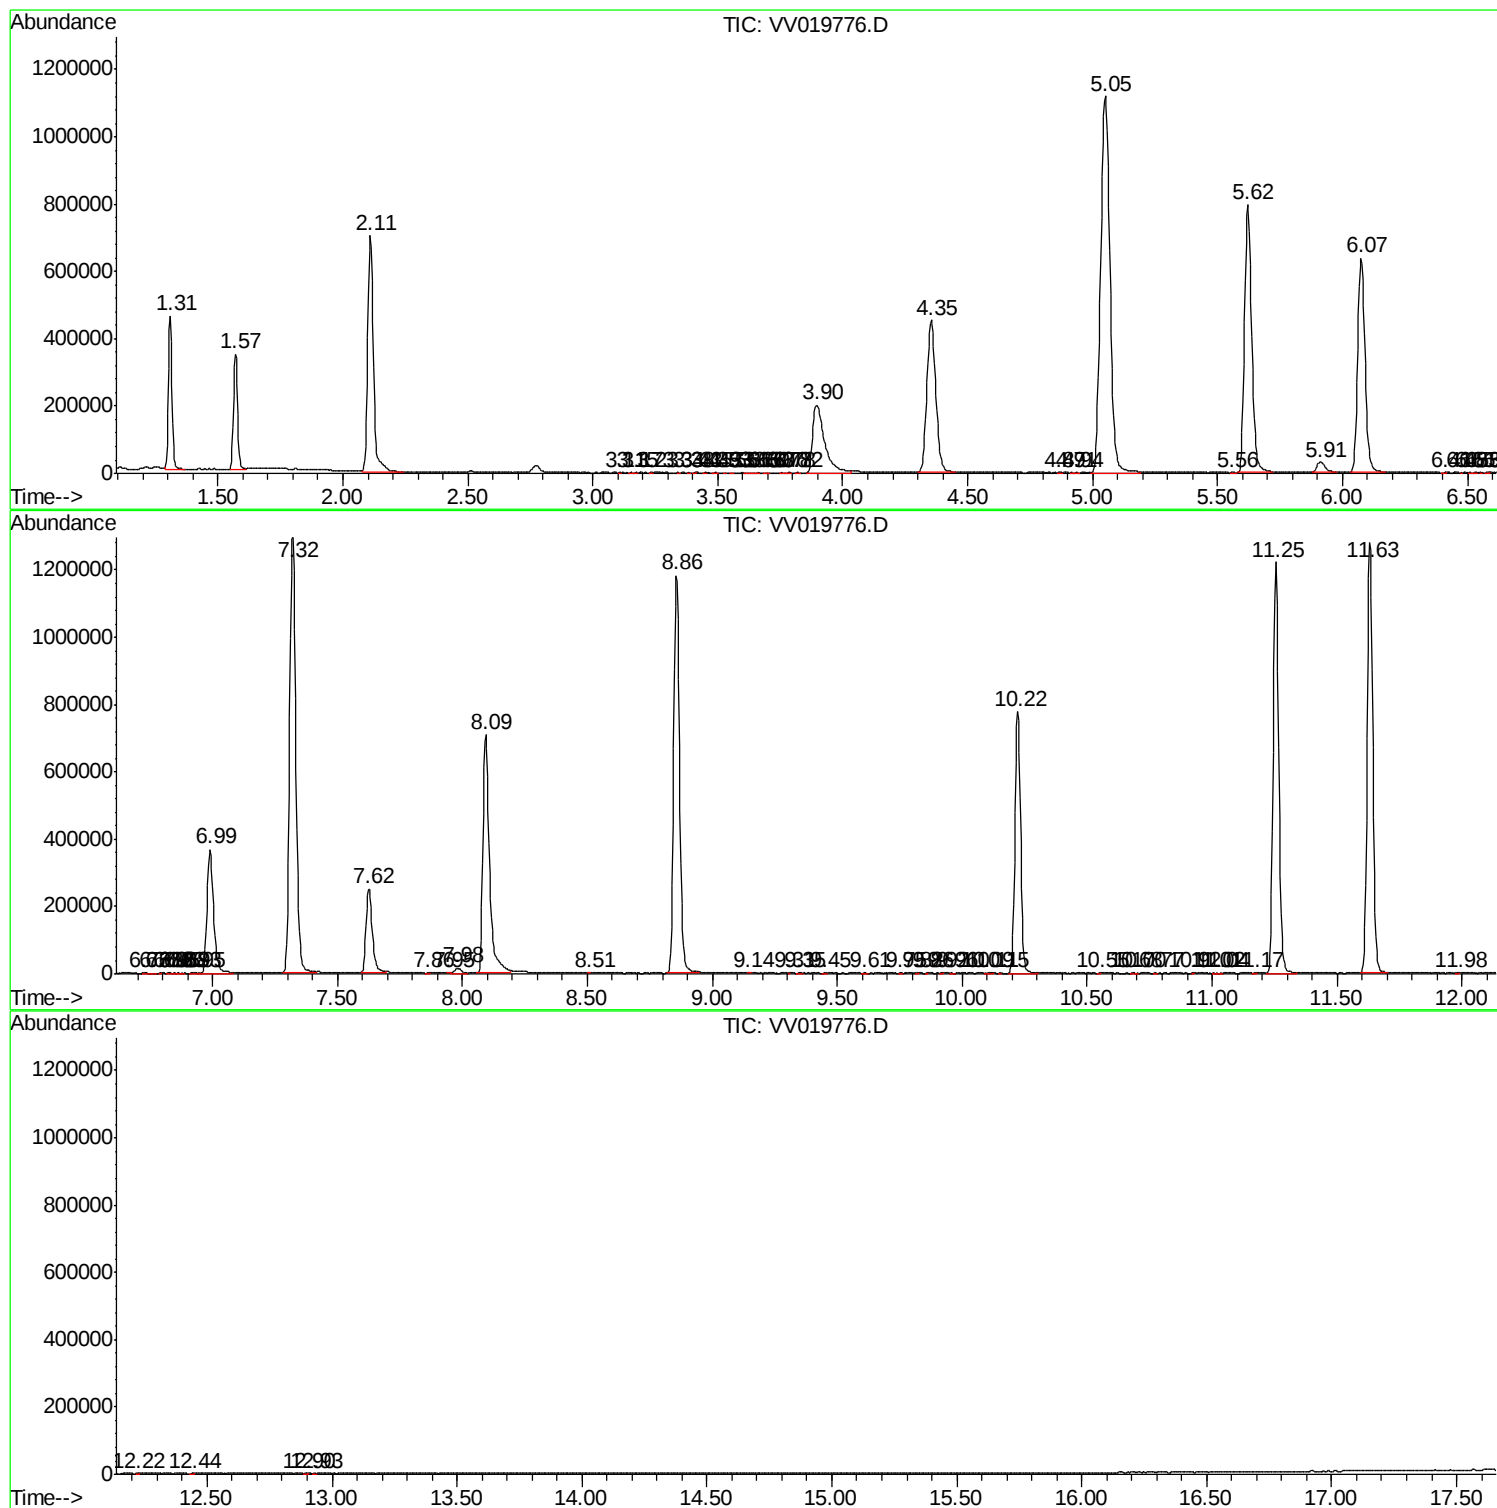

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
Data File : VV019776.D
Acq On : 21 Dec 2020 15:28
Operator : SY/MD
Sample : L5087-06 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Q1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
Data File : VV019776.D
Acq On : 21 Dec 2020 15:28
Operator : SY/MD
Sample : L5087-06 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG4Q1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc