

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
 Data File : VV019785.D
 Acq On : 21 Dec 2020 19:05
 Operator : SY/MD
 Sample : L5087-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.309	62	68	83	rVB	316583	312986	13.02%	1.614%
2	1.569	142	149	162	rVB	263579	297341	12.36%	1.533%
3	2.110	308	317	351	rVB	529621	826736	34.38%	4.263%
4	2.949	575	578	580	rBV3	853	532	0.02%	0.003%
5	3.013	596	598	600	rBV2	452	189	0.01%	0.001%
6	3.084	617	620	623	rBV3	431	388	0.02%	0.002%
7	3.116	628	630	633	rVV3	677	449	0.02%	0.002%
8	3.135	633	636	640	rVB4	1209	905	0.04%	0.005%
9	3.161	643	644	645	rBV	394	126	0.01%	0.001%
10	3.187	649	652	654	rBV3	786	553	0.02%	0.003%
11	3.216	659	661	663	rBV2	550	324	0.01%	0.002%
12	3.267	674	677	679	rBV3	604	330	0.01%	0.002%
13	3.299	685	687	691	rVB3	950	554	0.02%	0.003%
14	3.319	691	693	696	rBV	789	571	0.02%	0.003%
15	3.335	696	698	702	rVB3	899	502	0.02%	0.003%
16	3.418	723	724	726	rBV2	608	270	0.01%	0.001%
17	3.505	750	751	752	rVB	333	64	0.00%	0.000%
18	3.515	752	754	755	rBV	229	99	0.00%	0.001%
19	3.531	756	759	761	rVV3	898	473	0.02%	0.002%
20	3.566	767	770	775	rBV3	714	406	0.02%	0.002%
21	3.589	775	777	778	rBV	779	341	0.01%	0.002%
22	3.653	795	797	799	rVB3	881	298	0.01%	0.002%
23	3.666	799	801	803	rBV	391	145	0.01%	0.001%
24	3.682	803	806	808	rVV3	546	370	0.02%	0.002%
25	3.794	839	841	842	rBV3	470	249	0.01%	0.001%
26	3.833	849	853	856	rVB4	450	333	0.01%	0.002%
27	3.849	856	858	860	rBV2	558	324	0.01%	0.002%
28	3.897	861	873	914	rBV	179386	571895	23.78%	2.949%
29	4.354	997	1015	1043	rBV	390588	955322	39.73%	4.926%
30	4.759	1139	1141	1144	rBV2	931	533	0.02%	0.003%
31	4.775	1144	1146	1147	rBV	458	151	0.01%	0.001%
32	4.859	1168	1172	1174	rBV3	1201	790	0.03%	0.004%
33	4.974	1204	1208	1210	rVB5	735	418	0.02%	0.002%
34	4.987	1210	1212	1214	rVB	688	260	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
 Data File : VV019785.D
 Acq On : 21 Dec 2020 19:05
 Operator : SY/MD
 Sample : L5087-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

35	5.052	1214	1232	1259	rBV2	928075	2404786	100.00%	12.401%
36	5.473	1360	1363	1365	rBV3	1207	830	0.03%	0.004%
37	5.621	1396	1409	1447	rBV	895149	1790603	74.46%	9.233%
38	5.910	1490	1499	1515	rBV	26902	54916	2.28%	0.283%
39	6.074	1536	1550	1580	rBV	543312	1109314	46.13%	5.720%
40	6.380	1643	1645	1646	rBV2	566	157	0.01%	0.001%
41	6.463	1668	1671	1672	rBV3	620	367	0.02%	0.002%
42	6.489	1677	1679	1681	rBV3	485	184	0.01%	0.001%
43	6.614	1714	1718	1721	rBV4	828	704	0.03%	0.004%
44	6.759	1760	1763	1764	rBV3	770	461	0.02%	0.002%
45	6.810	1777	1779	1781	rBV2	511	168	0.01%	0.001%
46	6.881	1797	1801	1803	rBV3	472	374	0.02%	0.002%
47	6.891	1803	1804	1805	rBV	363	100	0.00%	0.001%
48	6.923	1810	1814	1817	rBV5	1001	802	0.03%	0.004%
49	6.990	1822	1835	1863	rBV	307914	561590	23.35%	2.896%
50	7.322	1925	1938	1964	rBV	1072803	1867351	77.65%	9.629%
51	7.627	2020	2033	2056	rBV	208813	375978	15.63%	1.939%
52	7.987	2137	2145	2154	rVB7	5904	8601	0.36%	0.044%
53	8.093	2166	2178	2213	rBV	640980	1204528	50.09%	6.211%
54	8.772	2383	2389	2390	rBV4	883	851	0.04%	0.004%
55	8.859	2404	2416	2444	rBV	1317282	2162998	89.95%	11.154%
56	9.379	2575	2578	2582	rBV2	1246	820	0.03%	0.004%
57	9.460	2601	2603	2605	rBV2	489	277	0.01%	0.001%
58	9.566	2630	2636	2642	rBV5	1358	1671	0.07%	0.009%
59	9.698	2673	2677	2679	rBV2	404	299	0.01%	0.002%
60	9.733	2686	2688	2690	rBV2	733	400	0.02%	0.002%
61	9.794	2705	2707	2708	rBV2	478	168	0.01%	0.001%
62	9.804	2708	2710	2714	rVB3	523	312	0.01%	0.002%
63	9.823	2714	2716	2724	rBV6	805	1027	0.04%	0.005%
64	9.897	2737	2739	2742	rBV3	618	362	0.02%	0.002%
65	9.916	2743	2745	2747	rVV3	868	472	0.02%	0.002%
66	9.942	2750	2753	2756	rBV4	553	325	0.01%	0.002%
67	9.997	2768	2770	2771	rBV2	588	143	0.01%	0.001%
68	10.090	2796	2799	2800	rBV	797	400	0.02%	0.002%
69	10.122	2807	2809	2814	rVB3	965	558	0.02%	0.003%
70	10.222	2828	2840	2858	rBV	688384	1085143	45.12%	5.596%
71	10.450	2909	2911	2913	rBV	683	301	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
 Data File : VV019785.D
 Acq On : 21 Dec 2020 19:05
 Operator : SY/MD
 Sample : L5087-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis

72	10.621	2962	2964	2967	rVB2	594	327	0.01%	0.002%
73	10.675	2979	2981	2984	rBV2	636	284	0.01%	0.001%
74	10.714	2989	2993	2996	rBV4	804	560	0.02%	0.003%
75	10.733	2997	2999	3000	rBV2	412	164	0.01%	0.001%
76	10.846	3031	3034	3036	rBV2	1037	385	0.02%	0.002%
77	10.858	3036	3038	3040	rBV3	762	449	0.02%	0.002%
78	10.965	3066	3071	3072	rBV2	899	679	0.03%	0.004%
79	11.100	3107	3113	3118	rBV5	821	683	0.03%	0.004%
80	11.148	3126	3128	3129	rBV2	794	351	0.01%	0.002%
81	11.167	3132	3134	3136	rVV2	992	433	0.02%	0.002%
82	11.257	3150	3162	3182	rBV	1339153	2060051	85.66%	10.623%
83	11.633	3267	3279	3303	rBV	1090586	1711360	71.16%	8.825%
84	11.961	3378	3381	3383	rBV3	1393	878	0.04%	0.005%
85	12.302	3485	3487	3489	rBV2	472	141	0.01%	0.001%
86	12.318	3489	3492	3495	rBV2	853	529	0.02%	0.003%
87	13.180	3757	3760	3767	rVB6	1326	1273	0.05%	0.007%
88	13.903	3983	3985	3987	rBV3	936	518	0.02%	0.003%


Sum of corrected areas: 19392633

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
Data File : VV019785.D
Acq On : 21 Dec 2020 19:05
Operator : SY/MD
Sample : L5087-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

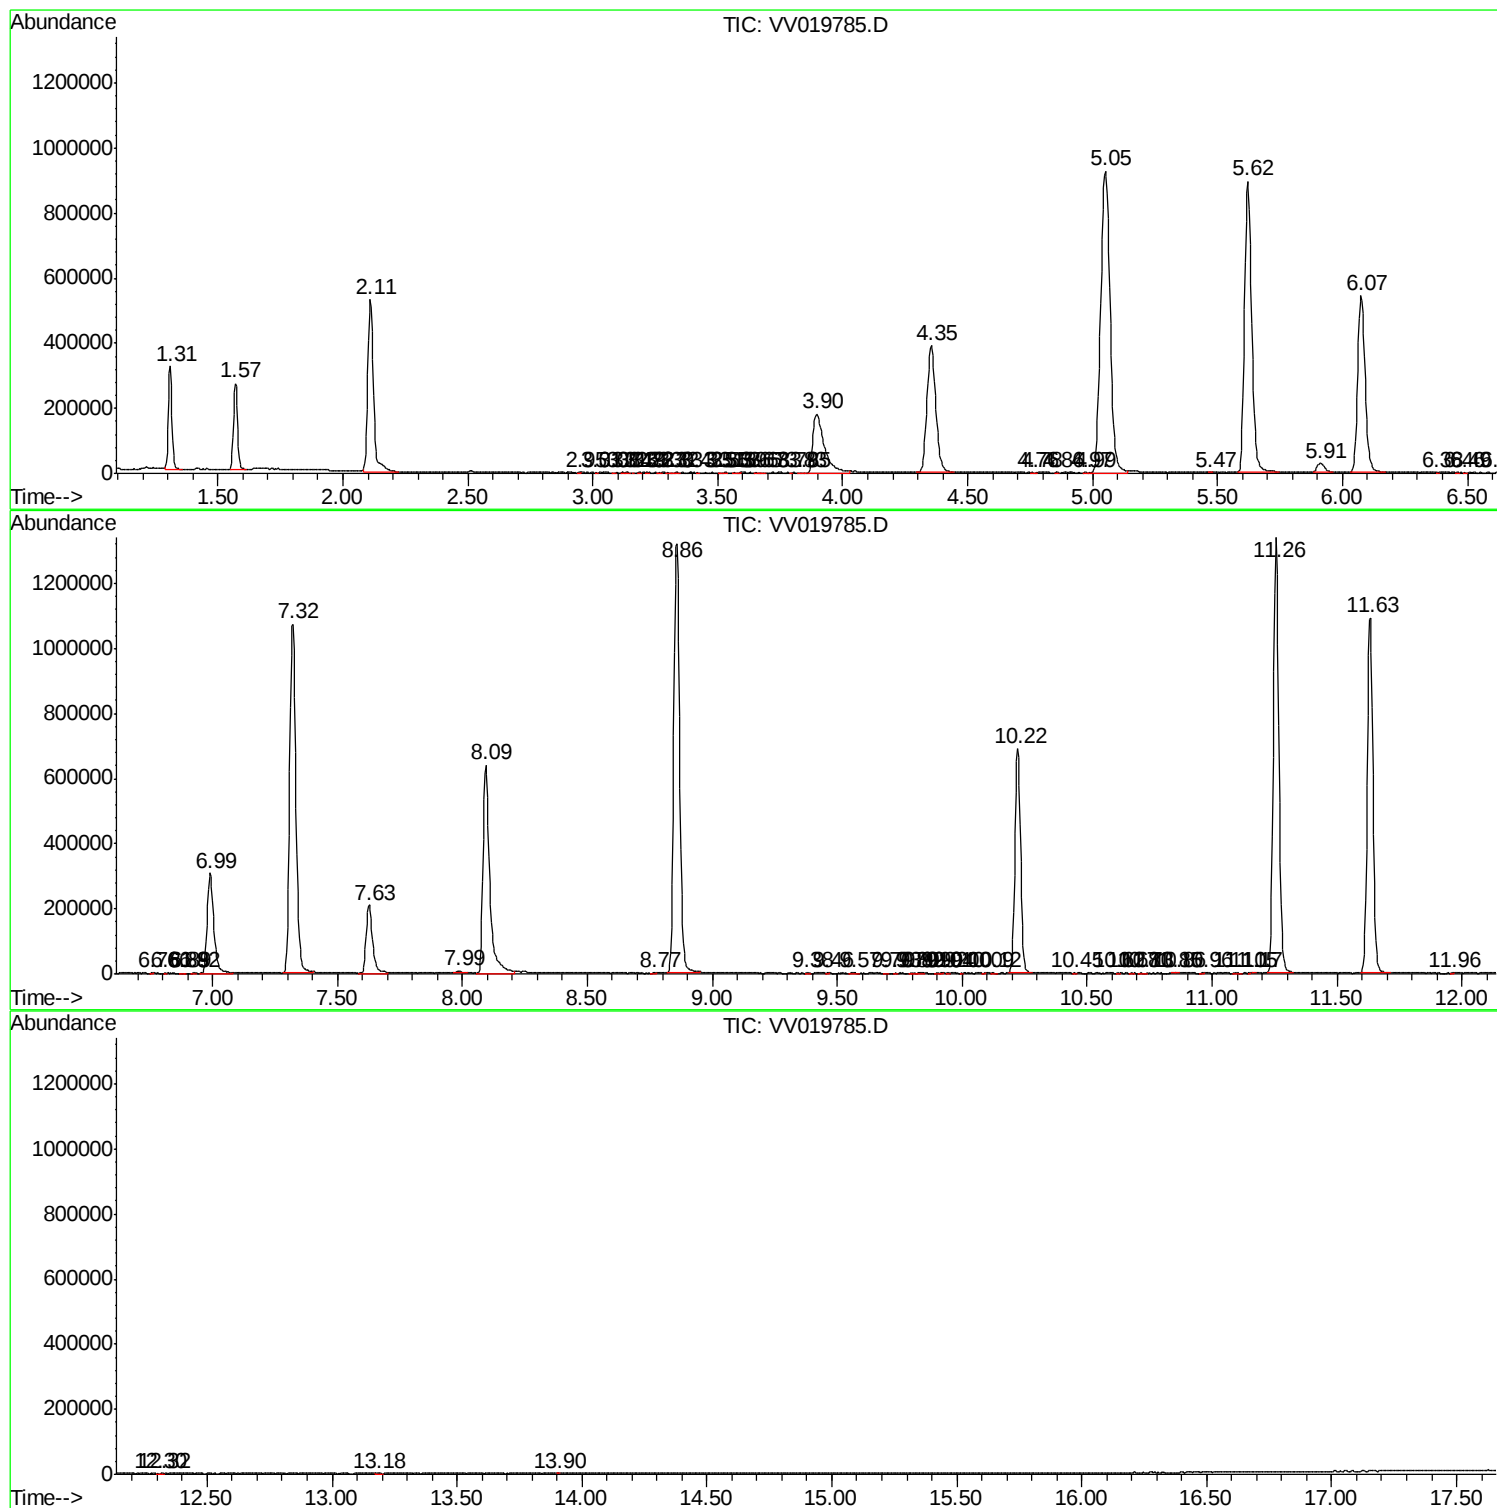

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
Data File : VV019785.D
Acq On : 21 Dec 2020 19:05
Operator : SY/MD
Sample : L5087-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV122120\
Data File : VV019785.D
Acq On : 21 Dec 2020 19:05
Operator : SY/MD
Sample : L5087-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc