


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV122120\
 Data File : VV019766.D
 Acq On : 21 Dec 2020 09:23
 Operator : SY/MD
 Sample : BFB70
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB70

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM121020WMA.M
 Title : VOC Analysis
 Last Update : Tue Dec 22 00:24:34 2020

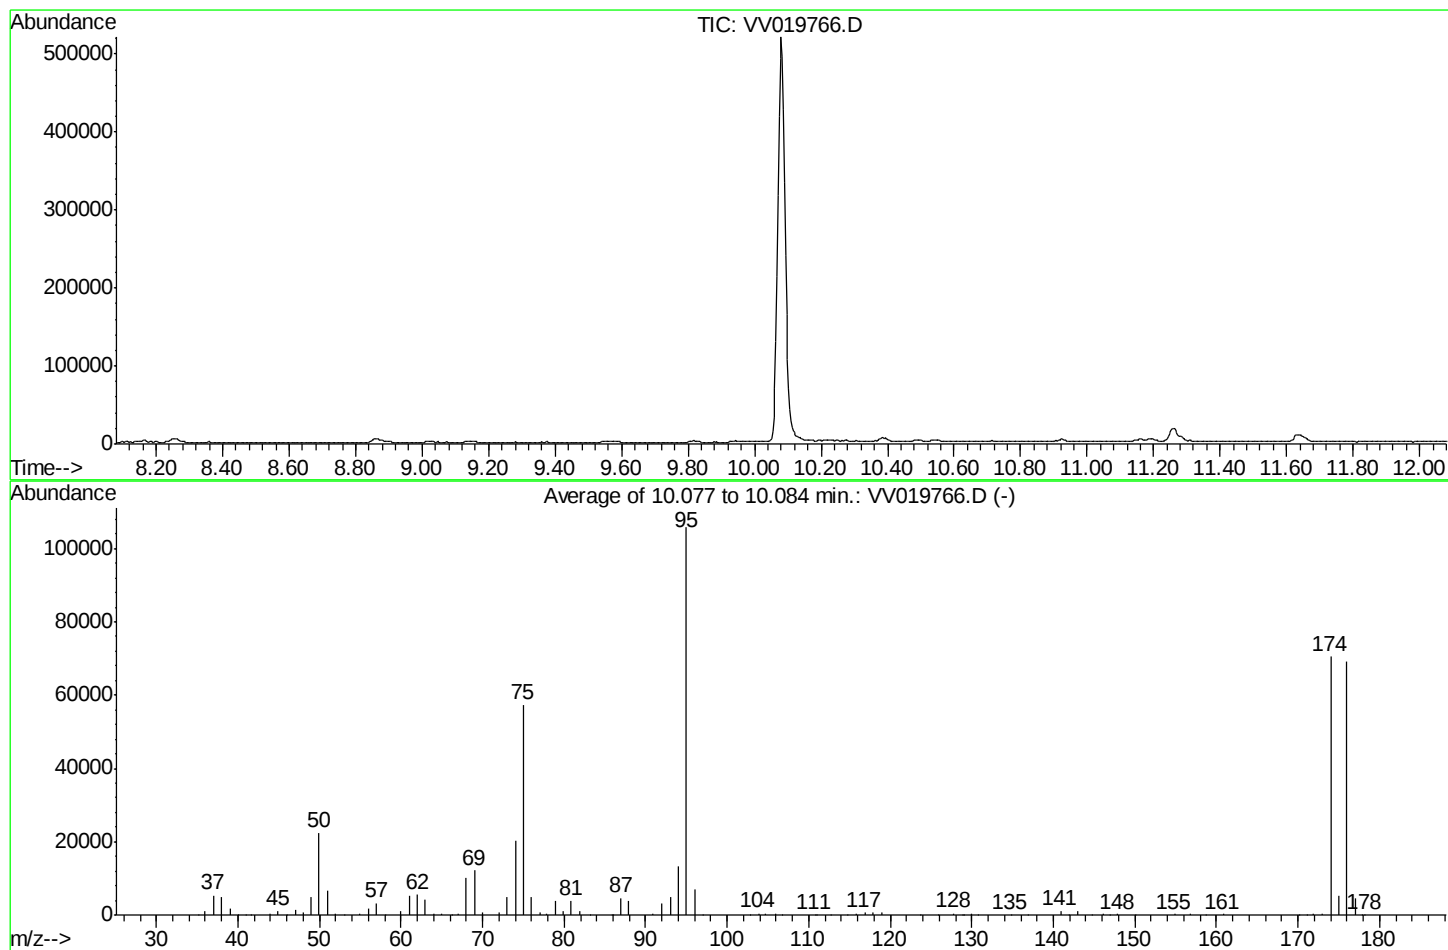

AutoFind: Scans 2795, 2796, 2797; Background Corrected with Scan 2784

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	22523	PASS
75	95	30	80	54.3	57421	PASS
95	95	100	100	100.0	105797	PASS
96	95	5	9	6.7	7054	PASS
173	174	0.00	2	0.5	328	PASS
174	95	50	120	66.7	70528	PASS
175	174	5	9	7.5	5302	PASS
176	174	95	101	97.9	69074	PASS
177	176	5	9	6.4	4419	PASS

m/z	Abundance
36.00	822.0
36.90	156.0
38.00	290.0
39.00	141.0
39.90	370.0
40.90	131.0
43.00	122.0
43.90	897.0
45.20	124.0
49.80	103.0
62.20	106.0
67.80	107.0
102.80	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
36.00	1900.0
37.00	5694.0
38.00	4997.0
39.00	1939.0
40.00	556.0
41.00	194.0
41.50	146.0
43.00	154.0
44.00	1344.0
44.90	1197.0
46.20	178.0
47.10	1408.0
48.00	844.0
49.00	4840.0
50.00	22768.0
51.00	6806.0
52.00	404.0
53.00	128.0
54.90	369.0
56.00	1893.0
57.00	3030.0
58.10	120.0
60.00	916.0
61.00	5319.0
62.00	5568.0
63.00	4222.0
64.00	490.0
64.90	301.0
67.10	298.0
68.00	10552.0
69.00	12014.0
70.00	777.0
72.00	657.0
73.00	5035.0
74.00	19920.0
75.00	56856.0
76.00	5379.0
77.00	676.0
77.90	411.0
78.90	3933.0
79.90	1183.0
80.90	3845.0
81.90	884.0
86.00	163.0
87.00	4628.0
87.90	3763.0
90.90	368.0
92.00	3134.0
93.00	5226.0
94.00	12817.0
95.00	103456.0
96.00	6726.0
97.00	202.0
102.90	154.0
103.90	519.0
104.70	238.0
105.80	429.0
110.80	126.0
112.80	121.0
114.90	135.0
115.90	459.0
116.90	706.0
117.90	464.0
118.90	500.0
125.90	113.0
127.80	471.0
128.80	151.0
129.90	310.0
134.70	186.0
136.90	182.0
140.90	973.0
141.90	131.0
143.00	920.0
144.90	135.0
146.10	224.0
146.90	121.0
147.90	294.0
150.00	113.0
154.90	252.0
156.80	181.0
158.70	162.0
160.80	164.0
170.20	127.0
171.10	121.0
171.80	325.0
173.00	985.0
174.00	67600.0
175.00	5268.0
176.00	65592.0
177.00	4421.0
177.90	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

178.20

129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

m/z	Abundance
35.10	273.0
36.00	1826.0
37.00	5781.0
38.00	5313.0
39.00	2119.0
40.00	536.0
41.00	153.0
41.60	122.0
43.00	120.0
44.00	1415.0
44.90	1219.0
46.00	176.0
47.10	1452.0
48.00	786.0
49.00	4982.0
50.00	23528.0
51.00	6862.0
52.00	452.0
53.00	119.0
54.90	319.0
56.00	2039.0
57.00	3276.0
58.10	108.0
60.00	992.0
61.00	5387.0
62.00	5786.0
63.00	4361.0
64.00	511.0
64.90	296.0
66.30	125.0
67.00	241.0
68.00	10788.0
69.00	12531.0
70.00	870.0
72.10	687.0
73.00	5227.0
74.00	20880.0
75.00	59384.0
76.00	5240.0
77.00	668.0
77.90	423.0
78.90	3988.0
79.90	1275.0
80.90	4096.0
82.00	1000.0
83.10	136.0
86.10	171.0
87.00	4863.0
87.90	4105.0
90.90	457.0
92.00	3320.0
93.00	5221.0
94.00	13695.0
95.00	109840.0
96.00	7254.0
96.90	190.0
102.90	154.0
103.90	494.0
104.80	264.0
105.90	465.0
106.70	112.0
110.70	136.0
112.70	122.0
114.80	136.0
115.90	439.0
116.90	697.0
117.90	550.0
118.90	589.0
123.70	116.0
125.90	113.0
127.80	551.0
129.00	181.0
129.90	341.0
134.80	166.0
136.80	182.0
140.90	1148.0
143.00	1080.0
144.70	163.0
146.10	197.0
146.80	150.0
147.90	265.0
150.00	102.0
154.80	247.0
156.90	223.0
158.70	131.0
160.90	197.0
170.20	112.0
171.10	119.0
171.80	402.0
174.00	72752.0
175.00	5476.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70

176.00

177.00

177.90

71576.0

4518.0

151.0

Instrument :

MSVOA_V

ClientSampleId :

BFB70

m/z	Abundance
36.00	1798.0
37.00	5222.0
38.00	5102.0
39.00	2118.0
40.00	466.0
40.90	109.0
44.00	1433.0
44.90	1067.0
45.90	198.0
47.00	1295.0
48.00	705.0
49.00	4710.0
50.00	21584.0
51.00	6260.0
52.00	467.0
55.00	302.0
56.00	1867.0
57.00	3163.0
60.00	984.0
61.00	4820.0
62.00	5440.0
63.00	4223.0
64.00	476.0
65.00	309.0
66.90	189.0
68.00	9869.0
69.00	11798.0
70.00	894.0
72.00	641.0
73.00	4968.0
74.00	19744.0
75.00	56024.0
76.00	4570.0
77.00	641.0
77.80	362.0
78.90	3695.0
79.90	1171.0
80.90	3991.0
82.00	1003.0
83.10	204.0
85.80	130.0
86.10	147.0
86.90	4410.0
87.90	4085.0
90.90	485.0
92.00	3135.0
93.00	4671.0
94.00	13316.0
95.00	104096.0
96.00	7184.0
96.90	161.0
102.80	110.0
103.90	494.0
104.80	258.0
106.00	493.0
106.60	127.0
111.00	156.0
112.80	104.0
114.70	117.0
115.90	383.0
116.90	656.0
117.90	611.0
119.00	628.0
123.70	128.0
127.80	513.0
129.00	202.0
129.90	381.0
130.80	118.0
134.90	168.0
136.80	190.0
140.90	1219.0
143.00	1160.0
144.70	176.0
145.90	144.0
146.80	148.0
147.90	222.0
154.80	240.0
156.90	217.0
158.70	112.0
160.80	207.0
171.20	111.0
171.90	411.0
174.00	71232.0
175.00	5163.0
176.00	70056.0
177.00	4320.0
177.80	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB70