
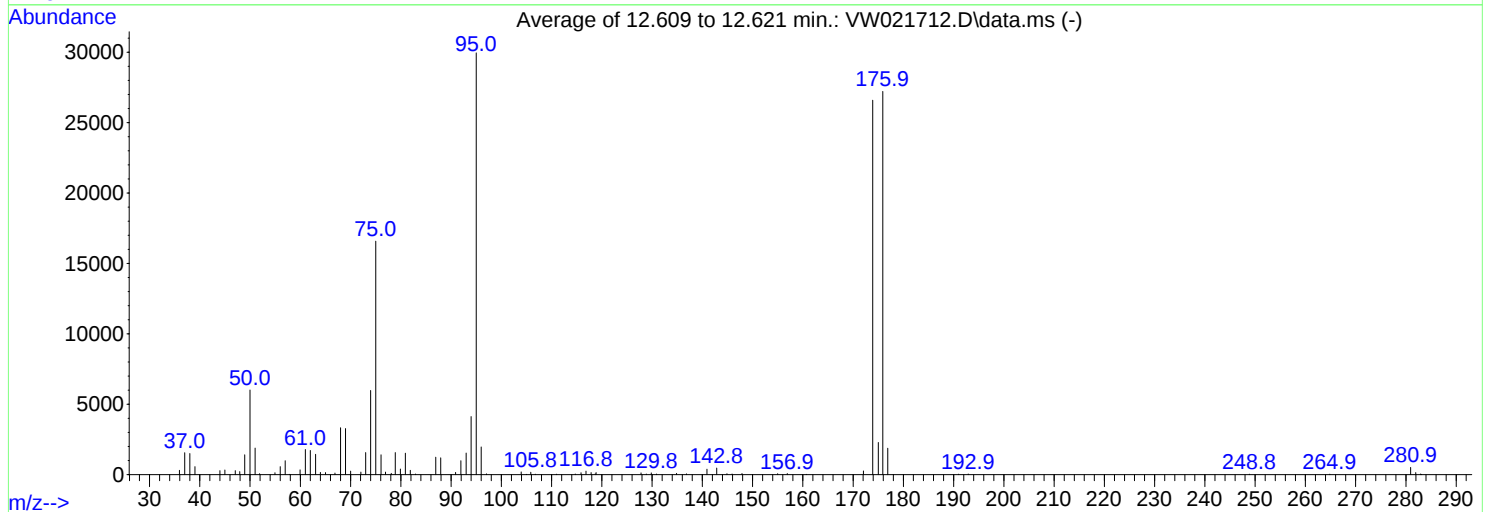


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010322\
 Data File : VW021712.D
 Acq On : 03 Jan 2022 09:29
 Operator : SY/VA
 Sample : BFB493
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB493

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Title : SFAM01.0
 Last Update : Tue Jan 04 00:22:49 2022

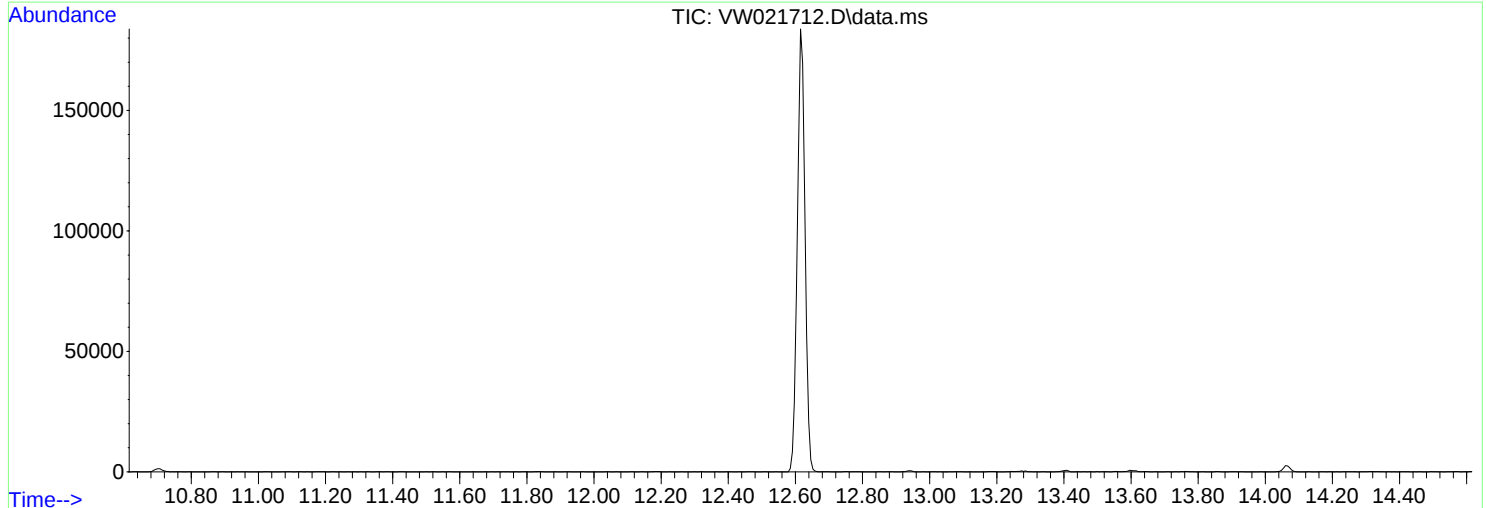

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	6008	PASS
75	95	30	80	55.3	16576	PASS
95	95	100	100	100.0	29957	PASS
96	95	5	9	6.5	1961	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.8	26589	PASS
175	174	5	9	8.6	2281	PASS
176	174	95	105	102.4	27221	PASS
177	176	5	10	6.9	1877	PASS

m/z

Abundance

Instrument :
MSVOA_W
ClientSampleId :
BFB493

m/z	Abundance
36.00	323.0
37.00	1497.0
38.00	1391.0
39.10	556.0
44.00	212.0
45.00	294.0
47.10	264.0
48.00	207.0
48.90	1347.0
50.00	5153.0
51.00	1722.0
51.90	54.0
55.00	111.0
56.00	501.0
57.00	865.0
60.00	320.0
61.00	1602.0
62.00	1537.0
63.00	1285.0
64.00	182.0
65.00	145.0
66.90	74.0
68.00	2872.0
69.00	2733.0
70.00	230.0
72.10	148.0
73.00	1386.0
74.00	5033.0
75.00	14113.0
76.00	1378.0
77.00	179.0
78.10	74.0
78.90	1368.0
79.90	340.0
80.90	1291.0
81.90	303.0
83.00	56.0
86.90	1039.0
88.00	1064.0
90.90	164.0
92.00	715.0
93.00	1192.0
94.00	3442.0
95.00	25248.0
96.00	1599.0
103.90	144.0
105.90	144.0
106.70	51.0
115.80	67.0
116.90	177.0
117.90	147.0
118.70	168.0
128.00	88.0
129.80	100.0
134.90	82.0
140.90	355.0
142.80	340.0
144.90	51.0
147.90	65.0
156.90	59.0
172.00	283.0
173.90	20144.0
175.00	1773.0
175.90	19408.0
176.90	1516.0
191.00	95.0
192.90	76.0
248.80	62.0
264.80	70.0
281.00	838.0
281.90	158.0
282.90	130.0

Instrument :
MSVOA_W
ClientSampleId :
BFB493

m/z	Abundance
35.90	298.0
37.00	1722.0
38.00	1601.0
39.00	663.0
44.00	318.0
45.00	350.0
47.00	315.0
47.90	253.0
49.00	1656.0
50.00	7006.0
51.00	2125.0
51.90	70.0
55.00	128.0
56.00	639.0
57.00	1177.0
59.90	387.0
61.00	1981.0
62.00	1987.0
63.10	1522.0
64.00	199.0
65.00	176.0
67.00	151.0
68.00	3688.0
69.00	3876.0
70.00	287.0
72.00	195.0
73.00	1875.0
74.00	6778.0
75.00	18792.0
76.00	1389.0
76.90	223.0
78.20	96.0
78.90	1807.0
79.90	420.0
80.90	1810.0
81.90	312.0
82.90	67.0
87.00	1419.0
87.90	1241.0
90.90	194.0
92.00	1085.0
93.00	1631.0
94.00	4532.0
95.00	32632.0
96.00	2239.0
97.00	98.0
104.00	216.0
105.00	75.0
105.80	158.0
106.80	60.0
111.00	88.0
114.70	88.0
115.90	138.0
116.90	318.0
117.80	151.0
118.90	219.0
127.80	105.0
128.80	94.0
129.90	131.0
130.90	71.0
134.80	104.0
136.80	87.0
141.00	448.0
142.90	548.0
144.90	88.0
145.90	61.0
147.80	67.0
155.00	92.0
156.90	90.0
160.70	55.0
172.10	276.0
173.90	33184.0
175.00	2700.0
175.90	29784.0
176.90	2057.0
178.00	51.0
192.90	78.0
248.90	55.0
264.90	51.0
280.90	356.0
282.00	159.0
283.10	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB493

m/z	Abundance
36.00	315.0
37.00	1446.0
38.00	1512.0
39.00	498.0
44.00	322.0
45.00	332.0
47.00	266.0
47.90	190.0
49.00	1241.0
50.00	5864.0
51.00	1807.0
51.90	79.0
54.90	163.0
56.00	580.0
57.00	935.0
57.90	56.0
60.00	314.0
61.00	1782.0
62.00	1625.0
63.00	1506.0
64.00	115.0
65.00	138.0
66.80	106.0
68.00	3446.0
69.00	3205.0
70.00	234.0
72.10	201.0
73.00	1450.0
74.00	6130.0
75.00	16824.0
76.10	1450.0
77.00	148.0
78.00	103.0
78.90	1523.0
79.90	425.0
80.90	1474.0
81.90	319.0
86.90	1270.0
87.90	1274.0
90.90	122.0
91.90	1159.0
93.00	1797.0
94.00	4408.0
95.00	31992.0
96.00	2045.0
97.10	72.0
103.90	210.0
105.90	200.0
114.70	60.0
115.80	192.0
116.80	268.0
117.90	136.0
118.80	239.0
127.70	169.0
128.90	53.0
129.80	134.0
130.90	63.0
134.90	95.0
136.90	78.0
140.80	372.0
142.90	497.0
144.90	82.0
145.90	79.0
148.00	108.0
155.00	126.0
156.90	75.0
172.10	227.0
173.90	26440.0
175.00	2371.0
175.90	32472.0
176.90	2057.0
281.00	341.0
282.00	136.0

Instrument :
MSVOA_W
ClientSampleId :
BFB493